

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD041219\
 Data File : VD061775.D
 Acq On : 12 Apr 2019 13:45
 Operator : VA/AP
 Sample : K2344-01RE
 Misc : 5.03g/5ml/MSVOA D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 WOOD-1RE

Quant Time: Apr 12 17:03:48 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D040619S.M
 Quant Title : SW846 8260
 QLast Update : Mon Apr 08 10:04:03 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.05	168	188151	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.21	114	297026	50.00	ug/l	0.00
63) Chlorobenzene-d5	12.36	117	227834	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	14.51	152	71619	50.00	ug/l	-0.01
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.45	65	119224	83.60	ug/l	0.00
Spiked Amount 50.000			Recovery	=	167.20%	
35) Dibromofluoromethane	6.92	113	147974	71.91	ug/l	0.00
Spiked Amount 50.000			Recovery	=	143.82%	
50) Toluene-d8	10.40	98	304202	58.84	ug/l	0.00
Spiked Amount 50.000			Recovery	=	117.68%	
62) 4-Bromofluorobenzene	13.54	95	81145	43.44	ug/l	0.00
Spiked Amount 50.000			Recovery	=	86.88%	
Target Compounds						
16) Acetone	3.22	43	18496	43.384	ug/l	98
18) Methyl Acetate	3.64	43	6186	7.712	ug/l #	89
20) Methylene Chloride	3.82	84	47345	19.570	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD041219\
Data File : VD061775.D
Acq On : 12 Apr 2019 13:45
Operator : VA/AP
Sample : K2344-01RE
Misc : 5.03g/5ml/MSVOA D/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
WOOD-1RE

Quant Time: Apr 12 17:03:48 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D040619S.M
Quant Title : SW846 8260
QLast Update : Mon Apr 08 10:04:03 2019
Response via : Initial Calibration




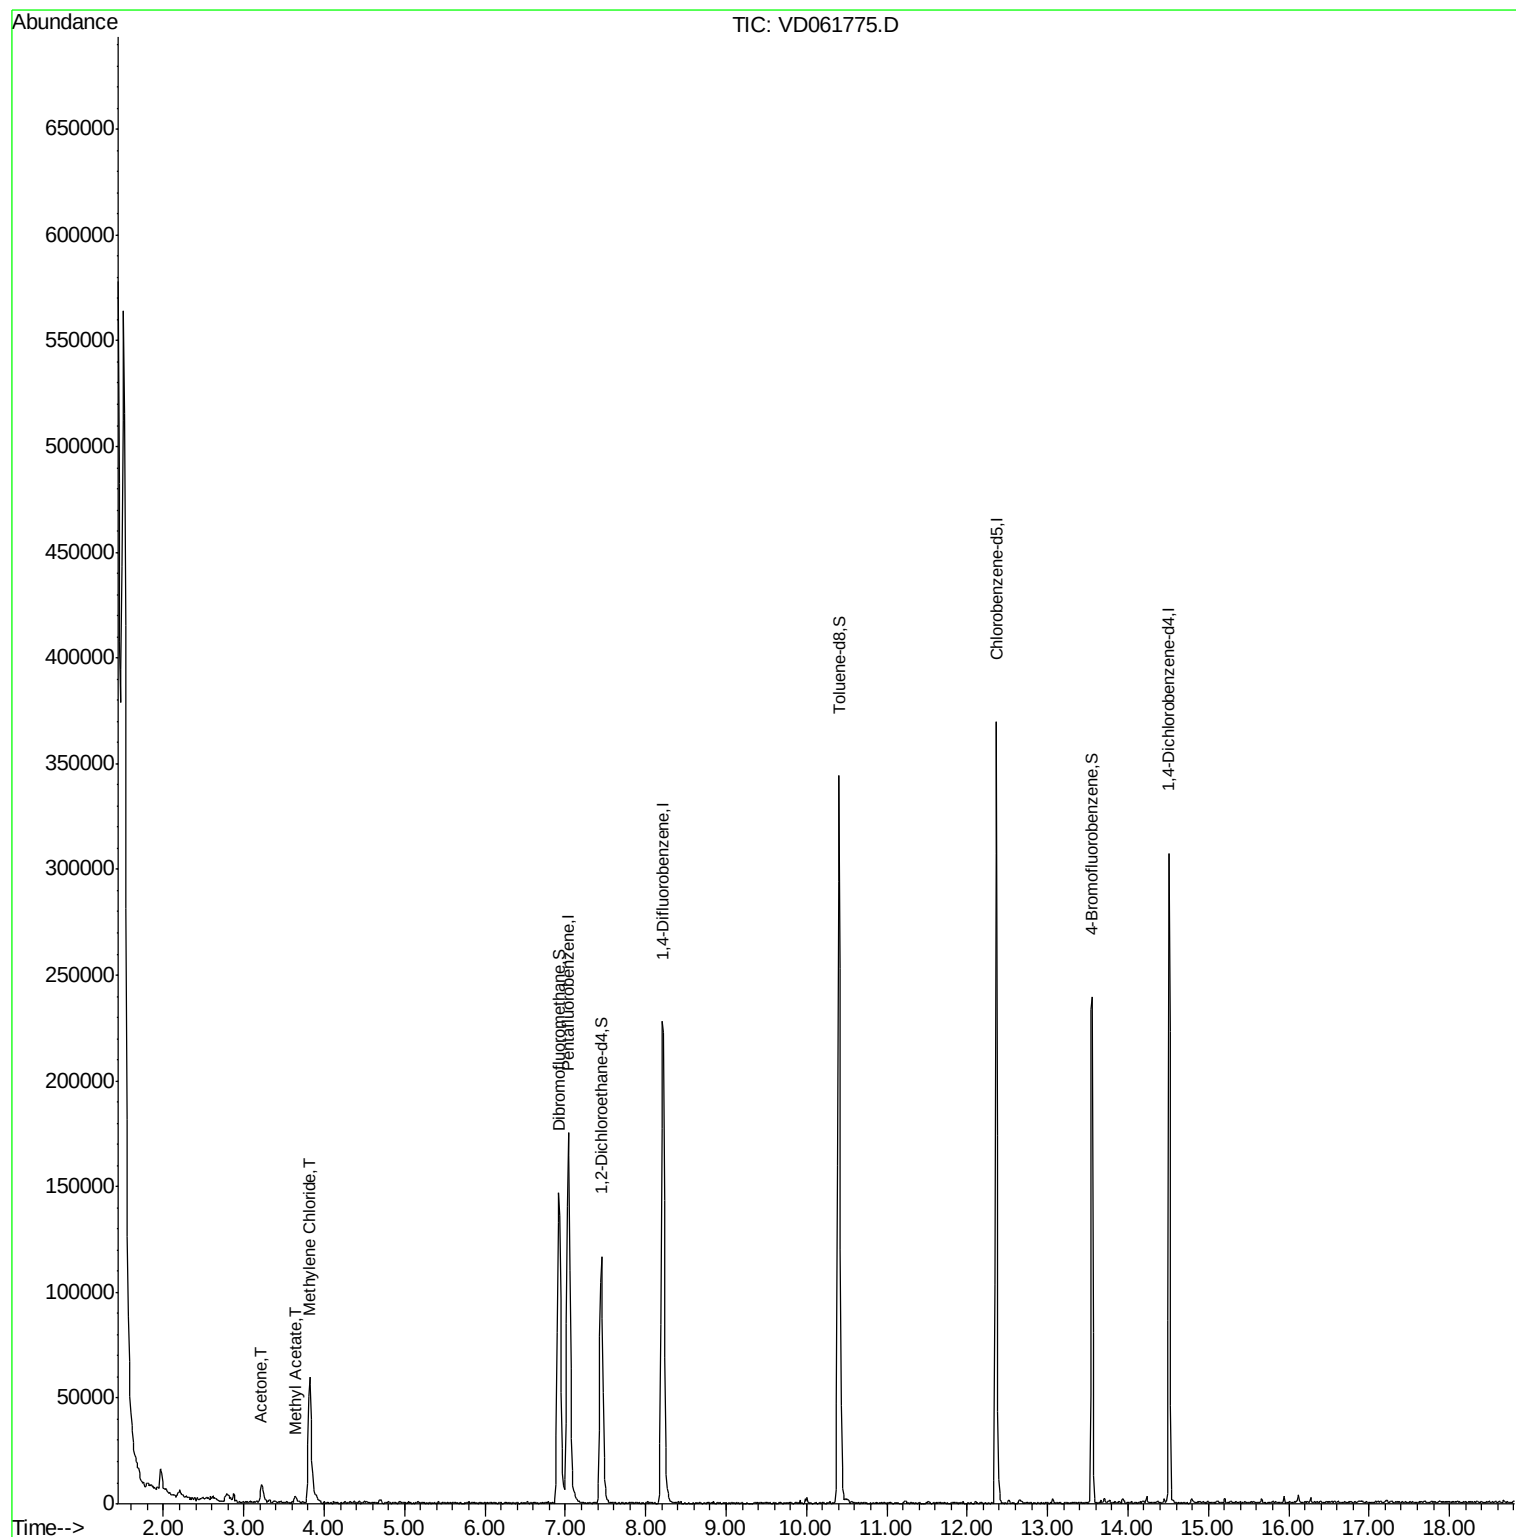


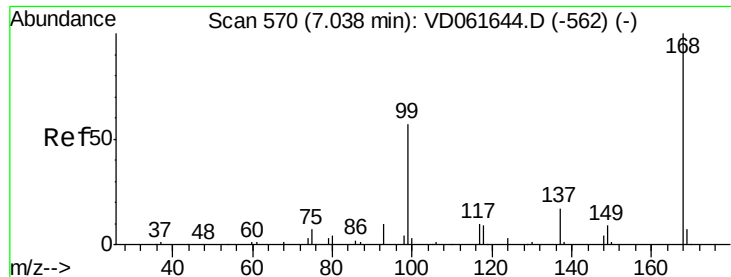

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.05 min Scan# 571
Delta R.T. 0.01 min
Lab File: VD061775.D
Acq: 12 Apr 2019 13:45




Instrument :
MSVOA_D
ClientSampleId :
WOOD-1RE


Tot Ion:168 Resp: 188151
Ion Ratio Lower Upper
168 100
99 50.4 46.8 70.2

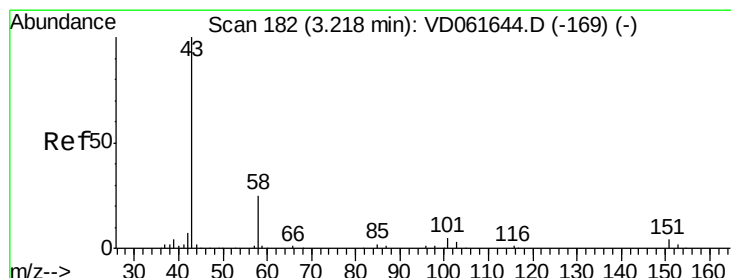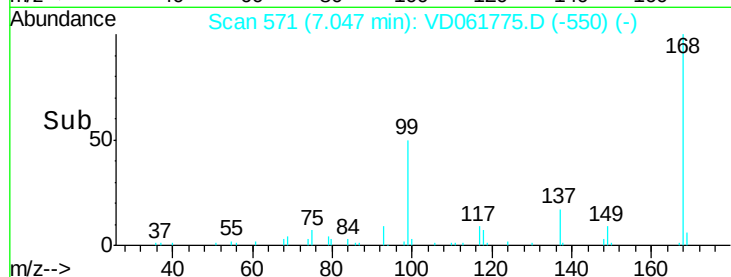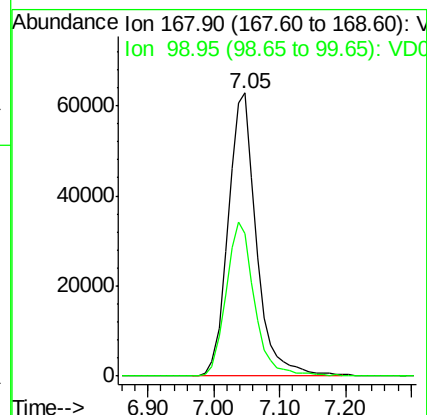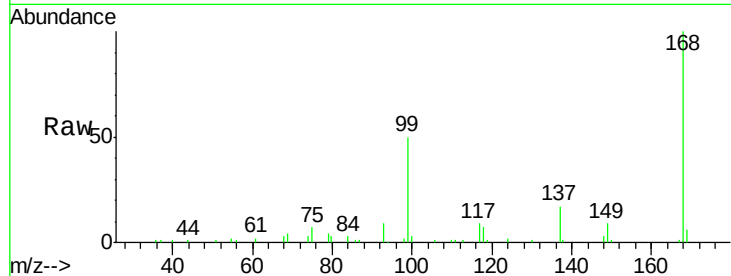

#16
Acetone
Concen: 43.384 ug/l
RT: 3.22 min Scan# 182
Delta R.T. -0.00 min
Lab File: VD061775.D
Acq: 12 Apr 2019 13:45

Tgt Ion: 43 Resp: 18496
Ion Ratio Lower Upper
43 100
58 25.4 19.7 29.5


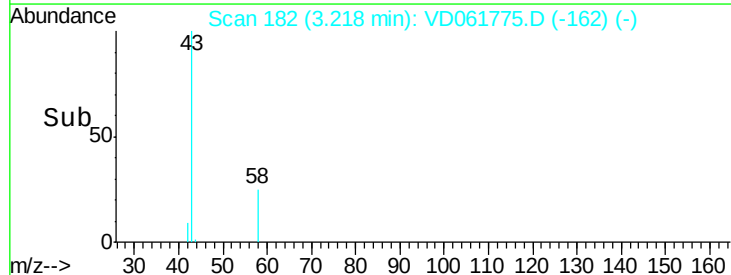
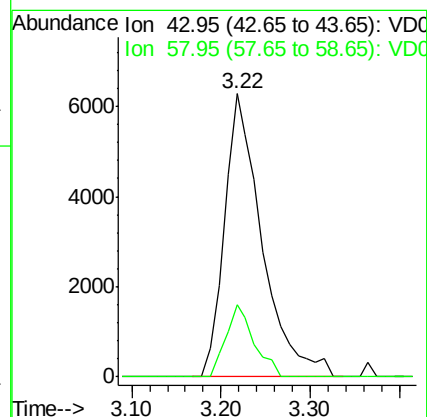
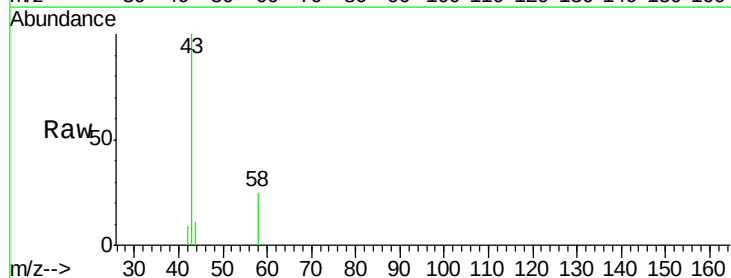


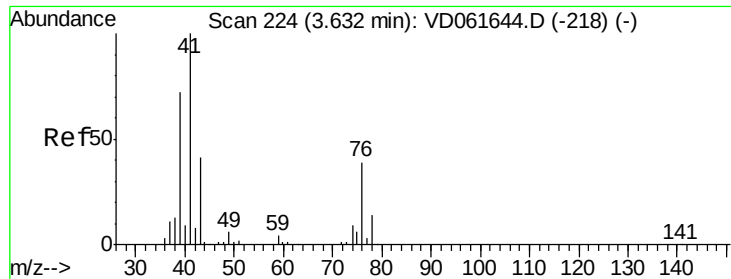

#18
Methyl Acetate
Concen: 7.712 ug/l
RT: 3.64 min Scan# 225
Delta R.T. 0.01 min
Lab File: VD061775.D
Acq: 12 Apr 2019 13:45




Instrument :
MSVOA_D
ClientSampleId :
WOOD-1RE


Tot Ion: 43 Resp: 6186
Ion Ratio Lower Upper
43 100
74 17.6 18.2 27.2#

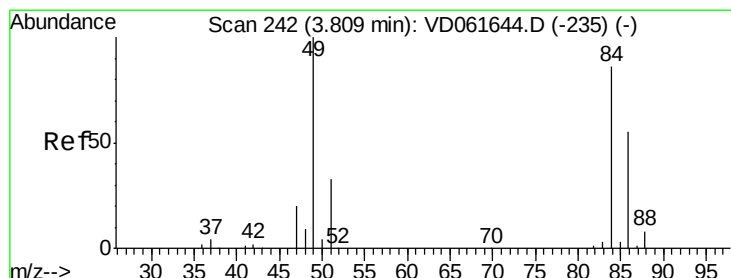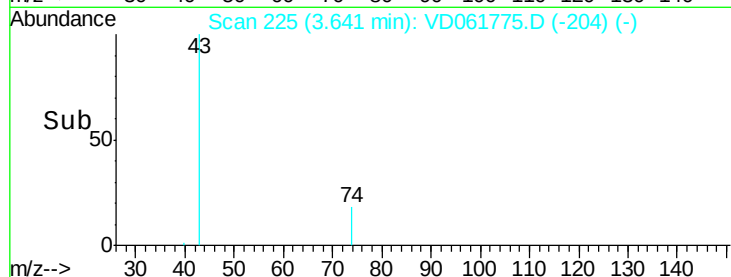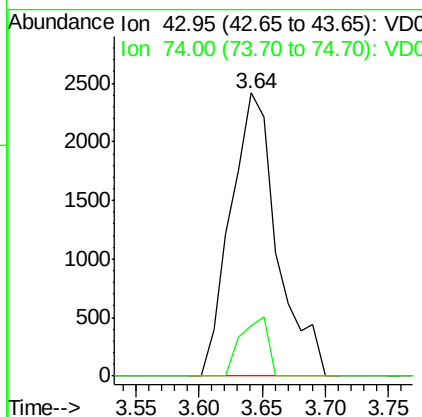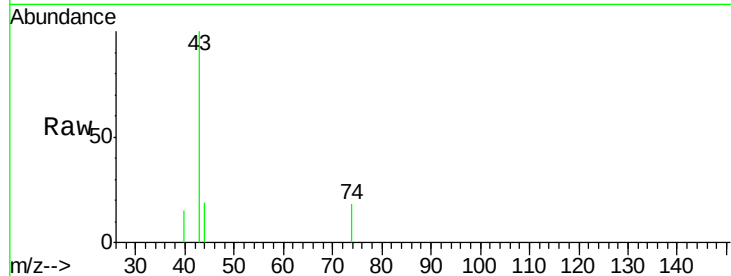

#20
Methylene Chloride
Concen: 19.570 ug/l
RT: 3.82 min Scan# 243
Delta R.T. 0.01 min
Lab File: VD061775.D
Acq: 12 Apr 2019 13:45

Tgt Ion: 84 Resp: 47345
Ion Ratio Lower Upper
84 100
49 111.3 93.0 139.4
51 38.7 30.4 45.6
86 64.4 51.0 76.4

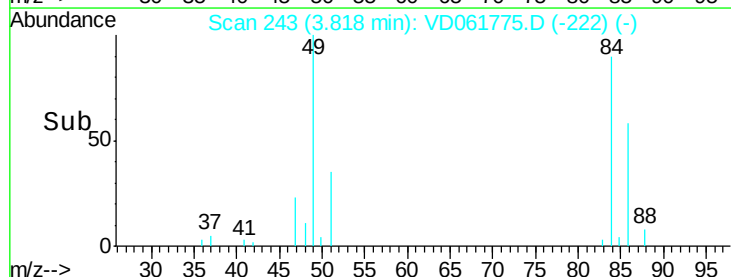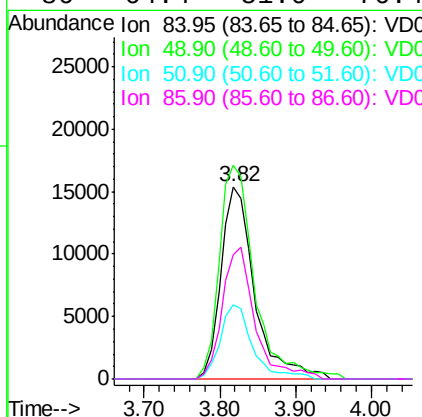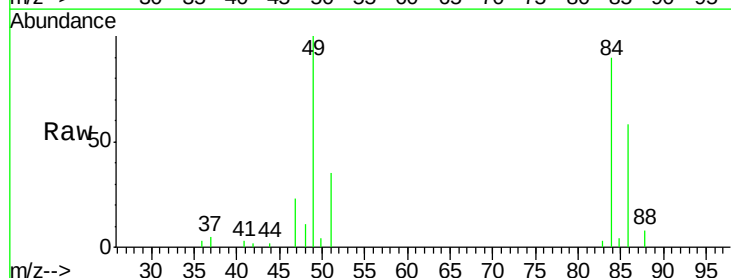

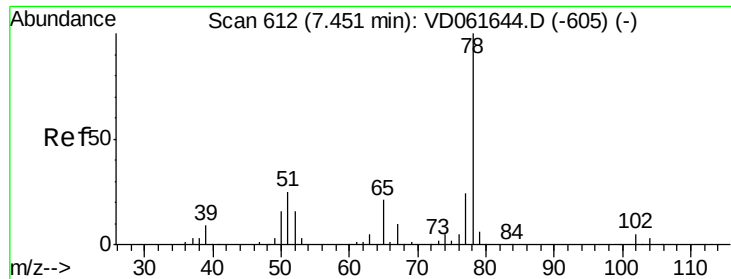

#33

1,2-Dichloroethane-d4

Concen: N.D. ug/l

RT: 7.45 min Scan# 612

Delta R.T. -0.00 min

Lab File: VD061775.D

Acq: 12 Apr 2019 13:45

Instrument :

MSVOA_D

ClientSampleId :


WOOD-1RE

Tot Ion: 65 Resp: 119224

Ion Ratio Lower Upper




65 100

67 49.4 0.0 99.4

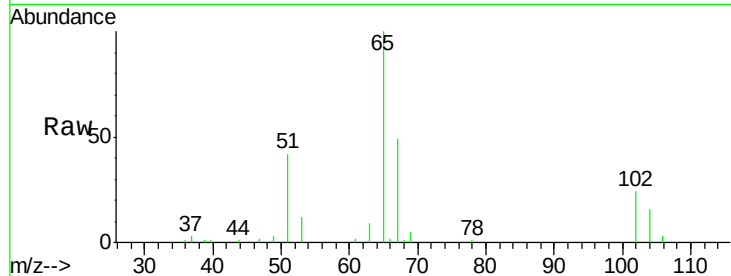

Abundance Ion 64.95 (64.65 to 65.65): VDC

Ion 66.90 (66.60 to 67.60): VDC

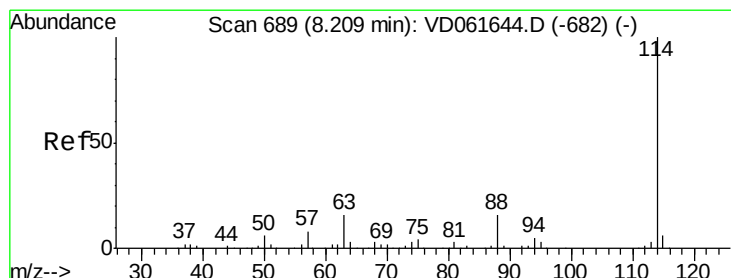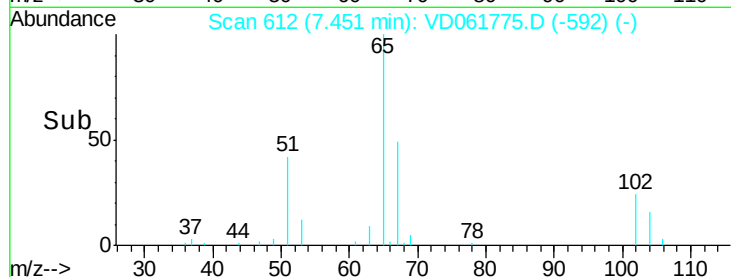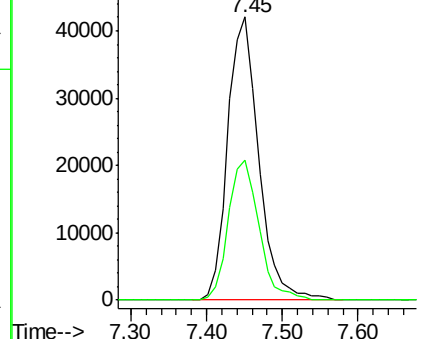

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.21 min Scan# 689

Delta R.T. -0.00 min

Lab File: VD061775.D

Acq: 12 Apr 2019 13:45


Tgt Ion: 114 Resp: 297026

Ion Ratio Lower Upper

114 100

63 16.1 0.0 31.2



88 16.5 0.0 31.8

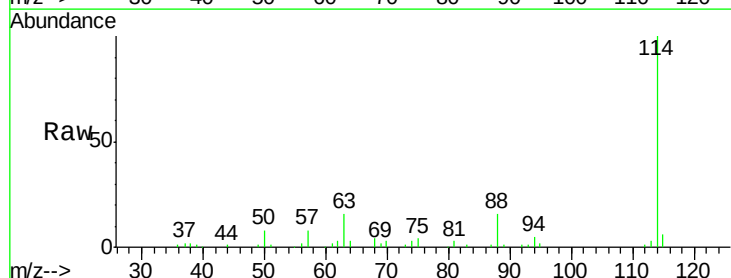


Abundance Ion 114.00 (113.70 to 114.70): V

Ion 62.95 (62.65 to 63.65): VDC

Ion 87.90 (87.60 to 88.60): VDC

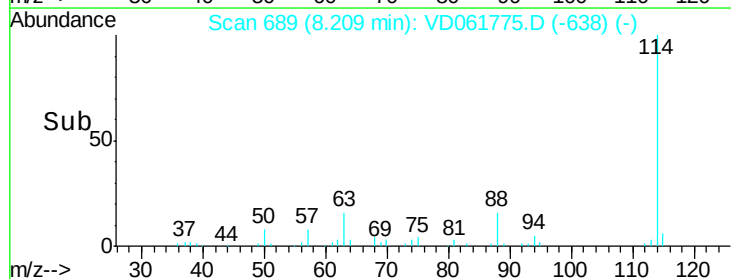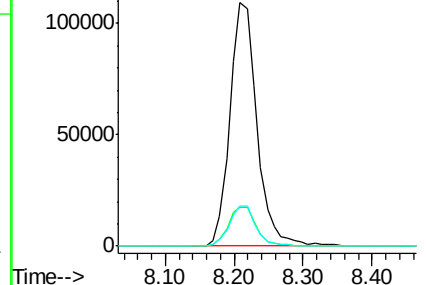


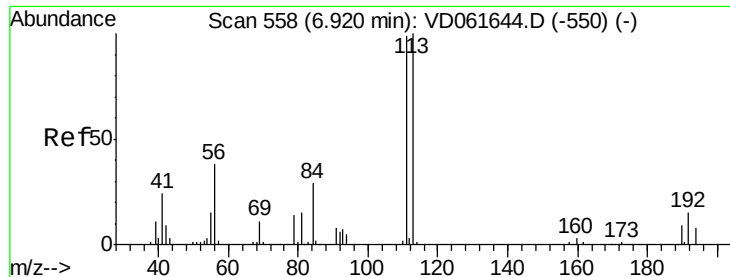




#35
 Dibromofluoromethane
 Concen: 50.000 ug/l
 RT: 6.92 min Scan# 558
 Delta R.T. -0.00 min
 Lab File: VD061775.D
 Acq: 12 Apr 2019 13:45

Instrument :
 MSVOA_D
 ClientSampleId :
 WOOD-1RE

Tot Ion:113 Resp: 147974
 Ion Ratio Lower Upper
 113 100
 111 104.7 79.3 118.9
 192 17.1 12.3 18.5

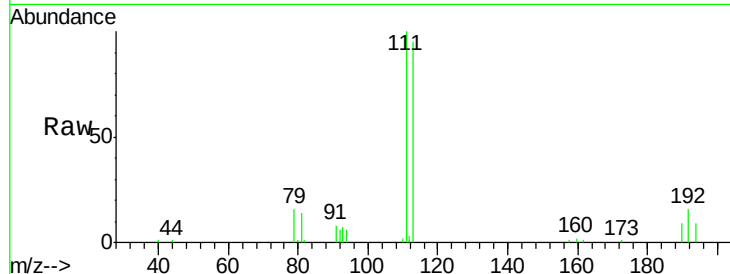


Abundance Ion 112.90 (112.60 to 113.60): V
 Ion 110.90 (110.60 to 111.60): V
 Ion 191.80 (191.50 to 192.50): V

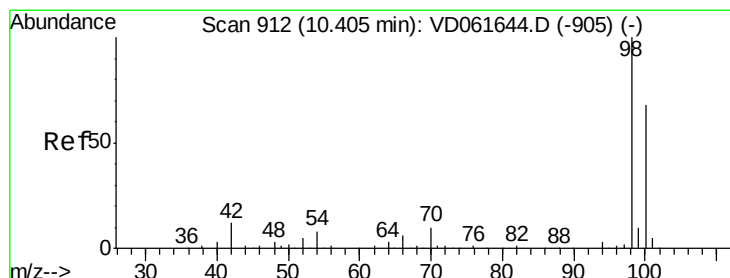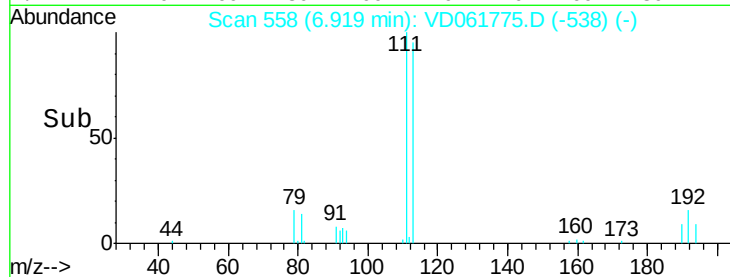
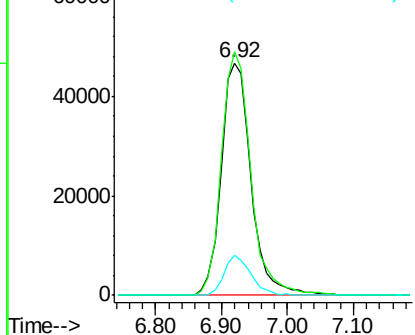



#50
 Toluene-d8
 Concen: N.D. ug/l
 RT: 10.40 min Scan# 912
 Delta R.T. -0.00 min
 Lab File: VD061775.D
 Acq: 12 Apr 2019 13:45

Tgt Ion: 98 Resp: 304202
 Ion Ratio Lower Upper
 98 100
 100 68.7 55.4 83.0

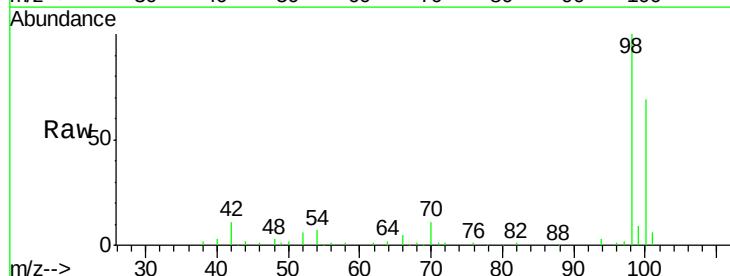

Abundance Ion 98.05 (97.75 to 98.75): VDC
 Ion 100.05 (99.75 to 100.75): VDC

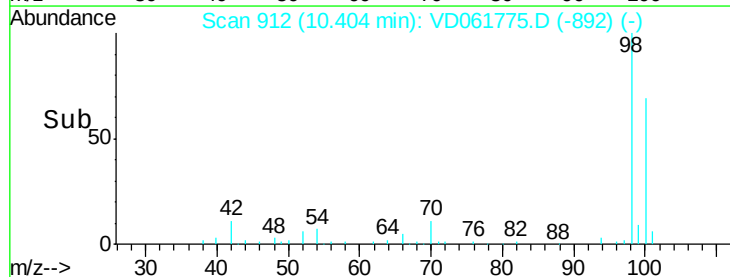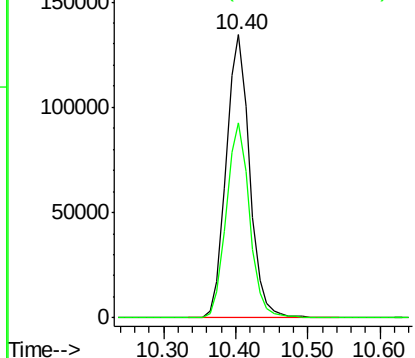

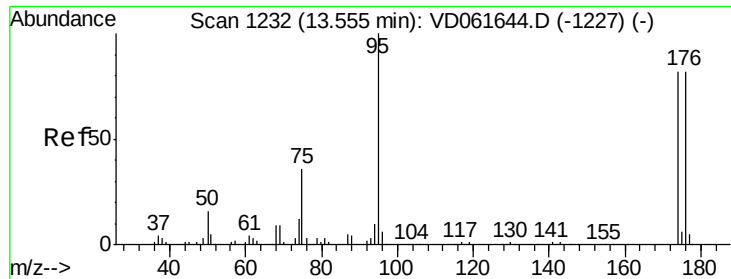

#62

4-Bromofluorobenzene

Concen: N.D. ug/l

RT: 13.54 min Scan# 1231

Delta R.T. -0.01 min

Lab File: VD061775.D

Acq: 12 Apr 2019 13:45

Instrument :

MSVOA_D

ClientSampleId :

WOOD-1RE


Tot Ion: 95 Resp: 81145

Ion Ratio Lower Upper

95 100

174 64.0 0.0 164.6




176 64.3 0.0 165.0

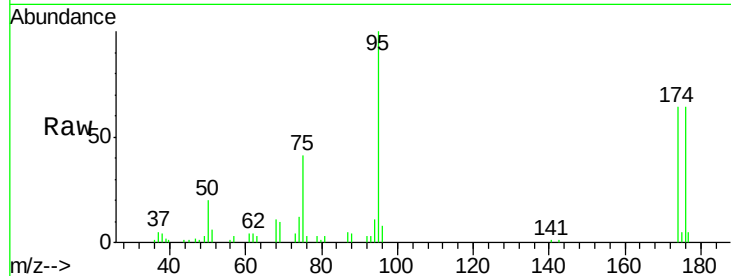

Abundance Ion 95.00 (94.70 to 95.70): V

Ion 173.90 (173.60 to 174.60): V

Ion 175.90 (175.60 to 176.60): V

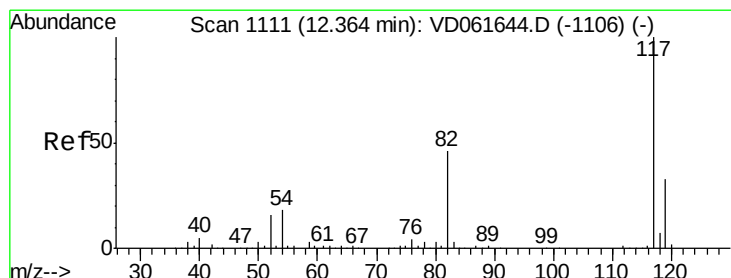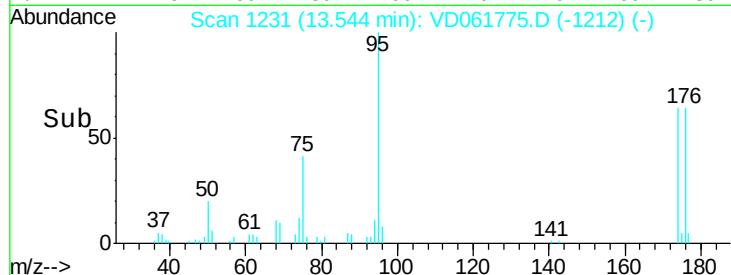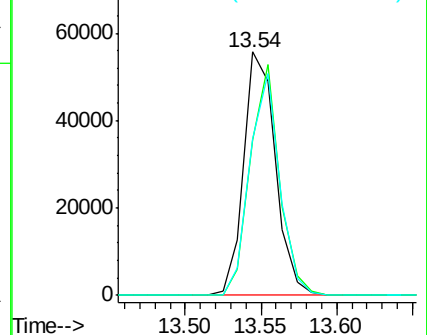

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 12.36 min Scan# 1111

Delta R.T. -0.00 min

Lab File: VD061775.D

Acq: 12 Apr 2019 13:45


Tgt Ion: 117 Resp: 227834

Ion Ratio Lower Upper

117 100

82 45.4 36.8 55.2



119 33.6 26.1 39.1

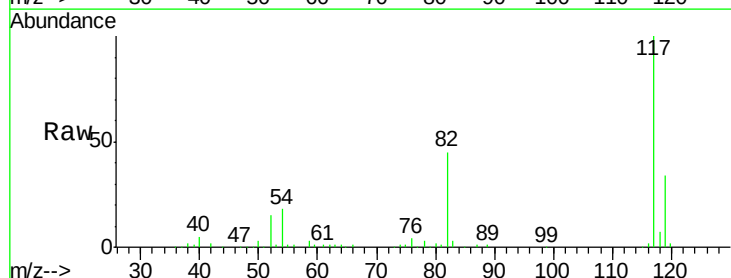


Abundance Ion 116.95 (116.65 to 117.65): V

Ion 82.05 (81.75 to 82.75): V

Ion 118.95 (118.65 to 119.65): V

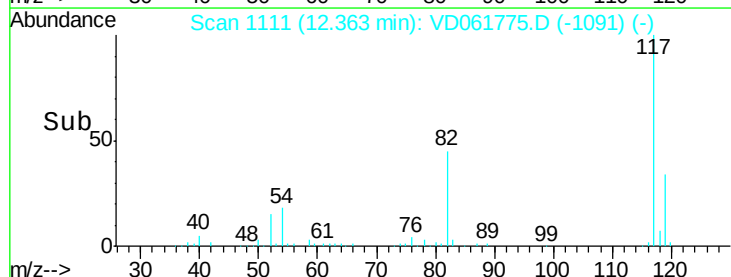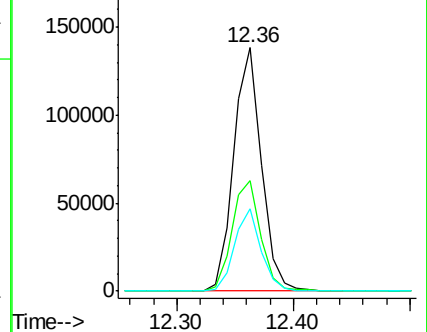


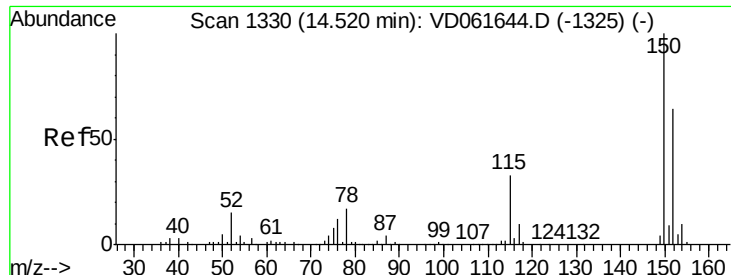

#72
 1,4-Dichlorobenzene-d4
 Concen: 50.000 ug/l
 RT: 14.51 min Scan# 1329
 Delta R.T. -0.01 min
 Lab File: VD061775.D
 Acq: 12 Apr 2019 13:45

Instrument :
 MSVOA_D
 ClientSampleId :
 WOOD-1RE

Tot Ion:152 Resp: 71619
 Ion Ratio Lower Upper
 152 100
 115 62.5 26.4 79.2
 150 160.6 0.0 320.6

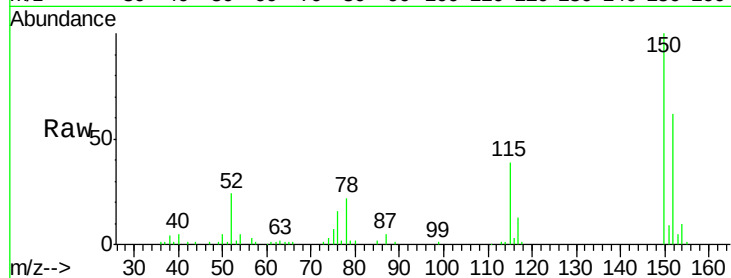

Abundance Ion 151.90 (151.60 to 152.60): V
 Ion 115.00 (114.70 to 115.70): V
 Ion 149.90 (149.60 to 150.60): V

