


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD041219\
Data File : VD061770.D
Acq On : 12 Apr 2019 9:36
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D040619S.M
Title : SW846 8260
Last Update : Mon Apr 08 10:04:03 2019

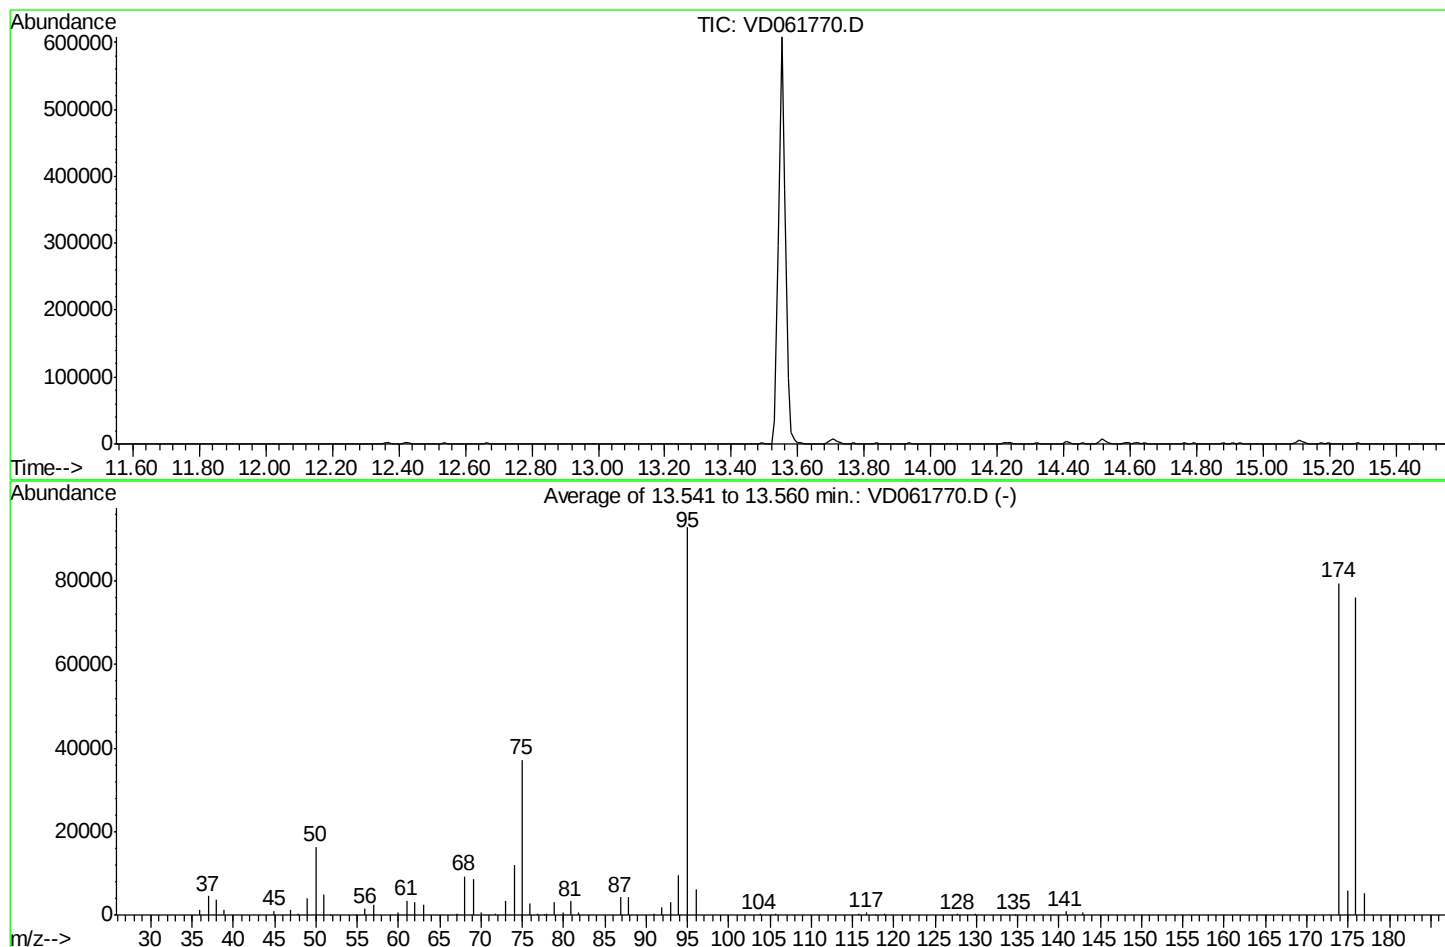

AutoFind: Scans 1231, 1232, 1233; Background Corrected with Scan 1226

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	16366	PASS
75	95	30	60	40.1	37253	PASS
95	95	100	100	100.0	92914	PASS
96	95	5	9	6.7	6201	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	85.7	79584	PASS
175	174	5	9	7.4	5893	PASS
176	174	95	101	95.7	76157	PASS
177	176	5	9	6.9	5273	PASS