
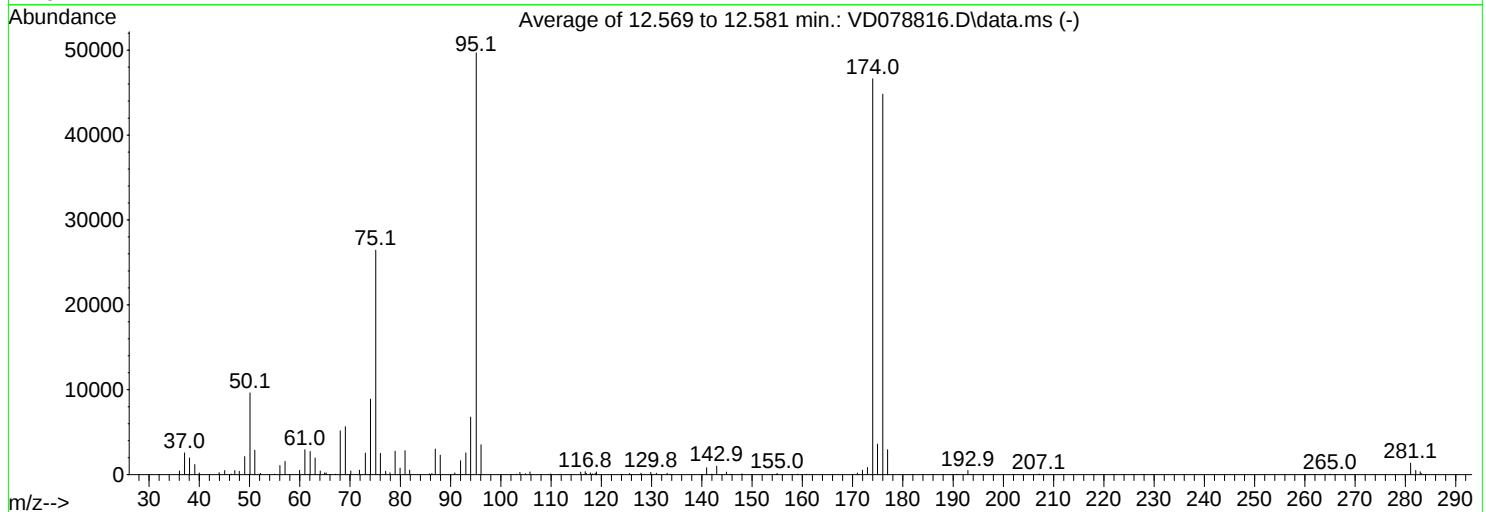


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD041624\  
Data File : VD078816.D  
Acq On : 16 Apr 2024 09:29  
Operator : RP/MD  
Sample : BFB  
Misc : 5.00G/5ml/MSVOA\_D/SOIL  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D031424S.M  
Title : SW846 8260  
Last Update : Fri Mar 15 05:38:03 2024

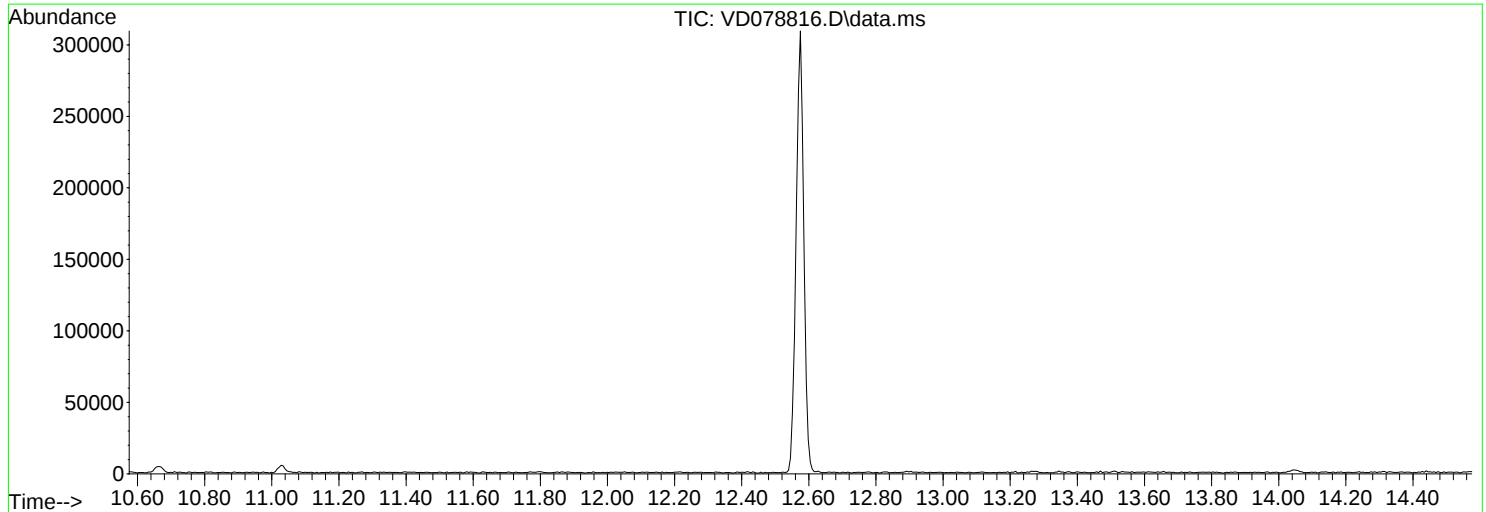

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

| Target | Rel. to | Lower  | Upper  | Rel.  | Raw   | Result    |
|--------|---------|--------|--------|-------|-------|-----------|
| Mass   | Mass    | Limit% | Limit% | Abn%  | Abn   | Pass/Fail |
| 50     | 95      | 15     | 40     | 19.4  | 9640  | PASS      |
| 75     | 95      | 30     | 60     | 53.2  | 26437 | PASS      |
| 95     | 95      | 100    | 100    | 100.0 | 49685 | PASS      |
| 96     | 95      | 5      | 9      | 7.1   | 3520  | PASS      |
| 173    | 174     | 0.00   | 2      | 1.8   | 848   | PASS      |
| 174    | 95      | 50     | 100    | 93.8  | 46627 | PASS      |
| 175    | 174     | 5      | 9      | 7.7   | 3601  | PASS      |
| 176    | 174     | 95     | 101    | 96.1  | 44819 | PASS      |
| 177    | 176     | 5      | 9      | 6.6   | 2947  | PASS      |