
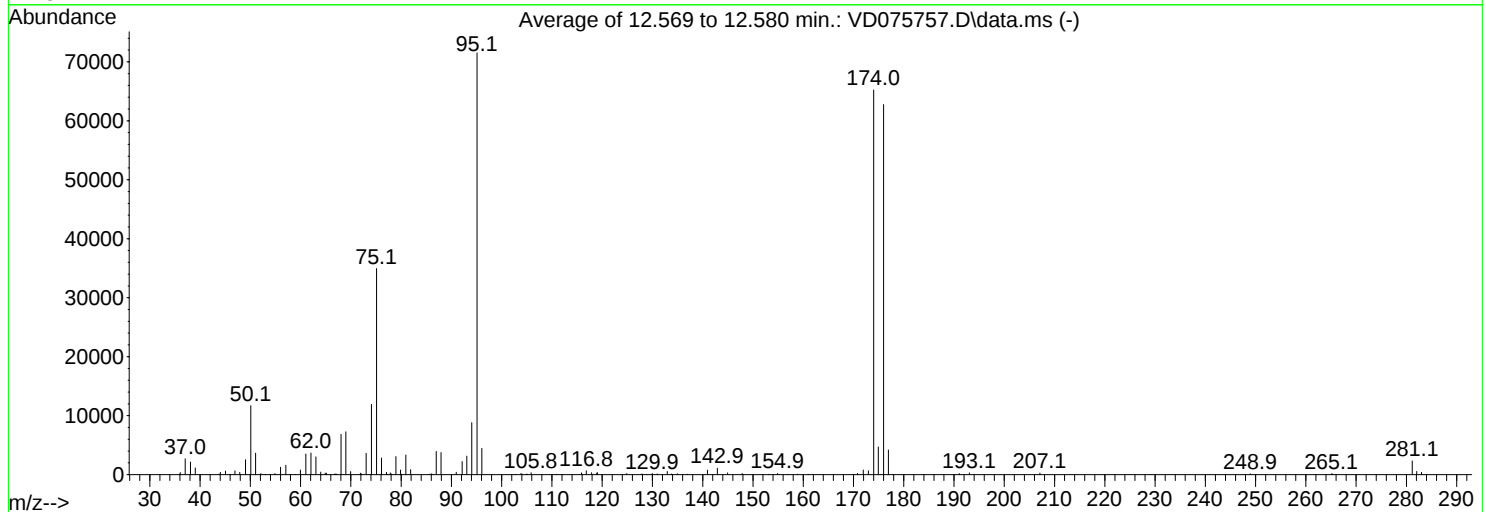


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042023\
Data File : VD075757.D
Acq On : 20 Apr 2023 09:15
Operator : KP/SY
Sample : BFB116
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB116

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Title : SFAM01.0
Last Update : Wed Apr 26 02:39:47 2023

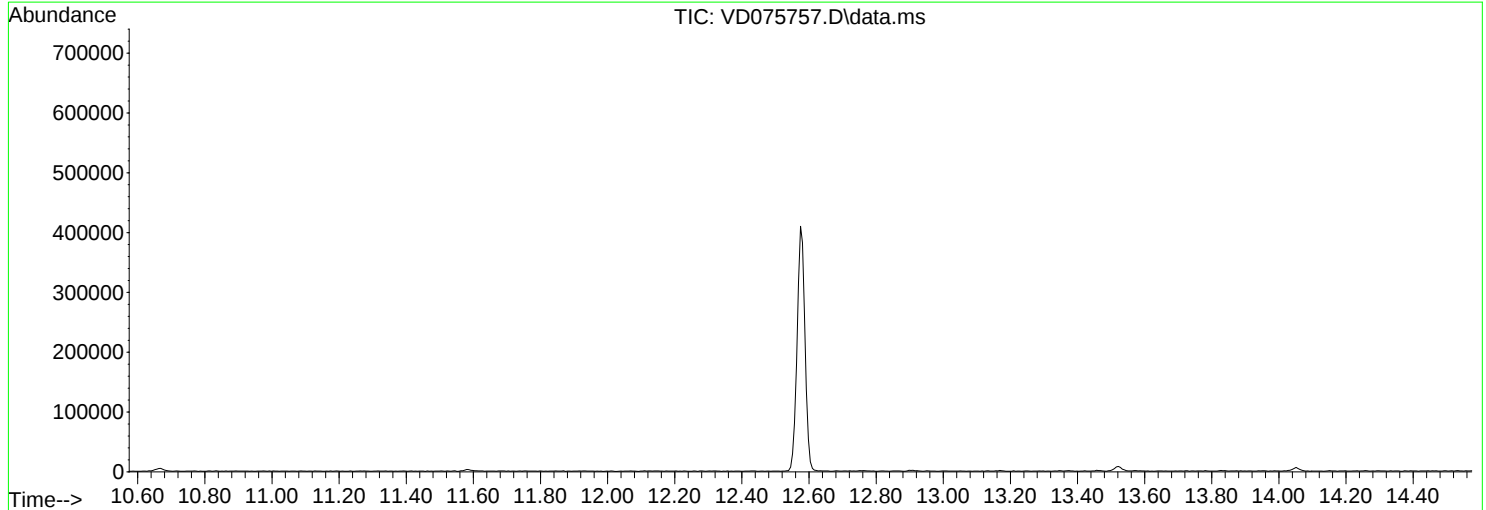

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	11703	PASS
75	95	30	80	48.8	34939	PASS
95	95	100	100	100.0	71525	PASS
96	95	5	9	6.2	4440	PASS
173	174	0.00	2	1.0	664	PASS
174	95	50	120	91.2	65219	PASS
175	174	5	9	7.2	4697	PASS
176	174	95	105	96.2	62755	PASS
177	176	5	10	6.7	4193	PASS

Scan 1860 (12.527 min): VD075757.D\data.ms
BFB116

m/z	Abundance
40.00	1076.0
44.00	310.0

Instrument :
MSVOA_D
ClientSampleId :
BFB116

m/z	Abundance
35.90	233.0
37.10	2645.0
38.10	2119.0
39.00	1097.0
39.90	849.0
44.10	594.0
45.00	536.0
46.90	610.0
47.90	439.0
49.10	2223.0
50.10	10432.0
51.10	2806.0
52.10	153.0
54.90	271.0
56.00	1126.0
57.10	1344.0
59.90	536.0
61.00	3254.0
62.10	2856.0
63.10	2922.0
64.00	478.0
64.90	501.0
66.80	361.0
68.00	5484.0
69.00	6000.0
69.90	348.0
71.90	312.0
73.00	3472.0
74.10	10934.0
75.10	30760.0
76.10	2450.0
77.10	346.0
78.10	369.0
78.90	2327.0
79.90	679.0
80.90	3065.0
81.90	726.0
86.20	306.0
87.00	3149.0
87.90	2886.0
90.90	453.0
92.10	1753.0
93.00	2866.0
94.10	7739.0
95.10	62752.0
96.10	3607.0
103.80	209.0
105.80	266.0
115.90	296.0
116.90	486.0
118.00	412.0
118.90	743.0
127.70	160.0
130.00	195.0
130.90	184.0
133.00	180.0
133.70	159.0
135.00	158.0
141.10	768.0
142.80	908.0
145.00	322.0
147.80	233.0
153.10	183.0
154.90	408.0
170.80	260.0
171.90	699.0
173.00	503.0
174.00	54128.0
175.00	4304.0
176.00	51128.0
177.00	4042.0
191.00	189.0
207.20	214.0
281.10	1504.0
282.00	399.0
283.00	273.0

Instrument :
MSVOA_D
ClientSampleId :
BFB116

m/z	Abundance
36.10	377.0
37.00	2633.0
38.10	2326.0
39.10	1082.0
40.00	1068.0
43.80	366.0
44.20	476.0
45.10	828.0
45.90	160.0
47.00	607.0
48.00	413.0
49.00	3012.0
50.10	12869.0
51.00	4210.0
52.20	238.0
56.00	1344.0
57.00	2007.0
58.90	163.0
60.00	992.0
61.10	4333.0
62.10	4430.0
63.00	3282.0
64.00	328.0
65.10	428.0
67.00	301.0
68.00	7699.0
69.00	8411.0
70.00	642.0
72.10	391.0
73.10	3196.0
74.10	13008.0
75.10	39192.0
76.10	3176.0
77.10	612.0
77.80	412.0
79.00	3612.0
80.00	902.0
81.00	3699.0
81.90	834.0
85.70	230.0
87.00	4737.0
88.00	4180.0
90.90	409.0
92.20	2242.0
93.10	2947.0
94.00	9566.0
95.10	80000.0
96.10	5257.0
104.10	276.0
104.90	218.0
105.90	280.0
115.90	249.0
116.80	777.0
117.80	320.0
119.10	543.0
124.90	291.0
127.90	217.0
128.90	167.0
130.00	193.0
131.00	211.0
133.00	835.0
133.90	169.0
134.90	166.0
140.90	768.0
142.90	1315.0
144.90	298.0
147.90	218.0
154.90	260.0
170.80	215.0
172.00	860.0
172.90	589.0
174.00	73344.0
174.90	5298.0
176.00	69160.0
177.00	4459.0
191.00	202.0
193.00	318.0
207.10	272.0
249.00	210.0
265.10	424.0
281.10	2549.0
282.10	627.0
283.00	525.0

Instrument :
MSVOA_D
ClientSampleId :
BFB116

m/z	Abundance
36.00	673.0
37.10	2830.0
38.10	1965.0
39.10	1261.0
40.00	1243.0
44.00	1008.0
45.10	417.0
46.90	732.0
47.80	333.0
49.00	2361.0
50.10	11809.0
51.10	3929.0
52.00	166.0
53.00	159.0
54.90	331.0
56.00	1299.0
57.10	1465.0
60.00	812.0
61.10	2956.0
62.00	3680.0
63.10	2841.0
64.00	475.0
64.90	325.0
65.20	288.0
67.20	222.0
68.10	7365.0
69.00	7376.0
70.00	557.0
71.90	451.0
73.10	4137.0
74.10	11785.0
75.10	34864.0
76.10	2836.0
77.00	211.0
77.30	195.0
77.90	506.0
79.00	3238.0
79.80	769.0
81.00	3285.0
81.90	936.0
86.00	186.0
87.00	3885.0
87.90	4144.0
91.00	384.0
92.10	2655.0
93.00	3600.0
94.10	9121.0
95.10	71824.0
96.00	4457.0
102.70	166.0
103.90	446.0
105.10	271.0
105.90	439.0
111.00	222.0
115.90	368.0
116.90	674.0
117.90	277.0
119.00	503.0
124.90	251.0
128.00	180.0
129.90	266.0
132.90	658.0
133.80	189.0
134.90	158.0
136.90	258.0
140.80	788.0
143.00	1034.0
145.00	298.0
147.90	163.0
156.90	188.0
158.90	230.0
161.00	168.0
170.80	212.0
172.00	807.0
173.00	900.0
174.00	68184.0
174.90	4490.0
176.00	67976.0
176.90	4077.0
177.80	157.0
191.10	192.0
193.10	562.0
207.00	310.0
248.90	194.0
265.30	363.0
281.20	2985.0
282.00	645.0
283.00	354.0

Instrument :
MSVOA_D
ClientSampleId :
BFB116