




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042123\
Data File : VD075773.D
Acq On : 21 Apr 2023 14:01
Operator : KP/SY
Sample : 02447-05
Misc : 3.48G/10.00ml/MSVOA_D/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
EW910

Manual IntegrationsAPPROVED

Quant Time: Apr 22 03:54:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 22 03:53:08 2023
Response via : Initial Calibration

Reviewed By :Krupa Patel 04/24/2023
Supervised By :Semsettin Yesilyurt 04/24/2023

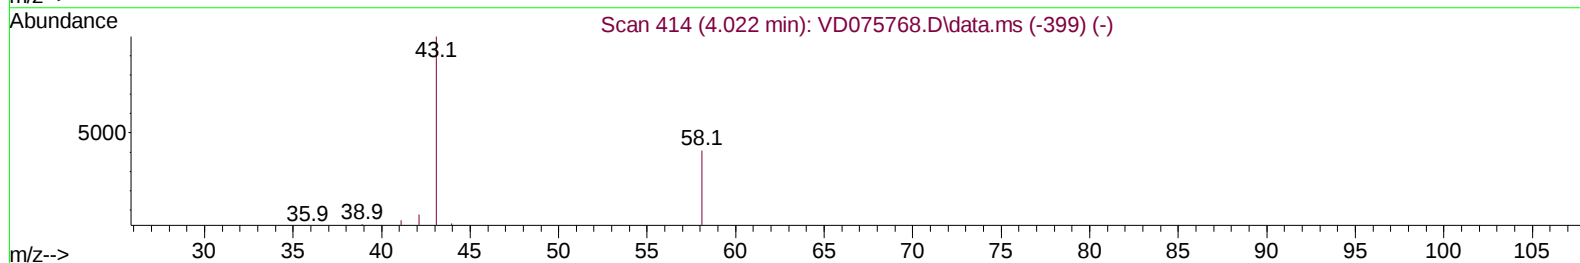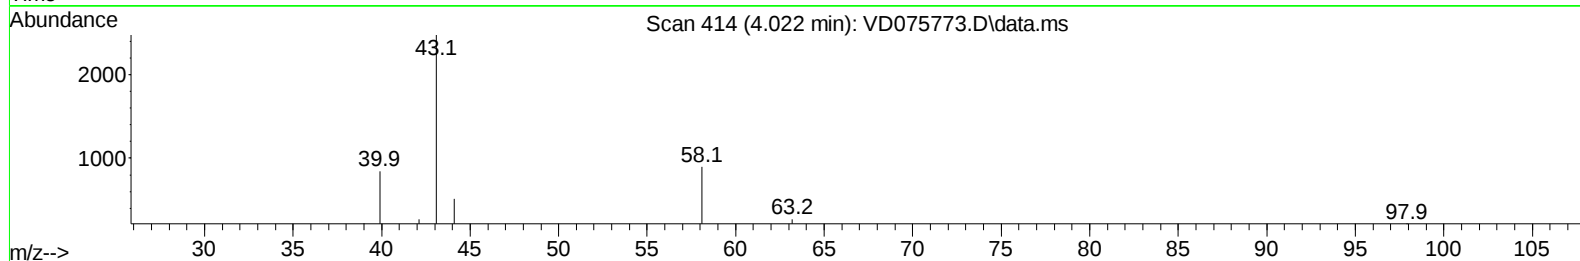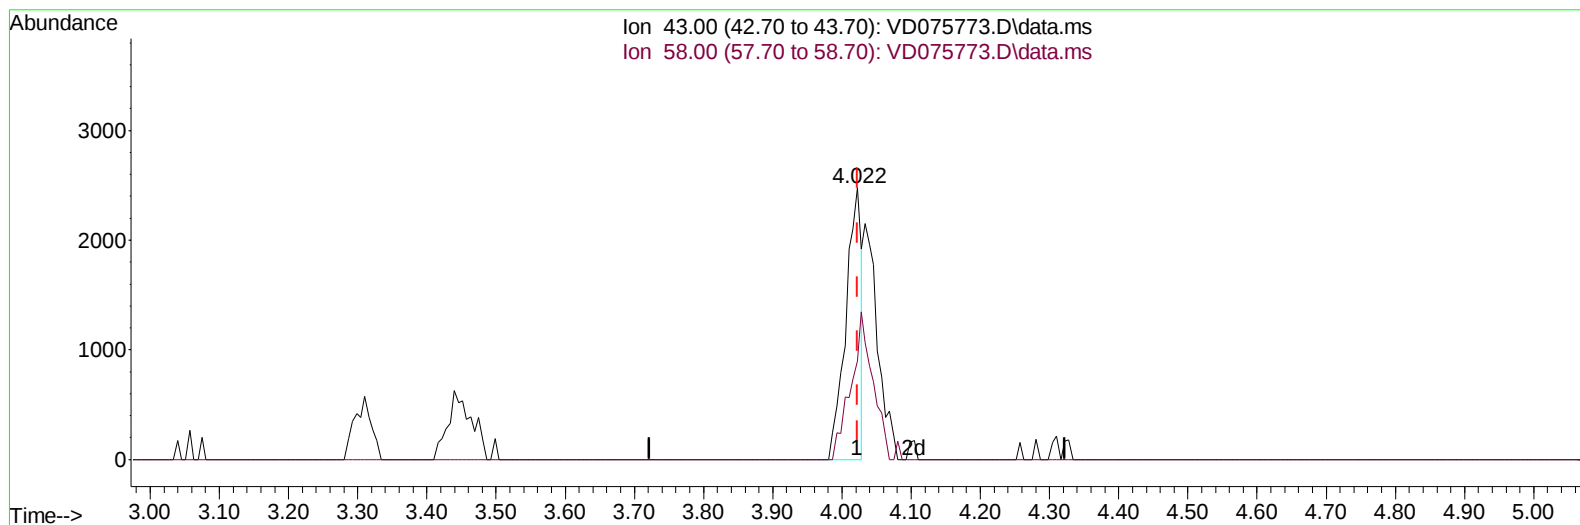

TIC: VD075773.D\data.ms

(13) Acetone (T)

4.022min (-0.000) 7.18 ug/L

response 3874

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	43.70	75.84
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042123\
 Data File : VD075773.D
 Acq On : 21 Apr 2023 14:01
 Operator : KP/SY
 Sample : 02447-05
 Misc : 3.48G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 EW910

Manual IntegrationsAPPROVED

Quant Time: Apr 22 03:54:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 22 03:53:08 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/24/2023
 Supervised By :Semsettin Yesilyurt 04/24/2023

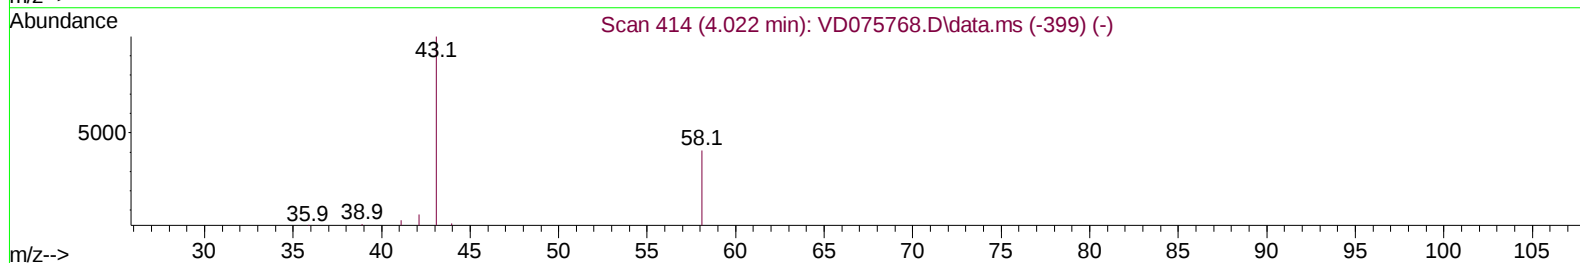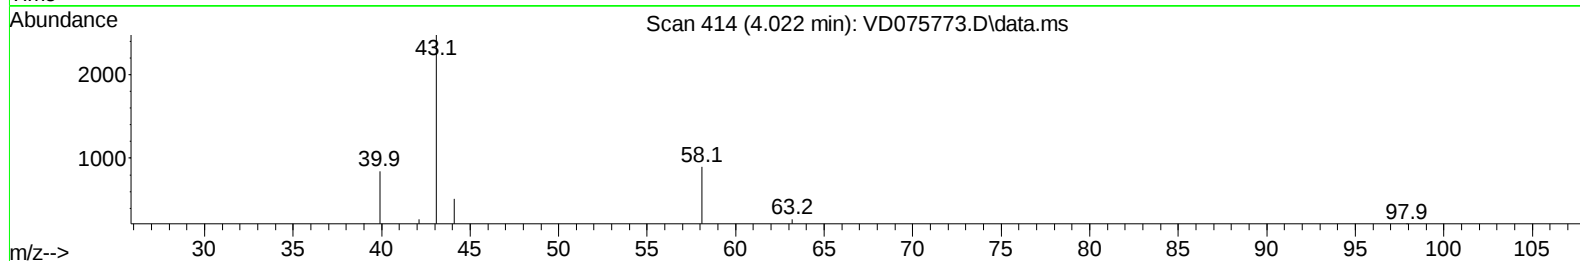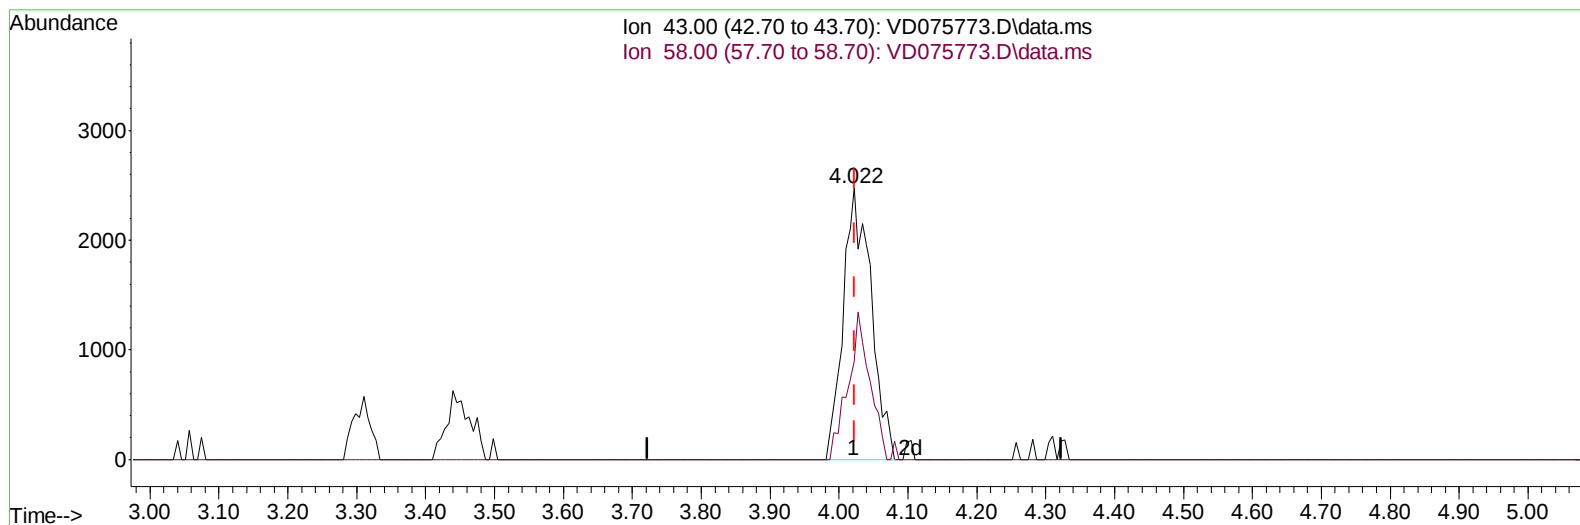

TIC: VD075773.D\data.ms

(13) Acetone (T)

4.022min (-0.000) 12.85 ug/L m

response 6929

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	43.70	42.40
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042123\
 Data File : VD075773.D
 Acq On : 21 Apr 2023 14:01
 Operator : KP/SY
 Sample : 02447-05
 Misc : 3.48G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 EW910

Manual IntegrationsAPPROVED

Quant Time: Apr 22 03:54:59 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 22 03:53:08 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/24/2023
 Supervised By :Semsettin Yesilyurt 04/24/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.781	114	330973	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.586	117	251036	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.521	152	61374	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.275	65	243858	33.586	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	134.360%		
7) Chloroethane-d5	2.804	69	197479	31.479	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	125.920%		
11) 1,1-Dichloroethene-d2	3.922	65	49526	29.587	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	118.360%#		
21) 2-Butanone-d5	6.992	46	30361	48.168	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	96.340%		
24) Chloroform-d	7.569	84	227210	27.452	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	109.800%		
26) 1,2-Dichloroethane-d4	8.228	65	97465	27.576	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	110.320%		
32) Benzene-d6	8.204	84	483884	33.071	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	132.280%		
36) 1,2-Dichloropropane-d6	9.210	67	137404	33.928	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	135.720%#		
41) Toluene-d8	10.269	98	401015	29.276	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	117.120%		
43) trans-1,3-Dichloroprop...	10.528	79	46739	27.921	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	111.680%		
47) 2-Hexanone-d5	10.880	63	25186	51.650	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	103.300%		
56) 1,1,2,2-Tetrachloroeth...	12.651	84	79712	25.722	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	102.880%		
66) 1,2-Dichlorobenzene-d4	13.816	152	53528	24.657	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	98.640%		
Target Compounds						
						Qvalue
13) Acetone	4.022	43	6929m	12.846	ug/L	
16) Methylene chloride	4.804	84	31162	4.641	ug/L	97

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042123\
Data File : VD075773.D
Acq On : 21 Apr 2023 14:01
Operator : KP/SY
Sample : 02447-05
Misc : 3.48G/10.00ml/MSVOA_D/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
EW910

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/24/2023
Supervised By :Semsettin Yesilyurt 04/24/2023

Quant Time: Apr 22 03:54:59 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 22 03:53:08 2023
Response via : Initial Calibration

