




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042123\
 Data File : VD075776.D
 Acq On : 21 Apr 2023 15:28
 Operator : KP/SY
 Sample : 02447-08
 Misc : 5.30G/10.00mL/MSVOA_D/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 EW913

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/24/2023
 Supervised By :Semsettin Yesilyurt 04/24/2023

Quant Time: Apr 22 03:55:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 22 03:53:08 2023
 Response via : Initial Calibration

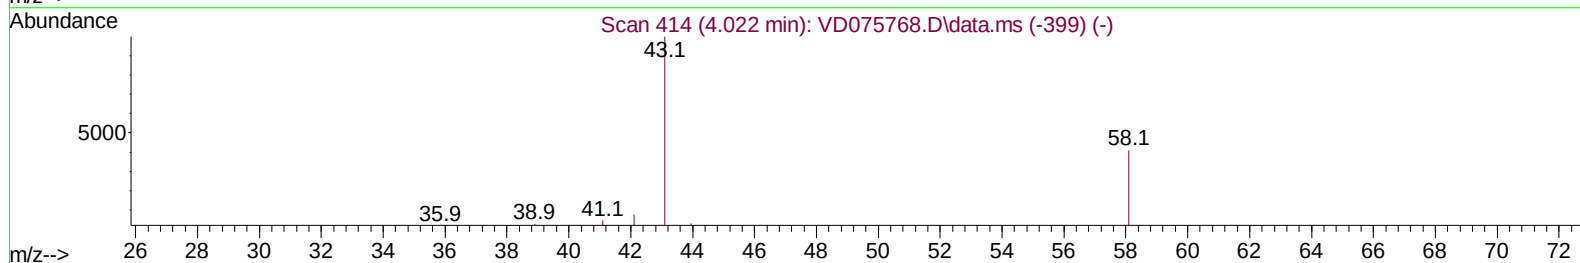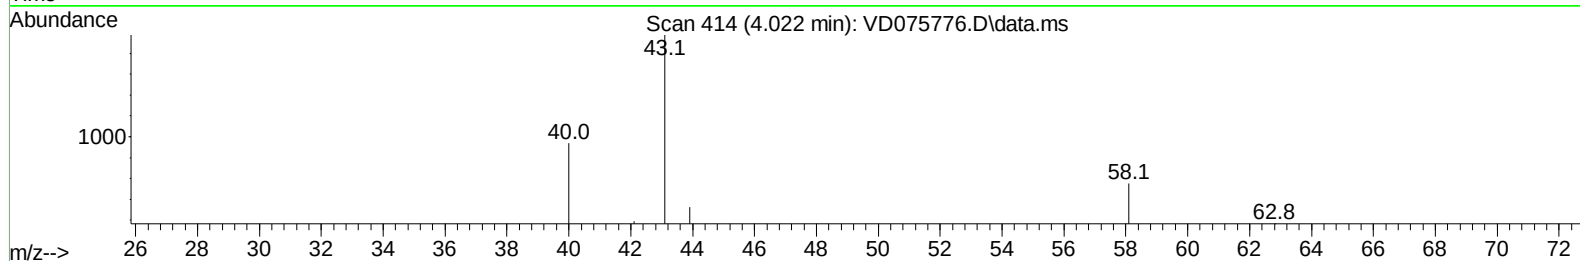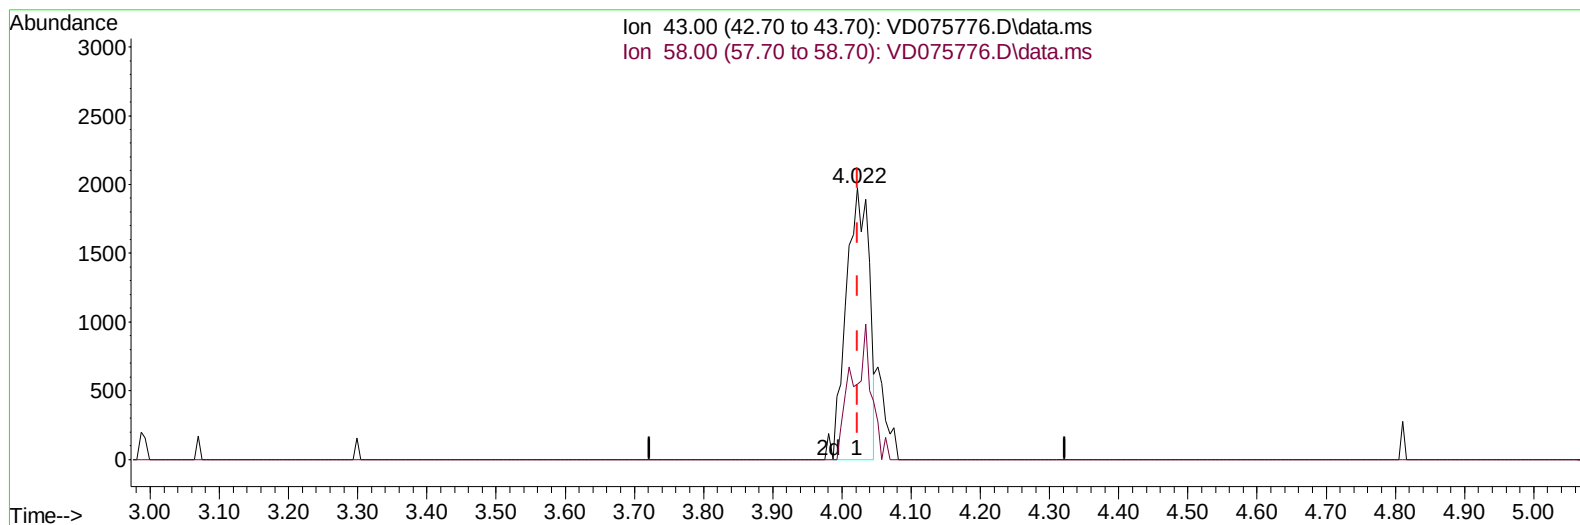

TIC: VD075776.D\data.ms

(13) Acetone (T)

4.022min (-0.000) 7.01 ug/L

response 4549

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	43.70	21.37
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042123\
 Data File : VD075776.D
 Acq On : 21 Apr 2023 15:28
 Operator : KP/SY
 Sample : 02447-08
 Misc : 5.30G/10.00mL/MSVOA_D/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 EW913

Manual IntegrationsAPPROVED

Quant Time: Apr 22 03:55:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 22 03:53:08 2023
 Response via : Initial Calibration

Reviewed By :Krupa Patel 04/24/2023
 Supervised By :Semsettin Yesilyurt 04/24/2023

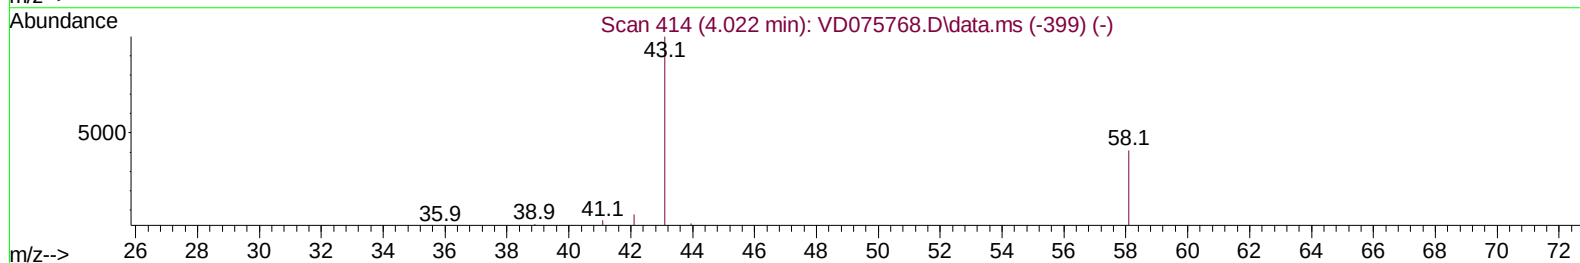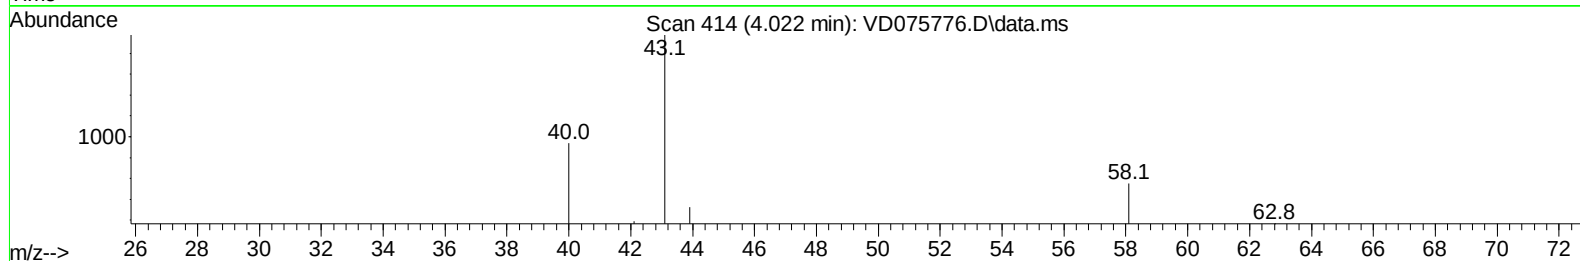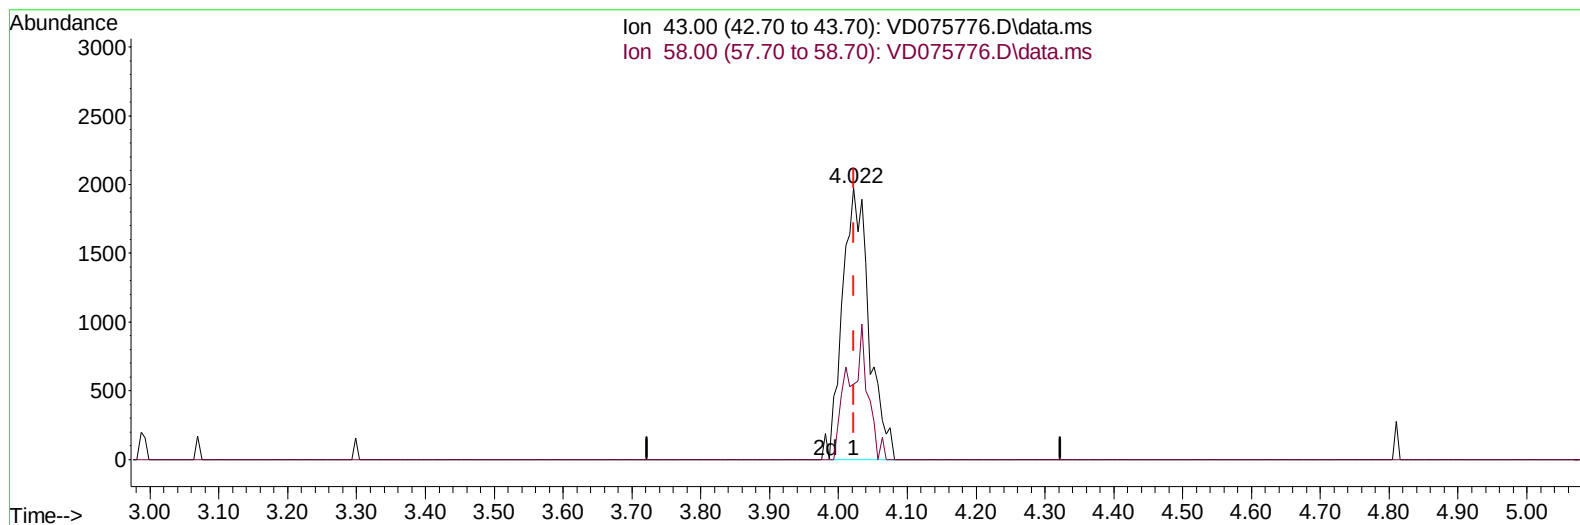

TIC: VD075776.D\data.ms

(13) Acetone (T)

4.022min (-0.000) 8.06 ug/L m

response 5228

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	43.70	18.59
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042123\
 Data File : VD075776.D
 Acq On : 21 Apr 2023 15:28
 Operator : KP/SY
 Sample : 02447-08
 Misc : 5.30G/10.00ml/MSVOA_D/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 EW913

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/24/2023
 Supervised By :Semsettin Yesilyurt 04/24/2023

Quant Time: Apr 22 03:55:38 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Apr 22 03:53:08 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.781	114		397916	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117		330610	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.522	152		94266	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.275	65		220067	25.210	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	100.840%	
7) Chloroethane-d5	2.805	69		194772	25.824	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	103.280%	
11) 1,1-Dichloroethene-d2	3.916	65		46771	23.240	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	92.960%	
21) 2-Butanone-d5	6.987	46		34361	45.343	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	90.680%	
24) Chloroform-d	7.569	84		235893	23.707	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	94.840%	
26) 1,2-Dichloroethane-d4	8.228	65		105594	24.850	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	99.400%	
32) Benzene-d6	8.204	84		501093	26.005	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	104.000%	
36) 1,2-Dichloropropane-d6	9.210	67		143503	26.906	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	107.640%	
41) Toluene-d8	10.269	98		406869	22.554	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	90.200%	
43) trans-1,3-Dichloroprop...	10.528	79		52551	23.837	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	95.360%	
47) 2-Hexanone-d5	10.875	63		29065	45.259	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	90.520%	
56) 1,1,2,2-Tetrachloroeth...	12.651	84		87421	21.420	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	85.680%	
66) 1,2-Dichlorobenzene-d4	13.816	152		60637	18.186	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	72.760%#	
Target Compounds							
13) Acetone	4.022	43		5228m	8.062	ug/L	
16) Methylene chloride	4.805	84		40130	4.971	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD042123\
Data File : VD075776.D
Acq On : 21 Apr 2023 15:28
Operator : KP/SY
Sample : 02447-08
Misc : 5.30G/10.00mL/MSVOA_D/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
EW913

Manual IntegrationsAPPROVED

Reviewed By :Krupa Patel 04/24/2023
Supervised By :Semsettin Yesilyurt 04/24/2023

Quant Time: Apr 22 03:55:38 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM042023SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Apr 22 03:53:08 2023
Response via : Initial Calibration

