
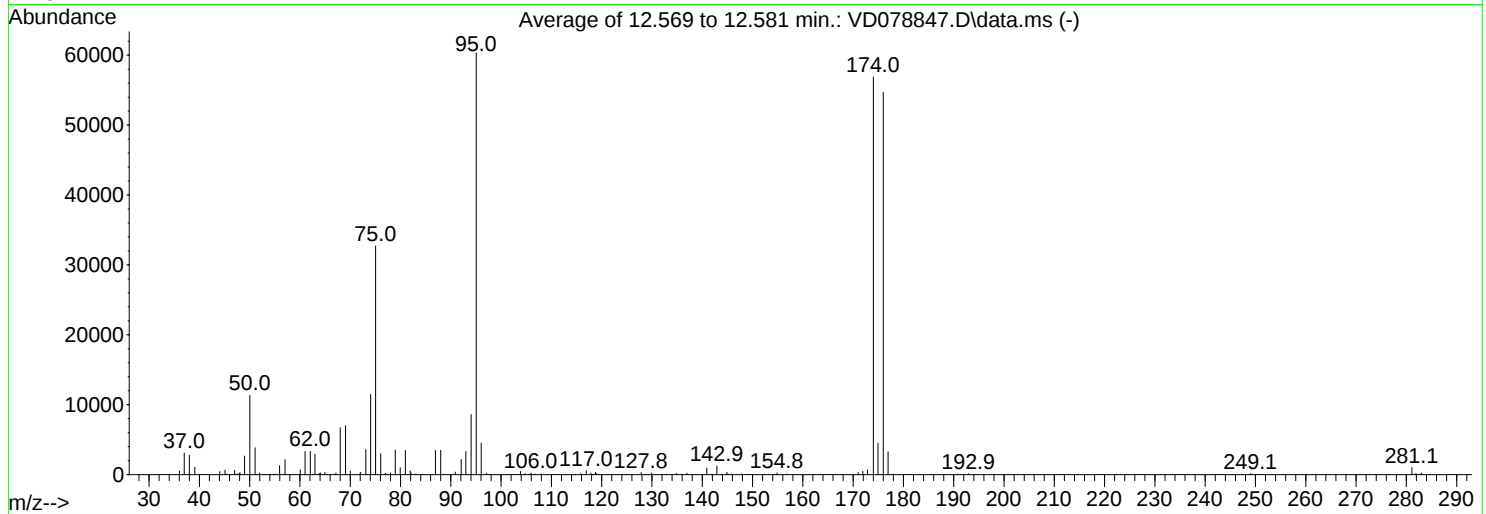


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD043024\
Data File : VD078847.D
Acq On : 30 Apr 2024 10:01
Operator : RP/MD
Sample : BFB211
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB211

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM041124SMA.M
Title : SFAM01.0
Last Update : Wed May 01 09:47:37 2024

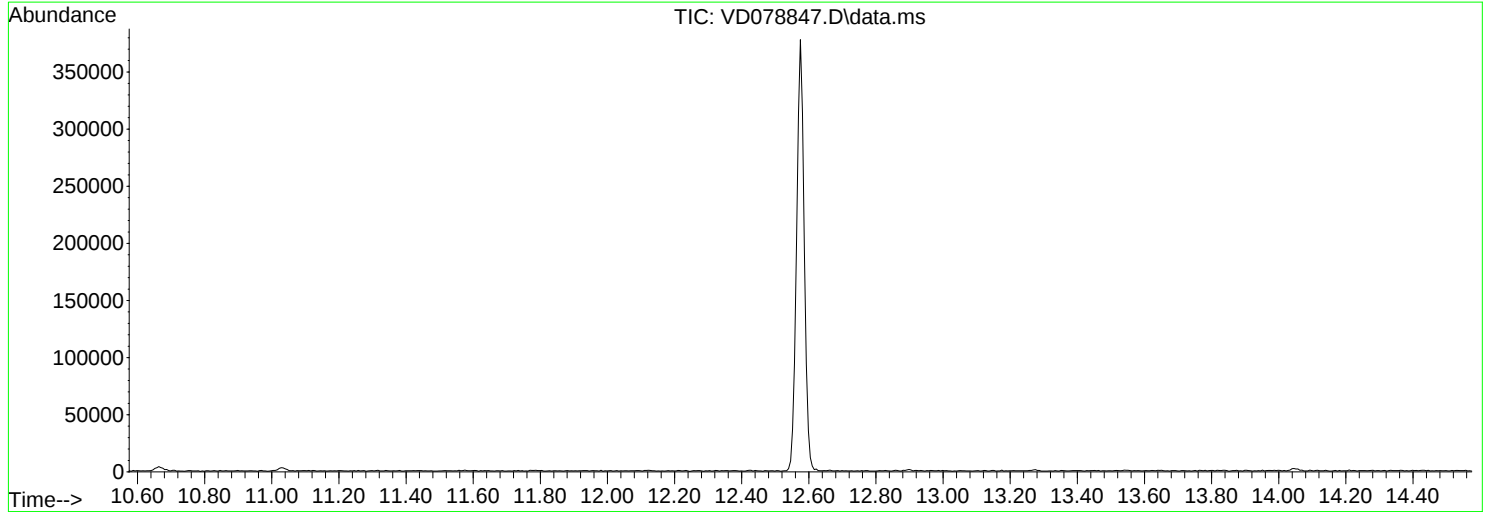

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.8	11336	PASS
75	95	30	80	54.2	32707	PASS
95	95	100	100	100.0	60333	PASS
96	95	5	9	7.5	4518	PASS
173	174	0.00	2	1.2	692	PASS
174	95	50	120	94.3	56864	PASS
175	174	5	9	7.9	4519	PASS
176	174	95	105	96.2	54685	PASS
177	176	5	10	6.0	3280	PASS

m/z	Abundance
40.00	621.0
44.10	425.0

Instrument :
MSVOA_D
ClientSampleId :
BFB211

m/z	Abundance
36.00	395.0
37.00	3001.0
38.00	2382.0
39.20	1084.0
40.00	713.0
44.00	872.0
45.10	549.0
47.00	445.0
47.90	552.0
49.00	2629.0
50.00	10808.0
51.10	3846.0
52.10	161.0
56.00	1316.0
57.00	1946.0
60.00	596.0
61.00	3090.0
62.00	2822.0
63.00	2650.0
63.80	182.0
64.10	193.0
65.00	354.0
66.10	162.0
67.20	191.0
68.00	6609.0
69.10	6768.0
70.10	563.0
71.90	324.0
73.10	3509.0
74.10	10150.0
75.00	30496.0
76.10	2505.0
77.00	255.0
78.10	378.0
79.00	3656.0
80.00	895.0
81.00	3209.0
81.90	876.0
87.00	3265.0
88.00	3574.0
90.90	457.0
92.10	2128.0
93.00	2910.0
94.00	8569.0
95.10	57400.0
96.00	5026.0
97.10	354.0
103.80	381.0
104.80	206.0
105.80	257.0
108.00	183.0
117.00	603.0
118.20	214.0
118.80	560.0
128.00	375.0
128.70	156.0
130.00	333.0
132.90	196.0
134.80	200.0
137.00	394.0
140.90	901.0
141.90	174.0
142.90	1390.0
143.90	199.0
144.90	653.0
154.90	308.0
171.10	370.0
171.90	266.0
172.90	540.0
174.00	52528.0
174.90	4007.0
176.00	48496.0
176.90	2909.0
178.00	163.0
190.80	268.0
281.10	766.0
283.10	159.0

Instrument :
MSVOA_D
ClientSampleId :
BFB211

m/z	Abundance
36.00	458.0
37.00	3662.0
38.00	2937.0
39.10	1100.0
40.10	620.0
44.10	876.0
45.10	667.0
47.00	774.0
47.50	257.0
48.10	460.0
49.00	3445.0
50.10	12210.0
51.10	4121.0
51.90	334.0
53.00	155.0
55.10	260.0
56.00	1471.0
57.00	2371.0
60.00	898.0
61.00	3552.0
62.10	3952.0
63.00	3069.0
64.10	548.0
64.90	300.0
67.10	249.0
68.00	7050.0
69.00	8149.0
69.90	654.0
72.10	575.0
73.10	4219.0
74.10	12937.0
75.10	36912.0
76.10	3628.0
77.10	330.0
77.90	351.0
78.90	4029.0
79.90	1205.0
81.00	3778.0
81.90	765.0
86.90	3399.0
88.00	3666.0
91.00	271.0
92.00	2146.0
93.00	3946.0
94.00	9361.0
95.00	68168.0
96.00	5007.0
97.10	218.0
103.90	627.0
104.70	212.0
106.00	364.0
106.80	173.0
107.90	193.0
112.90	204.0
115.90	225.0
116.90	526.0
117.90	248.0
119.00	495.0
124.90	216.0
127.80	278.0
129.80	338.0
140.80	919.0
142.90	1406.0
144.90	344.0
145.80	252.0
147.80	211.0
154.90	236.0
170.90	413.0
172.00	644.0
172.80	769.0
174.00	64368.0
174.90	4870.0
176.00	63944.0
177.00	3950.0
177.90	186.0
192.90	203.0
249.10	193.0
281.10	1228.0
281.90	248.0
283.00	264.0

Instrument :
MSVOA_D
ClientSampleId :
BFB211

m/z	Abundance
36.10	708.0
37.00	2633.0
38.00	3075.0
39.00	964.0
40.10	508.0
44.00	865.0
45.10	764.0
47.00	663.0
48.00	434.0
49.00	1904.0
50.10	10990.0
51.10	3600.0
52.00	242.0
54.00	153.0
54.80	150.0
55.90	1056.0
57.10	2130.0
60.10	550.0
61.00	3300.0
62.00	3207.0
63.00	2984.0
63.90	463.0
65.00	319.0
67.20	235.0
68.00	6436.0
69.00	6125.0
70.10	274.0
72.00	395.0
73.10	3023.0
74.00	11282.0
75.00	30712.0
76.00	2890.0
76.80	285.0
77.50	238.0
78.90	2797.0
79.90	860.0
80.90	3371.0
82.10	750.0
82.90	190.0
87.00	3730.0
88.00	3185.0
90.80	409.0
92.00	2219.0
93.00	3013.0
94.10	7871.0
95.00	55432.0
96.10	3522.0
103.90	376.0
105.90	358.0
114.80	164.0
115.80	286.0
116.90	543.0
117.80	450.0
118.80	497.0
127.80	273.0
134.90	331.0
136.90	255.0
141.00	1006.0
143.00	921.0
145.10	380.0
147.90	167.0
148.90	157.0
154.80	213.0
156.80	265.0
171.10	164.0
171.80	567.0
172.80	766.0
174.00	53696.0
175.00	4681.0
176.00	51616.0
177.00	2981.0
193.00	237.0
249.00	298.0
281.10	1028.0
281.90	302.0
282.90	286.0

Instrument :
MSVOA_D
ClientSampleId :
BFB211