
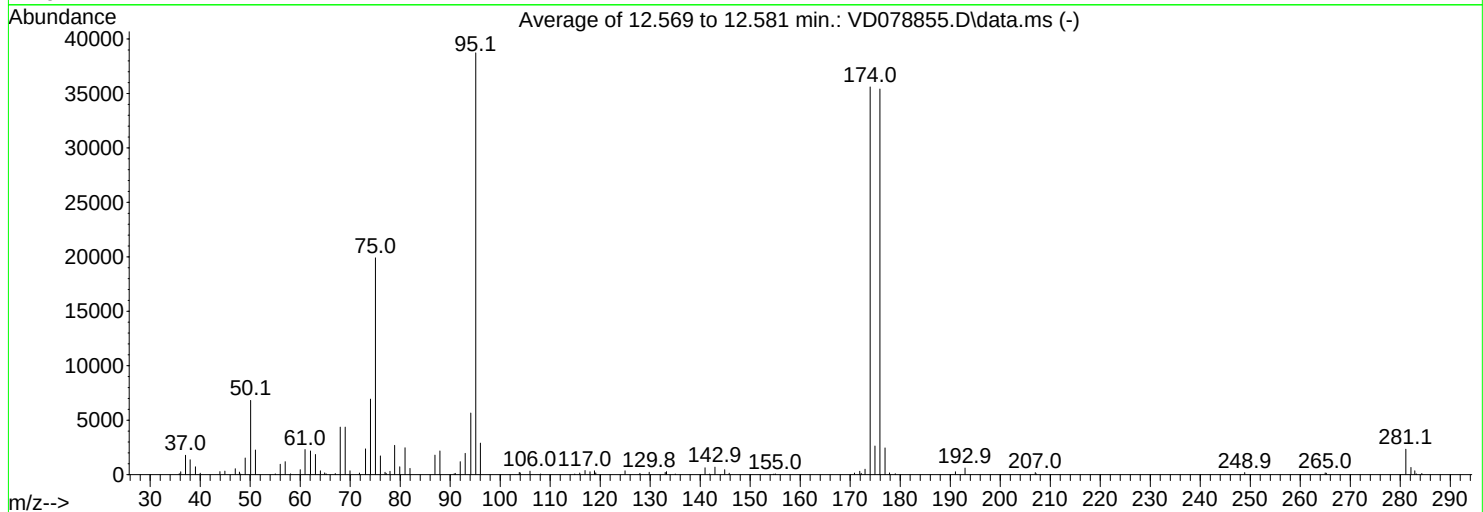


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050124\
Data File : VD078855.D
Acq On : 01 May 2024 10:54
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050124S.M
Title : SW846 8260
Last Update : Thu May 02 07:55:11 2024

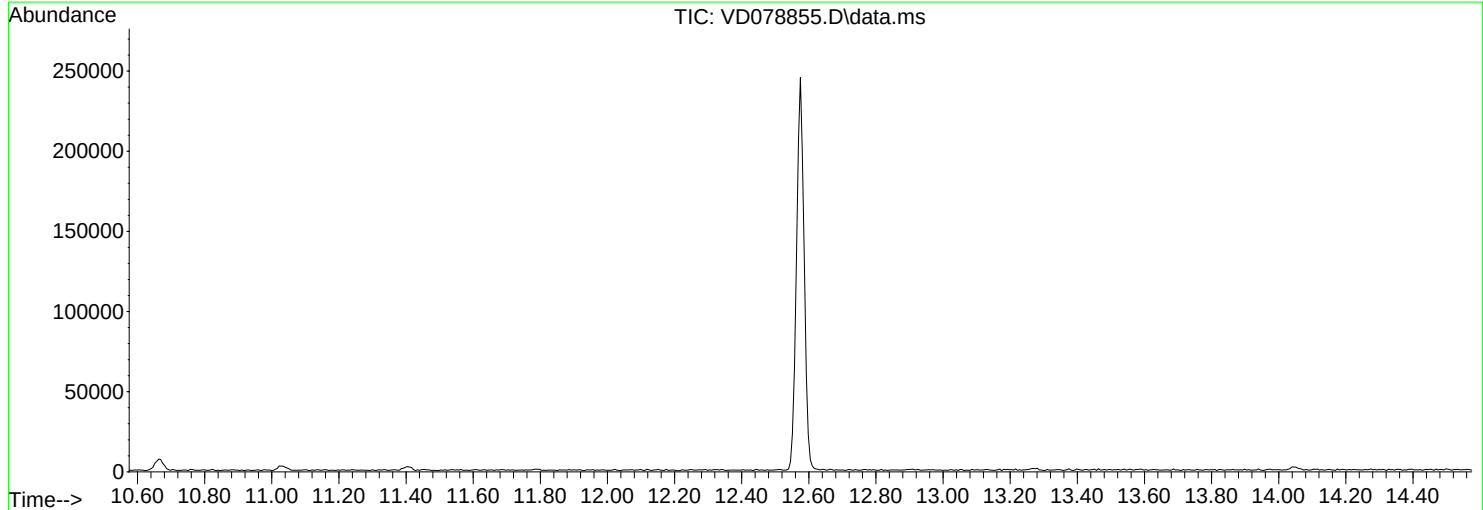

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.6	6822	PASS
75	95	30	60	51.4	19915	PASS
95	95	100	100	100.0	38731	PASS
96	95	5	9	7.5	2894	PASS
173	174	0.00	2	1.4	495	PASS
174	95	50	100	91.9	35595	PASS
175	174	5	9	7.4	2633	PASS
176	174	95	101	99.5	35411	PASS
177	176	5	9	6.9	2455	PASS