

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050422\
 Data File : VD072788.D
 Acq On : 04 May 2022 14:58
 Operator : VA/SY
 Sample : N2677-12
 Misc : 4.42G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SB-7,12

Quant Time: May 05 01:37:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050222S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 03 08:33:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.973	168	365258	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	720130	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	736262	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	338907	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	238807	50.367	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	100.740%
35) Dibromofluoromethane	7.908	113	232196	45.911	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	91.820%
50) Toluene-d8	10.332	98	918006	50.601	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	101.200%
62) 4-Bromofluorobenzene	12.620	95	359348	53.122	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	106.240%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050422\
Data File : VD072788.D
Acq On : 04 May 2022 14:58
Operator : VA/SY
Sample : N2677-12
Misc : 4.42G/5.00ml/MSVOA_D/SOIL
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SB-7,12

Quant Time: May 05 01:37:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050222S.M
Quant Title : SW846 8260
QLast Update : Tue May 03 08:33:49 2022
Response via : Initial Calibration

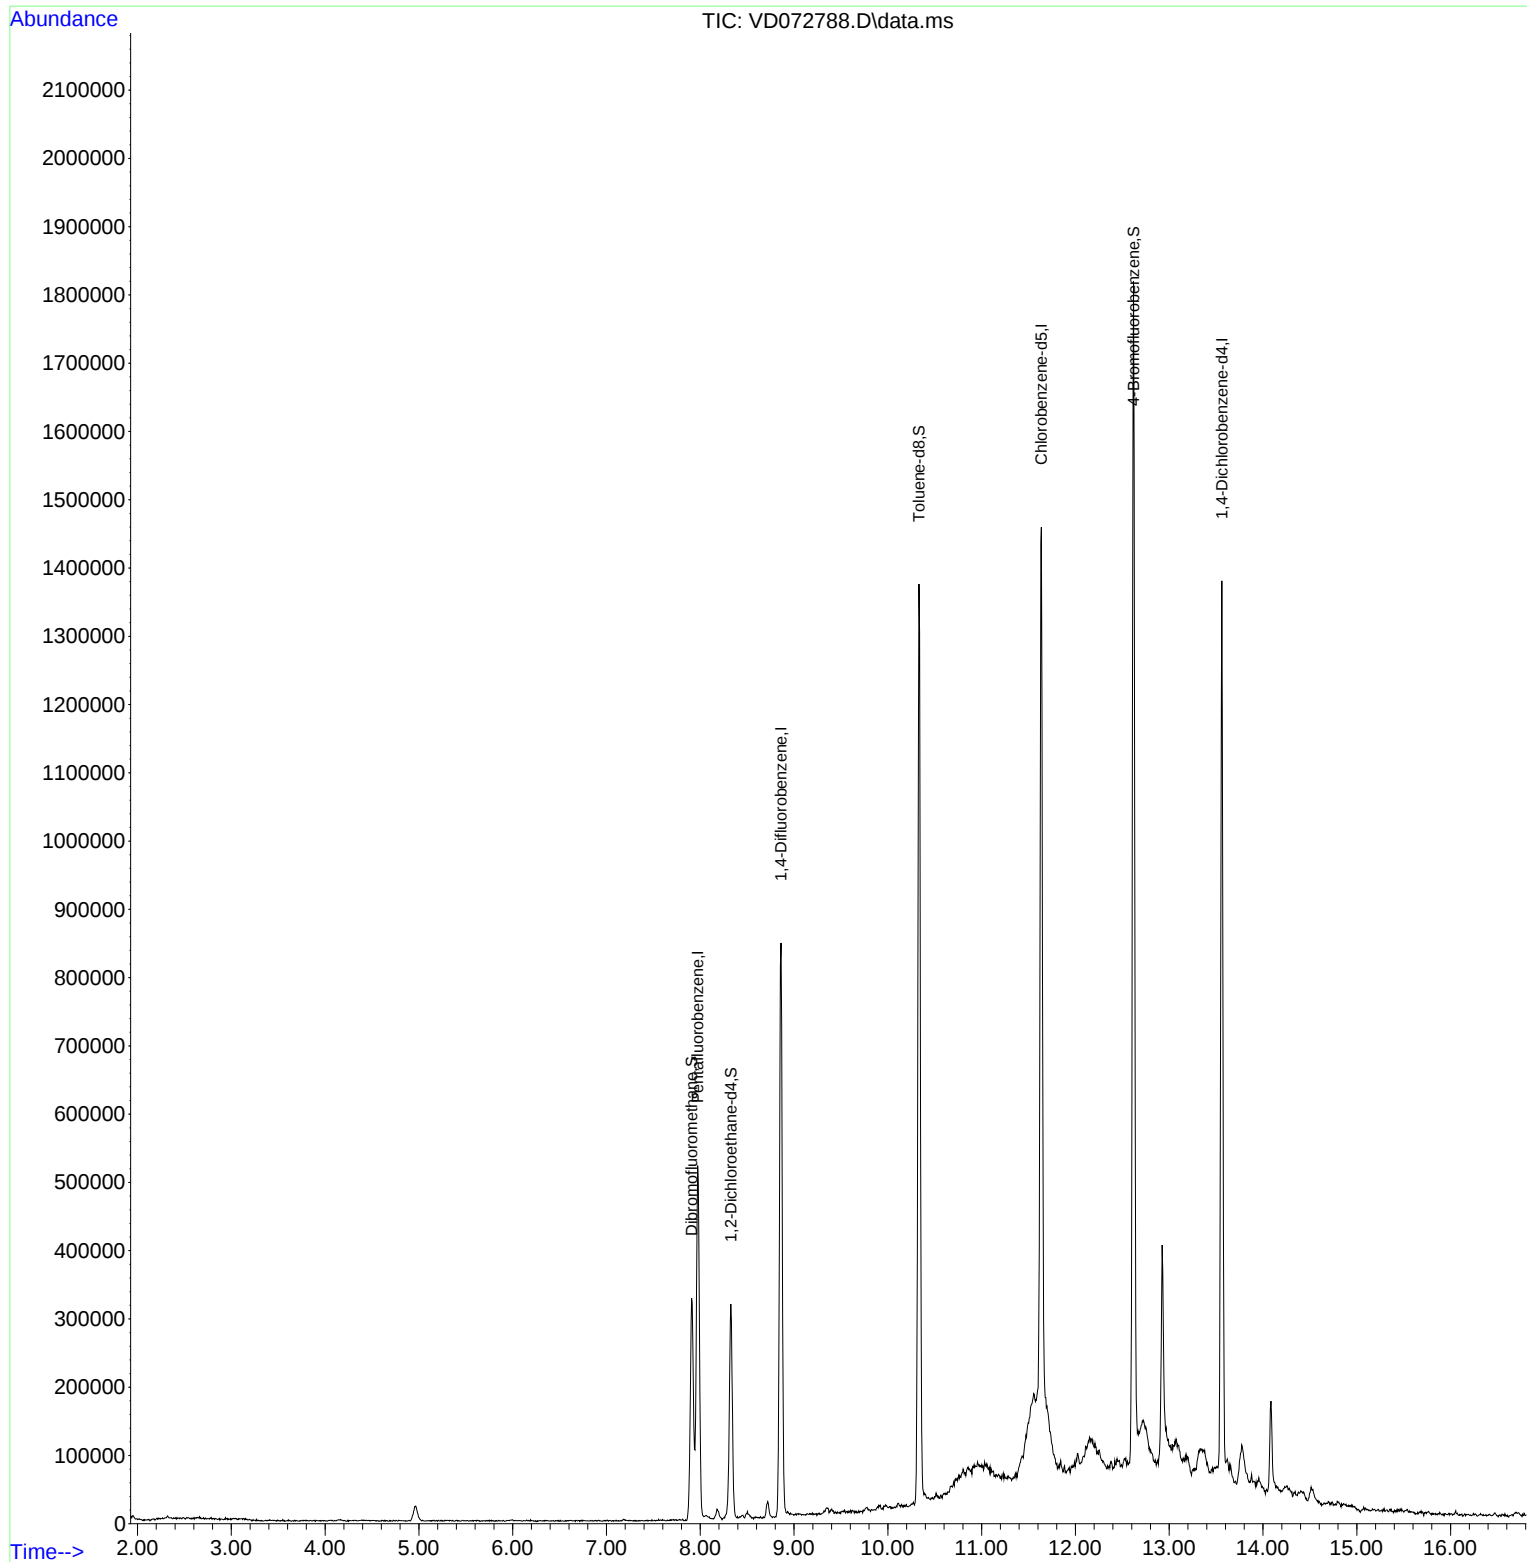



Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.973 min Scan# 1029

Delta R.T. -0.006 min

Lab File: VD072788.D

Acq: 04 May 2022 14:58

Instrument :

MSVOA_D

ClientSampleId :





SB-7,12

Tgt Ion:168 Resp: 365258

Ion Ratio Lower Upper

168 100

99 60.6 49.8 74.6

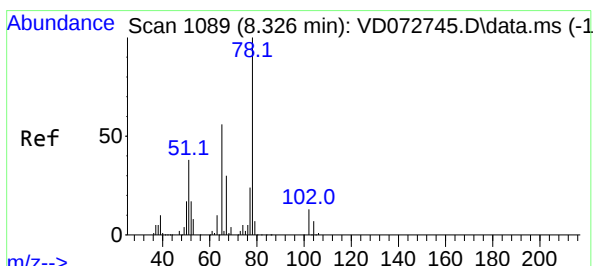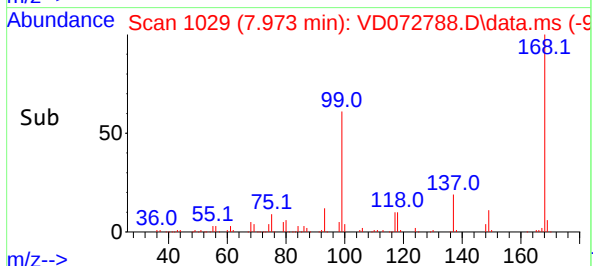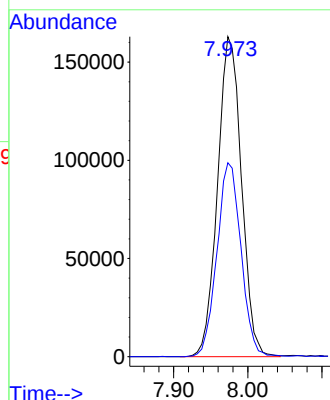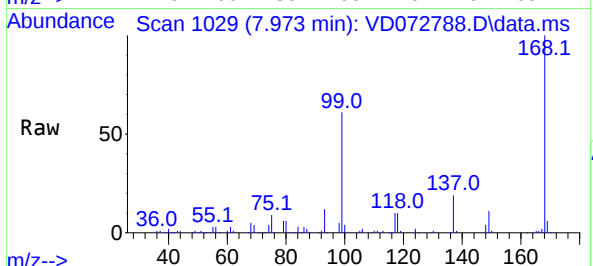

1,2-Dichloroethane-d4

Concen: 50.367 ug/l

RT: 8.326 min Scan# 1089

Delta R.T. 0.000 min

Lab File: VD072788.D




Acq: 04 May 2022 14:58


Tgt Ion: 65 Resp: 238807

Ion Ratio Lower Upper

65 100

67 53.6 0.0 101.4

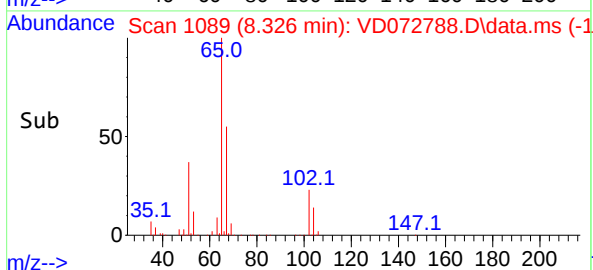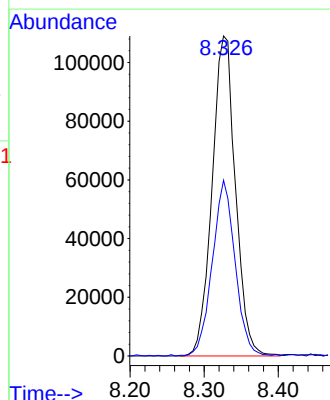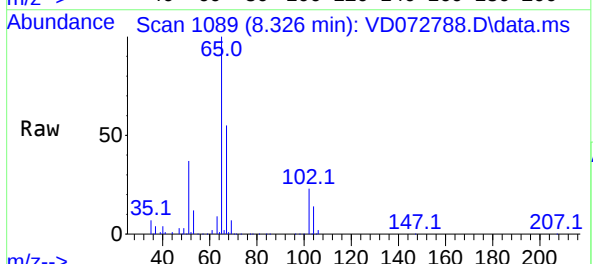



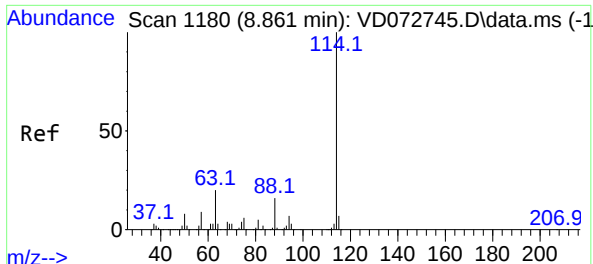


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.861 min Scan# 1180
Delta R.T. 0.000 min
Lab File: VD072788.D
Acq: 04 May 2022 14:58

Instrument :
MSVOA_D
ClientSampleId :
SB-7,12

Tgt Ion:114 Resp: 720130




Ion	Ratio	Lower	Upper
114	100		
63	21.4	0.0	46.6
88	15.9	0.0	33.2

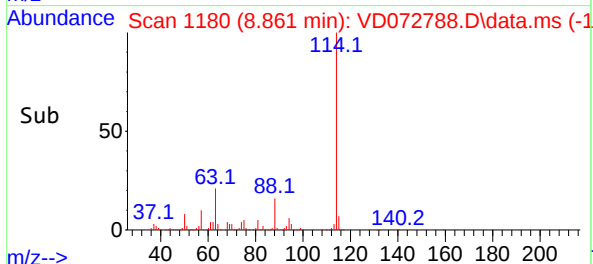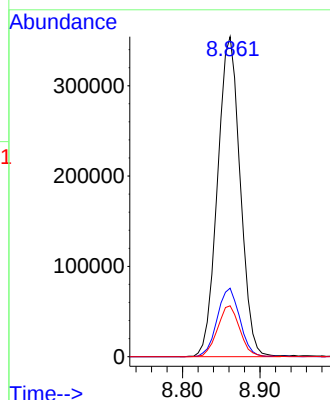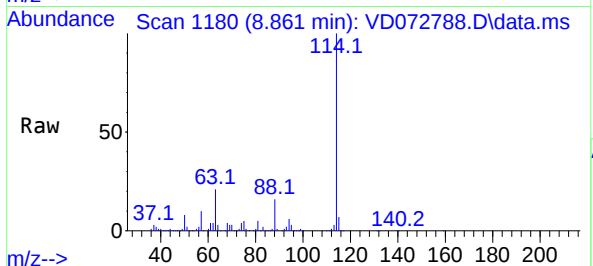


#35
Dibromofluoromethane
Concen: 45.911 ug/l
RT: 7.908 min Scan# 1018
Delta R.T. -0.001 min
Lab File: VD072788.D
Acq: 04 May 2022 14:58

Tgt Ion:113 Resp: 232196

Ion	Ratio	Lower	Upper
113	100		
111	104.7	83.8	125.6
192	17.7	14.6	21.8


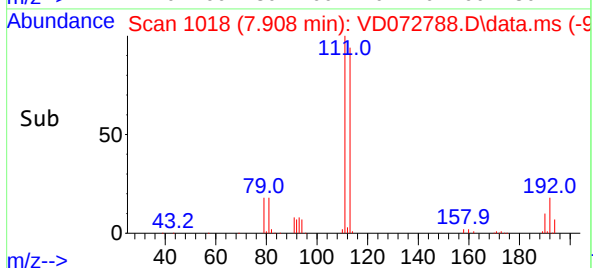
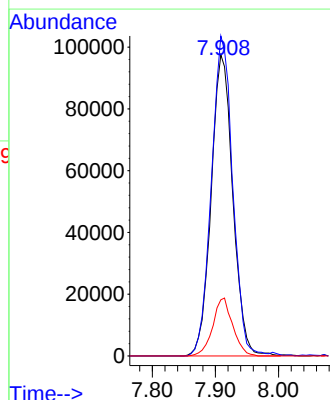
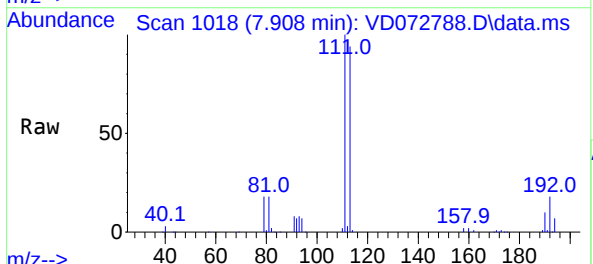


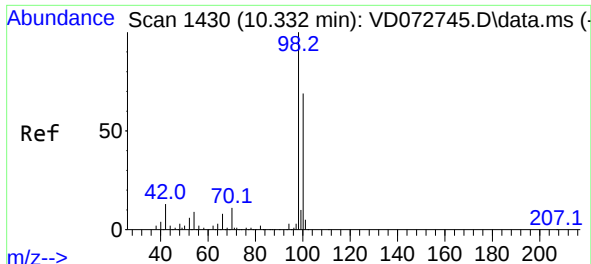

#50
Toluene-d8
Concen: 50.601 ug/l
RT: 10.332 min Scan# 1430
Delta R.T. -0.000 min
Lab File: VD072788.D
Acq: 04 May 2022 14:58




Instrument :
MSVOA_D
ClientSampleId :
SB-7,12


Tgt Ion: 98 Resp: 918006
Ion Ratio Lower Upper
98 100
100 65.7 52.4 78.6

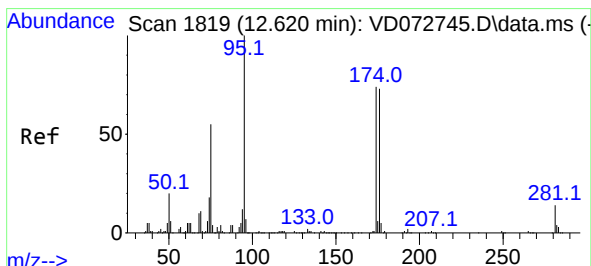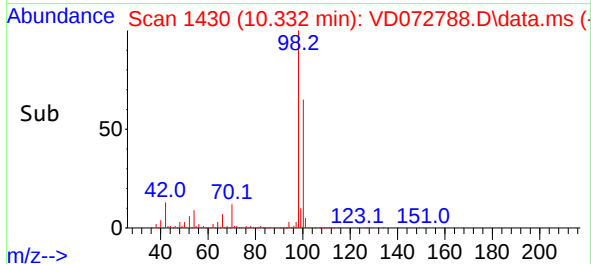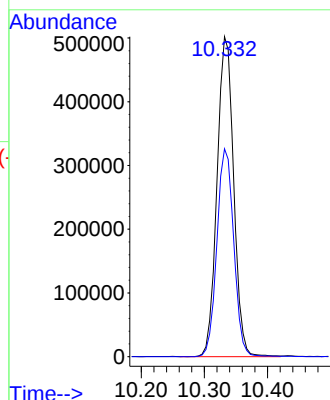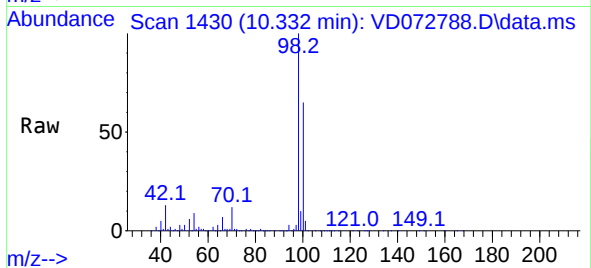

#62
4-Bromofluorobenzene
Concen: 53.122 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. -0.000 min
Lab File: VD072788.D
Acq: 04 May 2022 14:58

Tgt Ion: 95 Resp: 359348
Ion Ratio Lower Upper
95 100
174 71.8 0.0 152.8
176 70.2 0.0 145.4


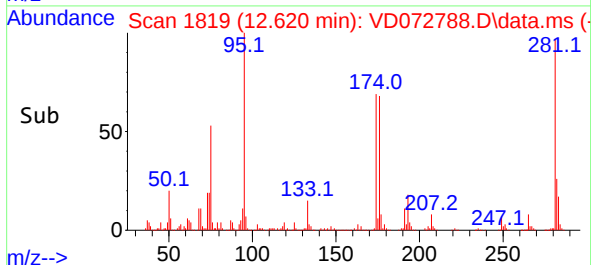
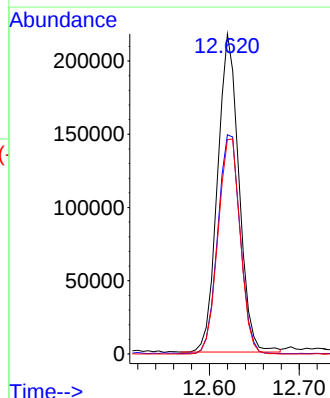
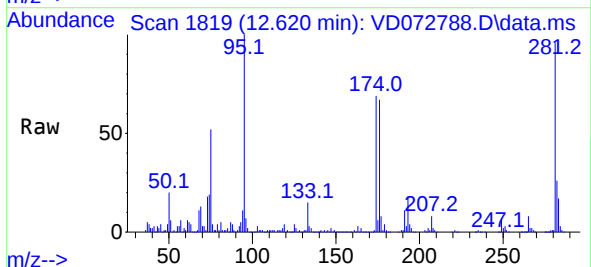


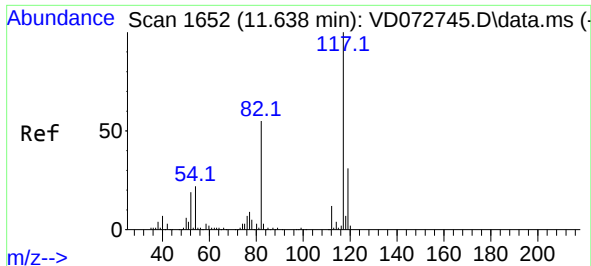

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 117
Delta R.T. -0.000 min
Lab File: VD072788.D
Acq: 04 May 2022 14:58

Instrument :
MSVOA_D
ClientSampleId :
SB-7,12

Tgt Ion:117 Resp: 736262
Ion Ratio Lower Upper
117 100
82 55.8 45.3 67.9
119 31.8 26.6 40.0

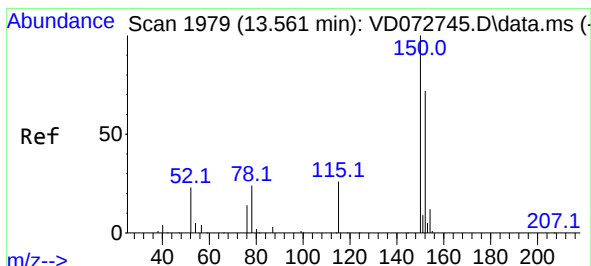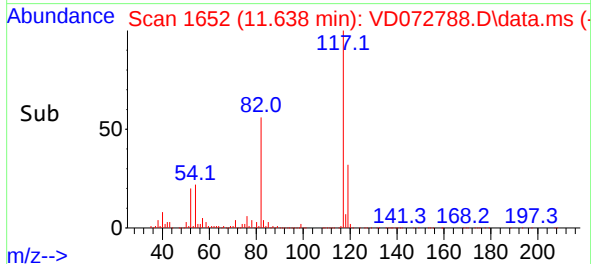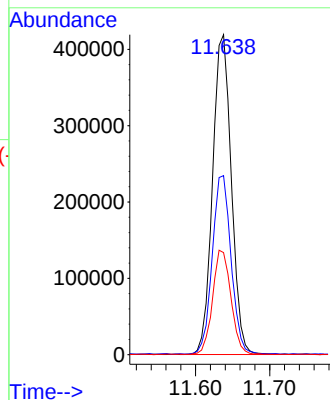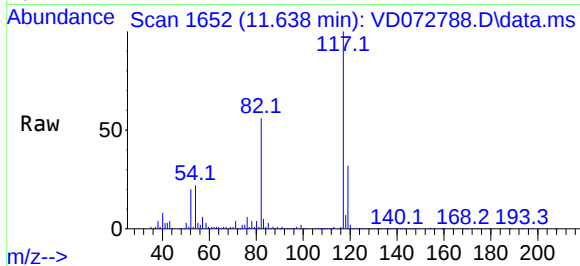

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. 0.000 min
Lab File: VD072788.D
Acq: 04 May 2022 14:58

Tgt Ion:152 Resp: 338907
Ion Ratio Lower Upper
152 100
115 60.8 31.3 93.8
150 154.3 0.0 348.6

