

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050625\
 Data File : VD080296.D
 Acq On : 06 May 2025 16:15
 Operator : RP/MD
 Sample : IBLK
 Misc : 5.00G/10ml/MSVOA_D/SOIL
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 IBLK

Quant Time: May 07 03:40:02 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050625S.M
 Quant Title : SW846 8260
 QLast Update : Wed May 07 03:36:54 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.876	168	152113	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.776	114	271303	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.582	117	238710	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.517	152	110960	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.235	65	89888	45.696	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	91.400%
35) Dibromofluoromethane	7.806	113	90621	49.836	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	99.680%
50) Toluene-d8	10.270	98	342054	47.742	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	=	95.480%
62) 4-Bromofluorobenzene	12.570	95	93856	40.814	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	=	81.620%
Target Compounds						
					Qvalue	
2) Dichlorodifluoromethane	1.935	85	687	Below Cal	#	56
3) Chloromethane	2.153	50	2260	Below Cal		94
13) Acrolein	3.794	56	446	2.124	ug/l #	14
16) Acetone	4.023	43	907	Below Cal		98
20) Methylene Chloride	4.800	84	3756	Below Cal	#	79
31) Cyclohexane	7.876	56	5180	1.621	ug/l #	38
49) 1,4-Dioxane	9.376	88	61	4.315	ug/l #	1
76) 1,2,3-Trichloropropane	12.570	75	50412	47.074	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.570	75	50412	89.354	ug/l #	14


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050625\
Data File : VD080296.D
Acq On : 06 May 2025 16:15
Operator : RP/MD
Sample : IBLK
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
IBLK

Quant Time: May 07 03:40:02 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050625S.M
Quant Title : SW846 8260
QLast Update : Wed May 07 03:36:54 2025
Response via : Initial Calibration

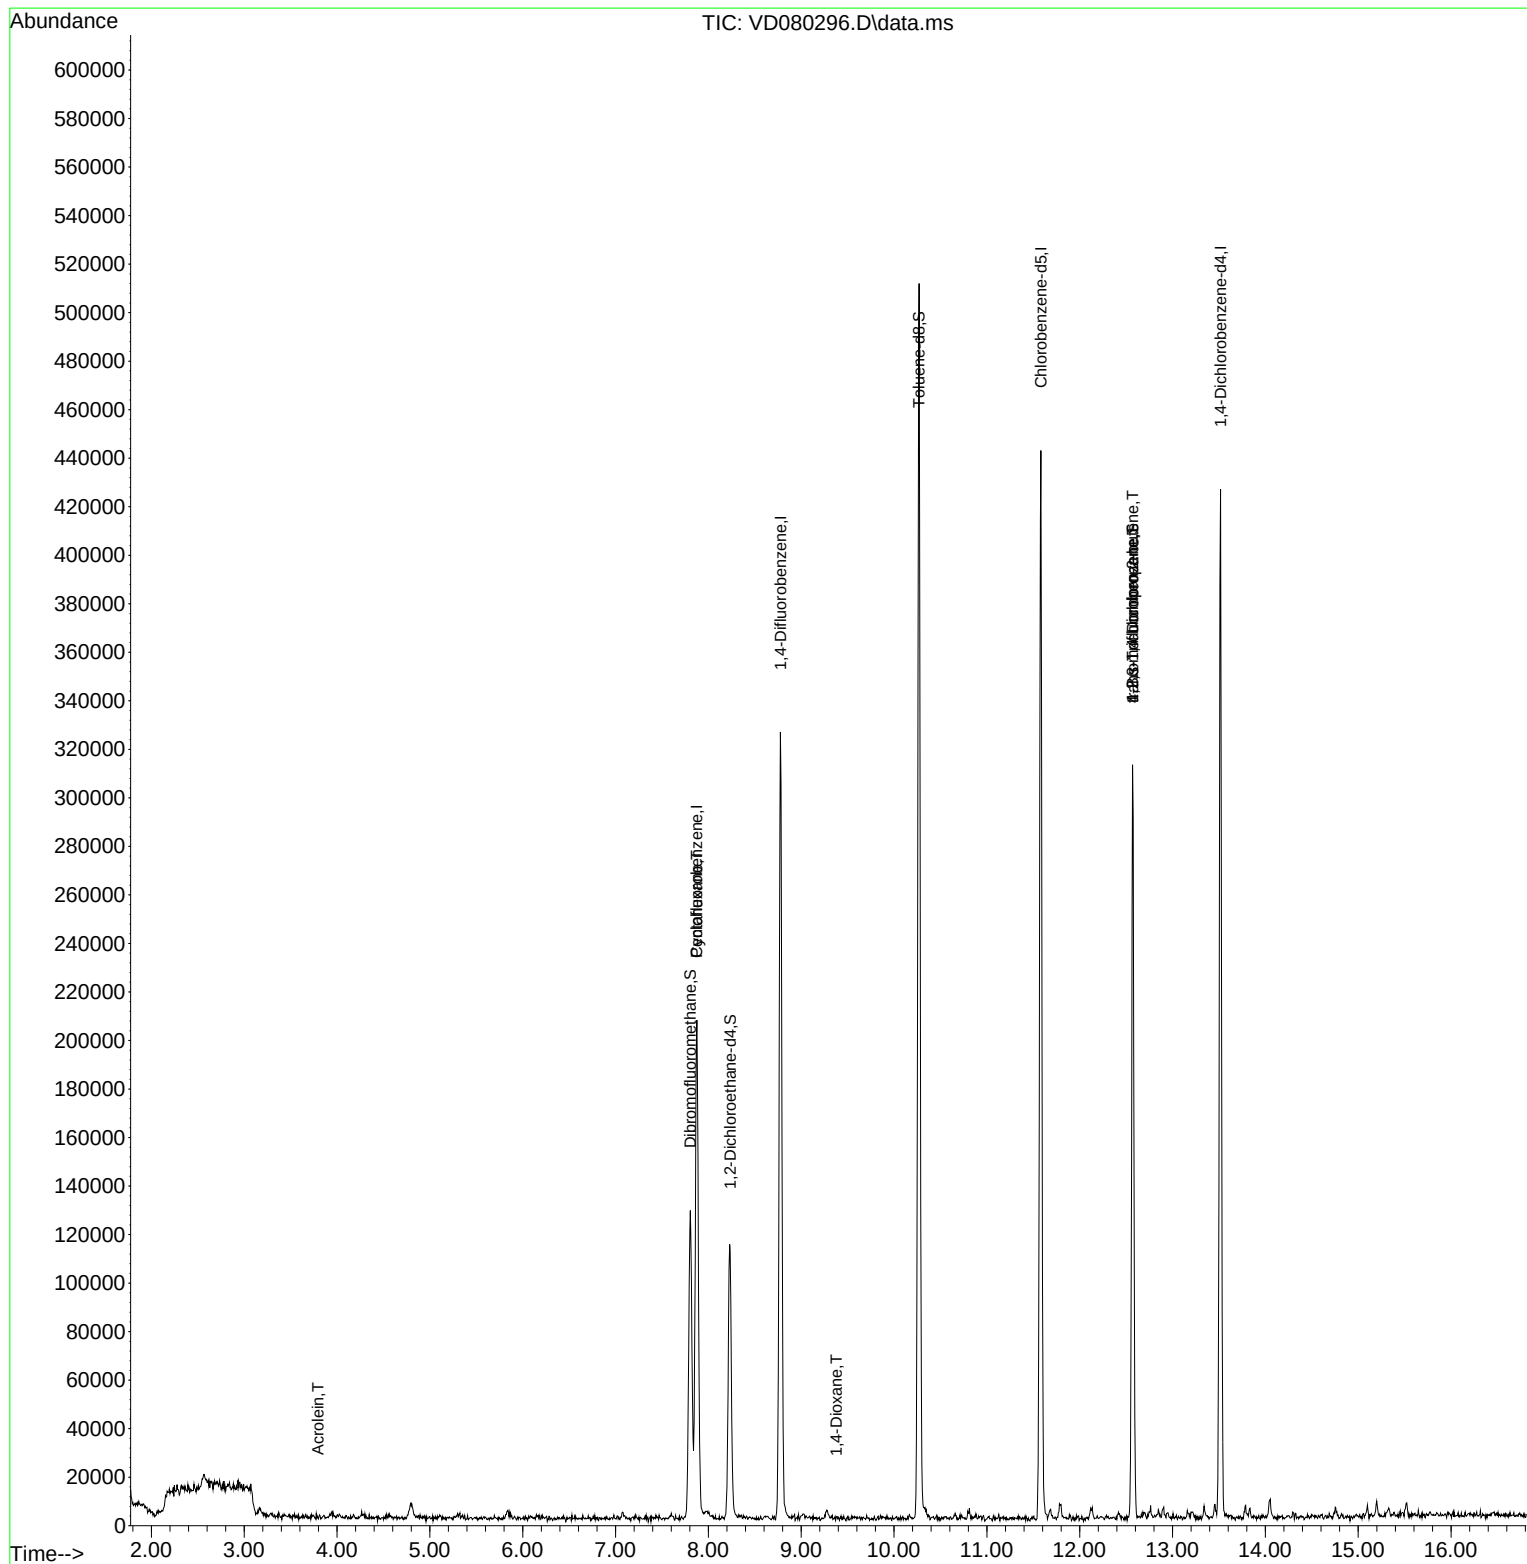

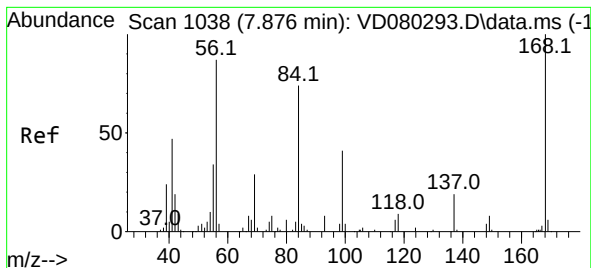

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.876 min Scan# 1038

Delta R.T. 0.000 min

Lab File: VD080296.D

Acq: 06 May 2025 16:15

Instrument :

MSVOA_D

ClientSampleId :





IBLK

Tgt Ion:168 Resp: 152113

Ion Ratio Lower Upper

168 100

99 53.4 46.4 69.6

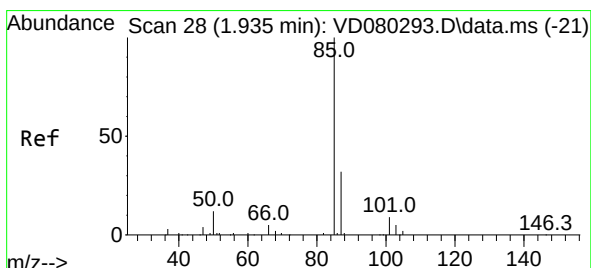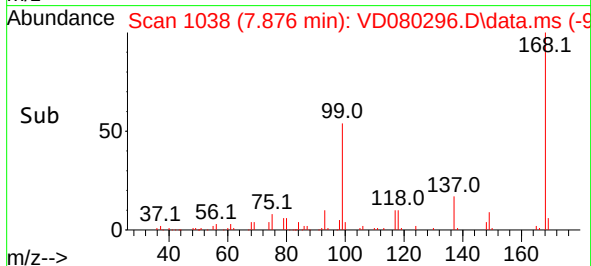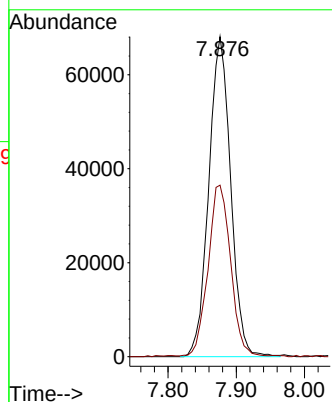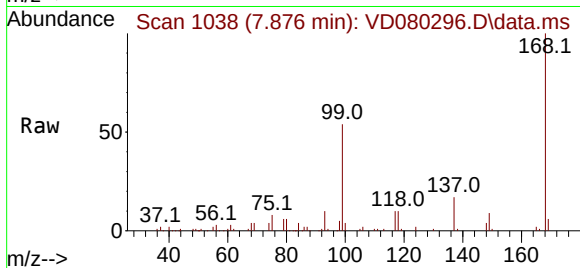

#2

Dichlorodifluoromethane

Concen: Below Cal

RT: 1.935 min Scan# 28

Delta R.T. 0.000 min

Lab File: VD080296.D




Acq: 06 May 2025 16:15


Tgt Ion: 85 Resp: 687

Ion Ratio Lower Upper

85 100

87 56.9 16.2 48.6#


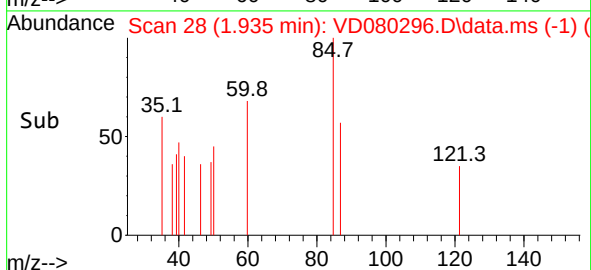
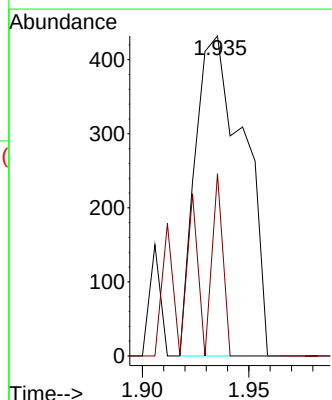
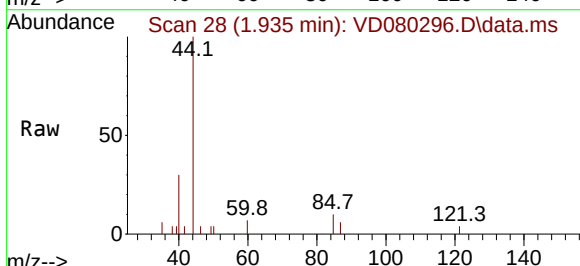


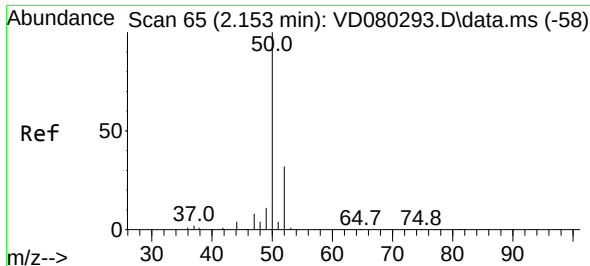

#3
Chloromethane
Concen: Below Cal
RT: 2.153 min Scan# 61
Delta R.T. -0.000 min
Lab File: VD080296.D
Acq: 06 May 2025 16:15




Instrument :
MSVOA_D
ClientSampleId :
IBLK


Tgt Ion: 50 Resp: 2260
Ion Ratio Lower Upper
50 100
52 29.0 25.7 38.5

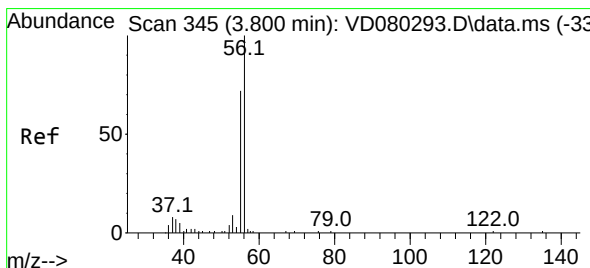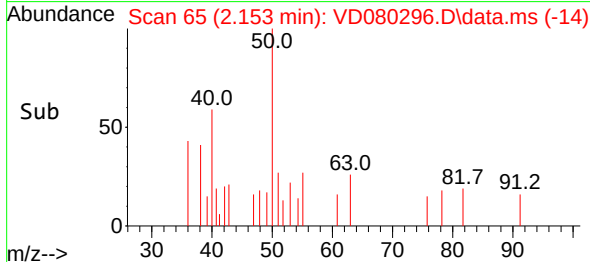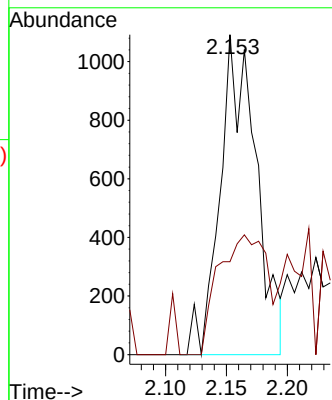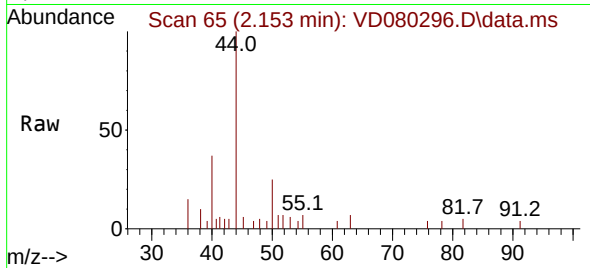

#13
Acrolein
Concen: 2.124 ug/l
RT: 3.794 min Scan# 344
Delta R.T. -0.006 min
Lab File: VD080296.D
Acq: 06 May 2025 16:15

Tgt Ion: 56 Resp: 446
Ion Ratio Lower Upper
56 100
55 0.0 57.4 86.2#


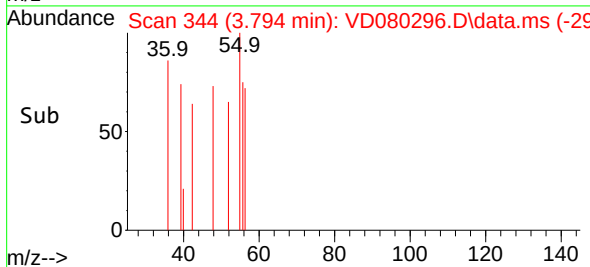
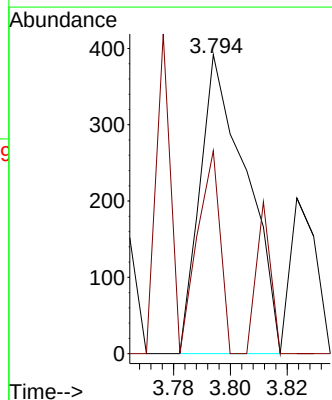
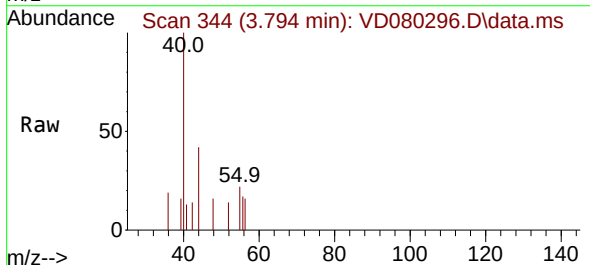


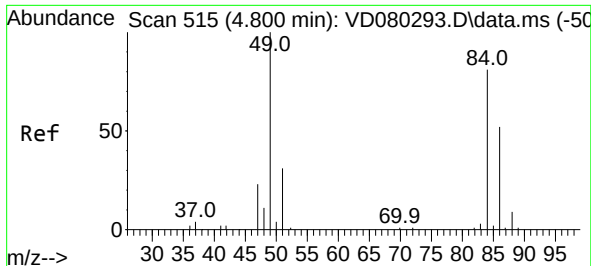

#20
Methylene Chloride
Concen: Below Cal
RT: 4.800 min Scan# 515
Delta R.T. -0.000 min
Lab File: VD080296.D
Acq: 06 May 2025 16:15




Instrument :
MSVOA_D
ClientSampleId :
IBLK


Tgt Ion:	84	Resp:	3756
Ion	Ratio	Lower	Upper
84	100		
49	99.8	98.7	148.1
51	16.4	30.8	46.2#
86	54.0	51.4	77.0

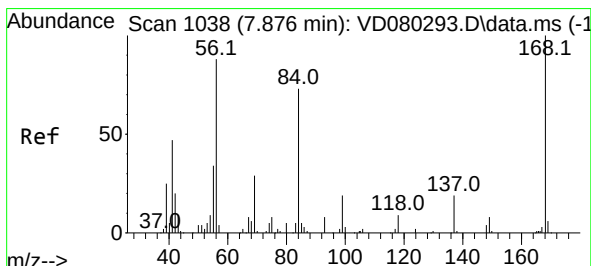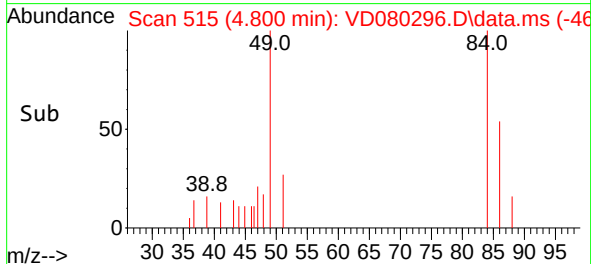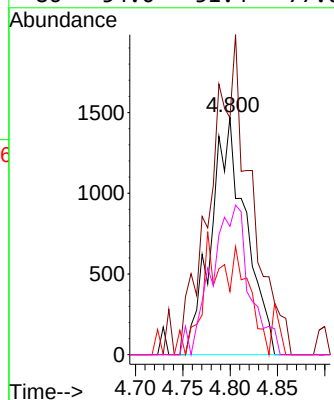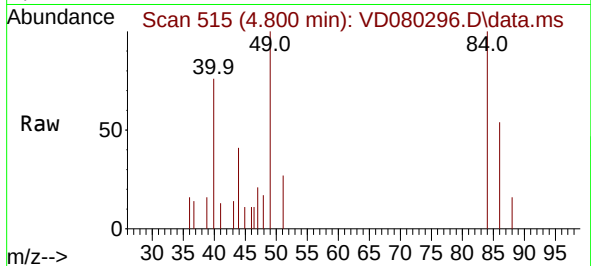

#31
Cyclohexane
Concen: 1.621 ug/l
RT: 7.876 min Scan# 1038
Delta R.T. -0.000 min
Lab File: VD080296.D
Acq: 06 May 2025 16:15

Tgt Ion:	56	Resp:	5180
Ion	Ratio	Lower	Upper
56	100		
69	107.2	26.1	39.1#
84	114.4	66.5	99.7#

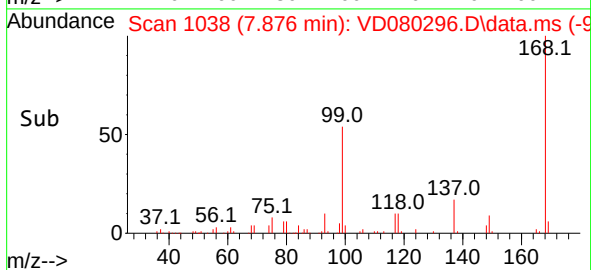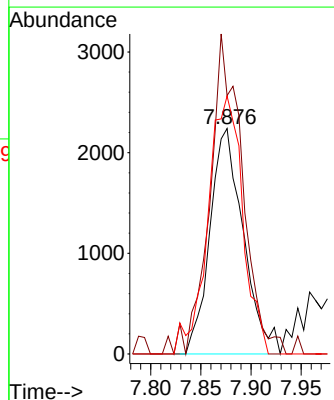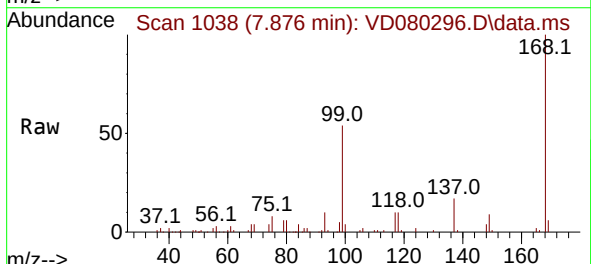

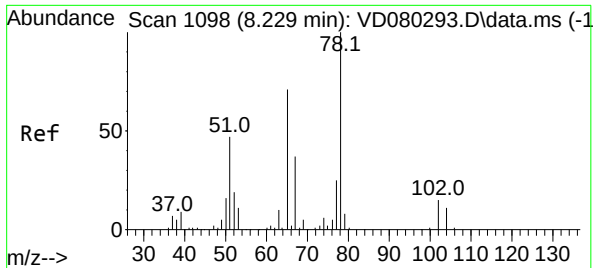

#33

1,2-Dichloroethane-d4

Concen: 45.696 ug/l

RT: 8.235 min Scan# 1098

Delta R.T. 0.006 min

Lab File: VD080296.D

Acq: 06 May 2025 16:15

Instrument :

MSVOA_D

ClientSampleId :





IBLK

Tgt Ion: 65 Resp: 89888

Ion Ratio Lower Upper

65 100

67 53.8 0.0 107.6

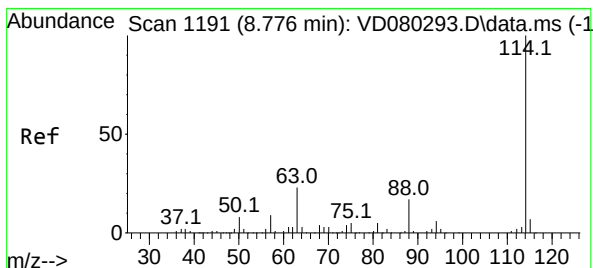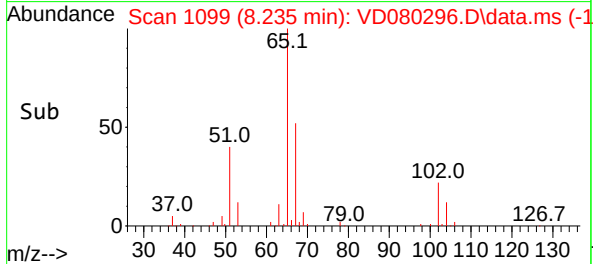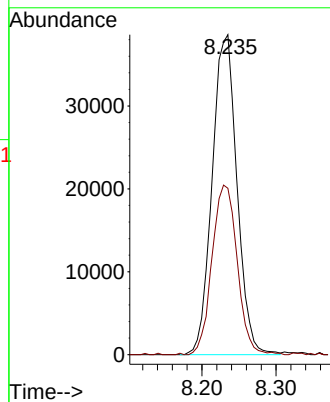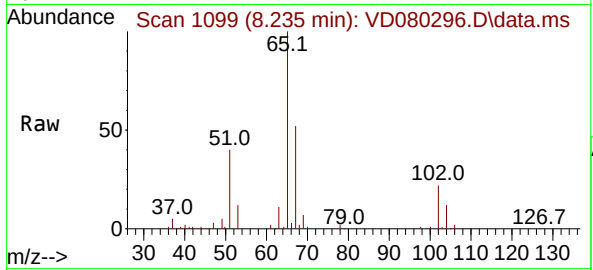

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.776 min Scan# 1191

Delta R.T. -0.000 min

Lab File: VD080296.D

Acq: 06 May 2025 16:15




Tgt Ion: 114 Resp: 271303


Ion Ratio Lower Upper

114 100

63 21.8 0.0 45.6

88 15.8 0.0 33.2

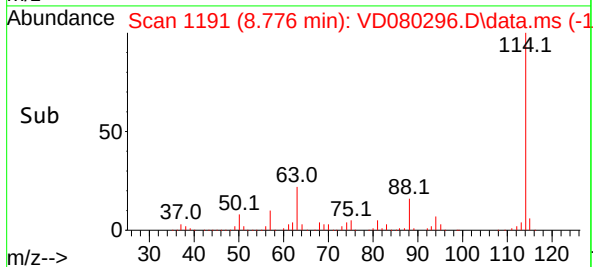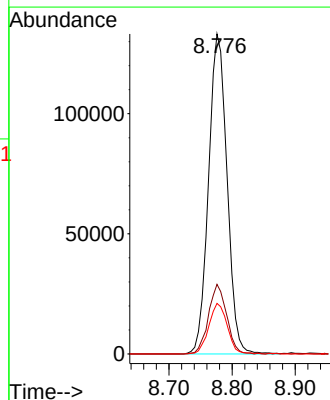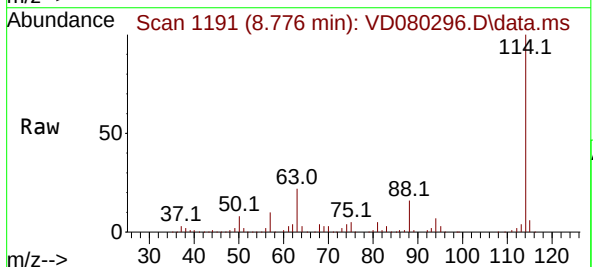

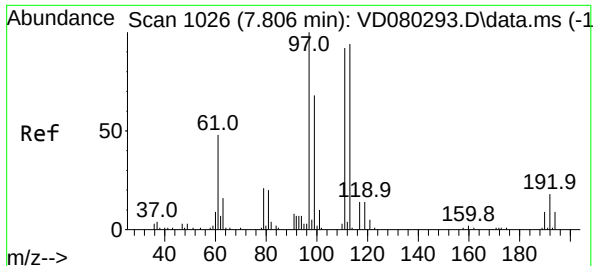

#35

Dibromofluoromethane

Concen: 49.836 ug/l

RT: 7.806 min Scan# 1026

Delta R.T. -0.000 min

Lab File: VD080296.D

Acq: 06 May 2025 16:15

Instrument :

MSVOA_D

ClientSampleId :

IBLK





Tgt Ion:113 Resp: 90621

Ion Ratio Lower Upper

113 100

111 103.3 80.7 121.1

192 19.4 15.7 23.5

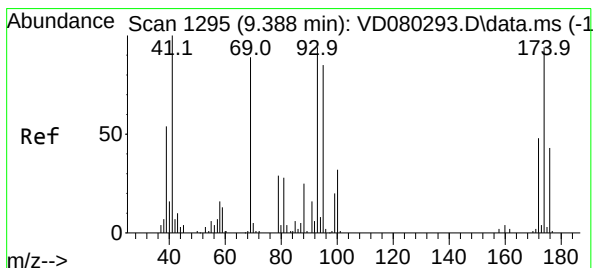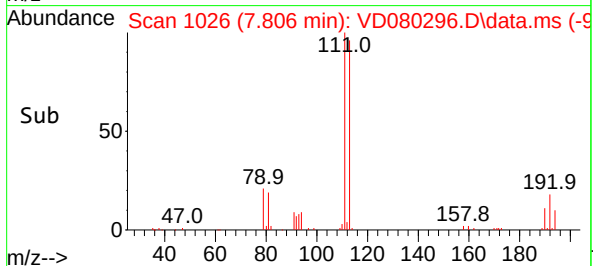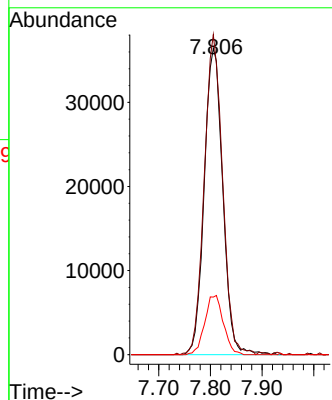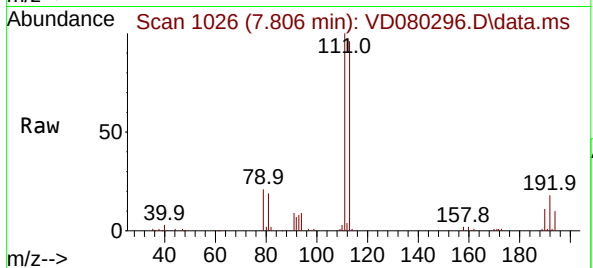

#49

1,4-Dioxane

Concen: 4.315 ug/l

RT: 9.376 min Scan# 1293

Delta R.T. -0.012 min

Lab File: VD080296.D

Acq: 06 May 2025 16:15




Tgt Ion: 88 Resp: 61


Ion Ratio Lower Upper

88 100

43 306.6 31.4 47.2#

58 0.0 61.8 92.6#


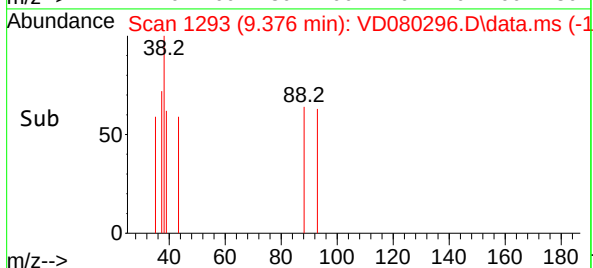
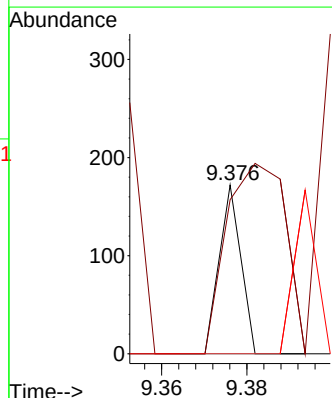
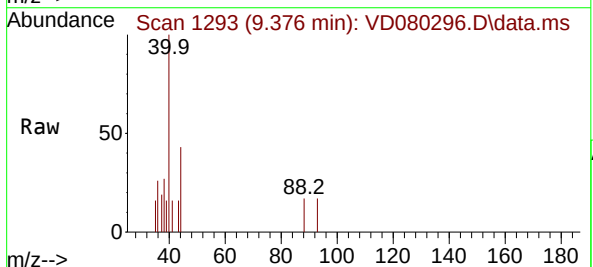


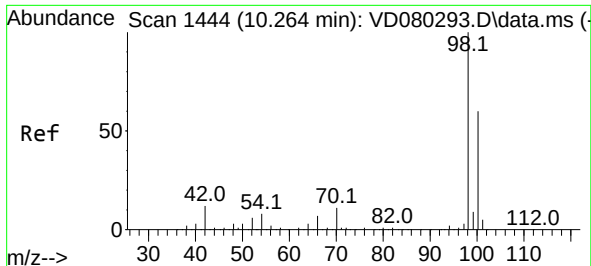

#50
Toluene-d8
Concen: 47.742 ug/l
RT: 10.270 min Scan# 1444
Delta R.T. 0.006 min
Lab File: VD080296.D
Acq: 06 May 2025 16:15




Instrument :
MSVOA_D
ClientSampleId :
IBLK


Tgt Ion: 98 Resp: 342054
Ion Ratio Lower Upper
98 100
100 61.5 50.0 75.0

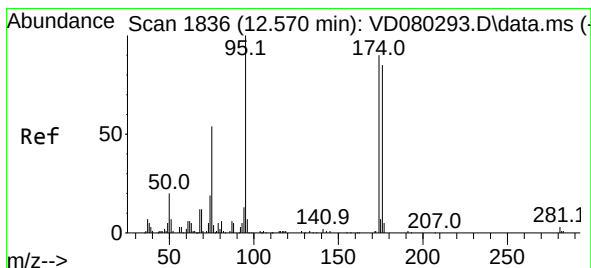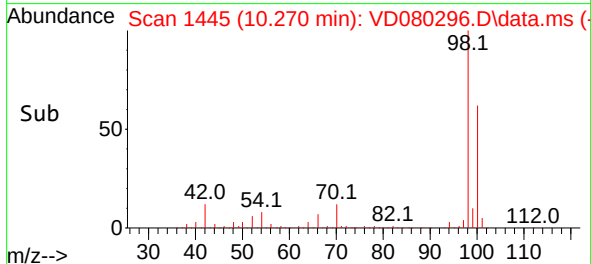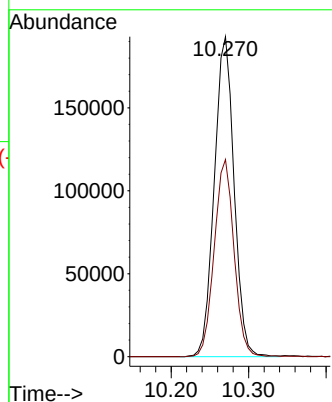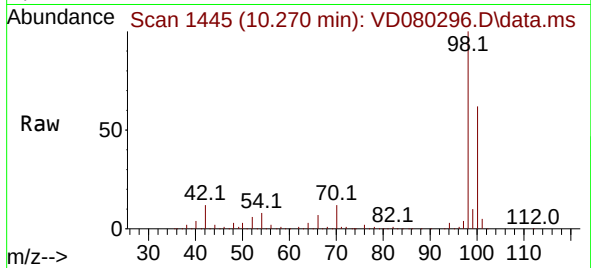

#62
4-Bromofluorobenzene
Concen: 40.814 ug/l
RT: 12.570 min Scan# 1836
Delta R.T. -0.000 min
Lab File: VD080296.D
Acq: 06 May 2025 16:15

Tgt Ion: 95 Resp: 93856
Ion Ratio Lower Upper
95 100
174 89.8 0.0 170.0
176 83.7 0.0 167.8


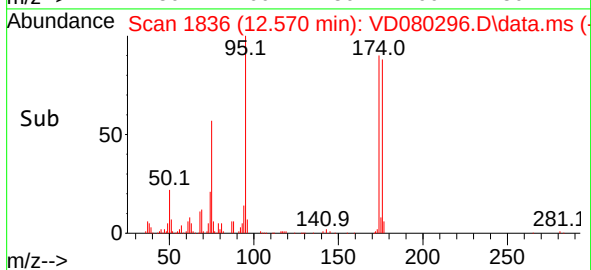
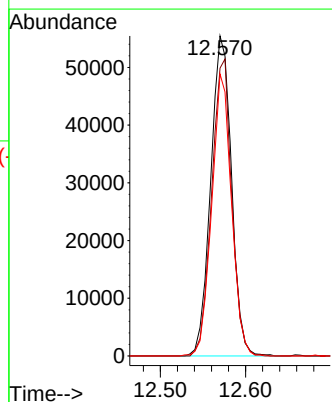
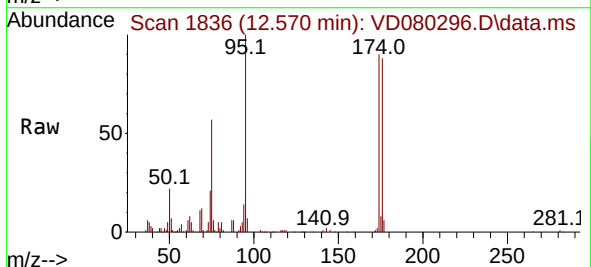


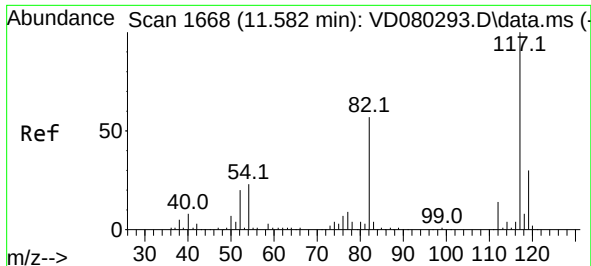

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.582 min Scan# 11
Delta R.T. -0.000 min
Lab File: VD080296.D
Acq: 06 May 2025 16:15




Instrument :
MSVOA_D
ClientSampleId :
IBLK


Tgt Ion:117 Resp: 238710
Ion Ratio Lower Upper
117 100
82 55.8 45.5 68.3
119 31.2 24.0 36.0

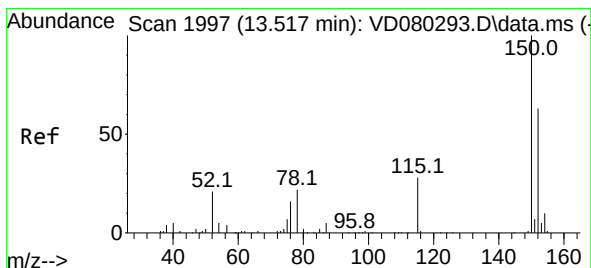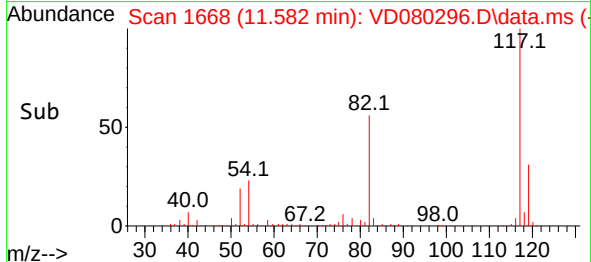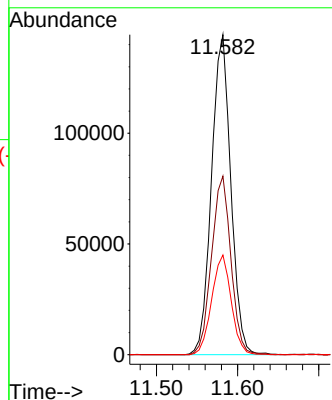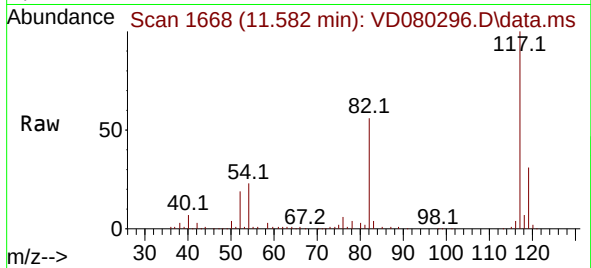

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.517 min Scan# 1997
Delta R.T. -0.000 min
Lab File: VD080296.D
Acq: 06 May 2025 16:15

Tgt Ion:152 Resp: 110960
Ion Ratio Lower Upper
152 100
115 57.6 29.0 87.1
150 155.6 0.0 354.6


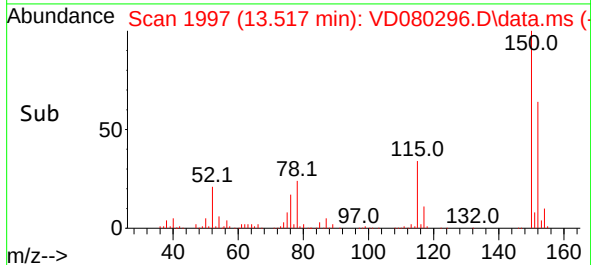
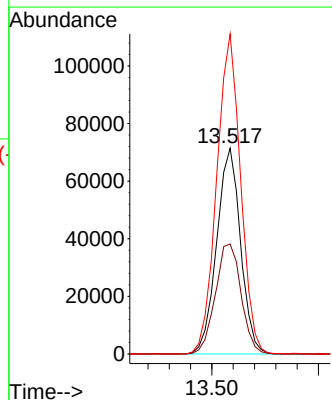
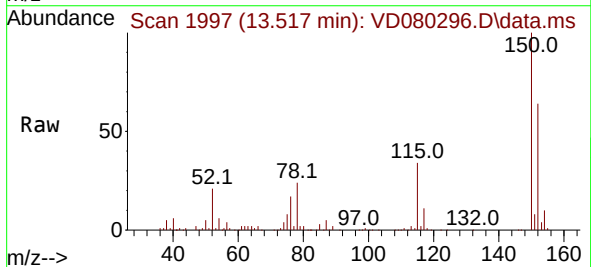


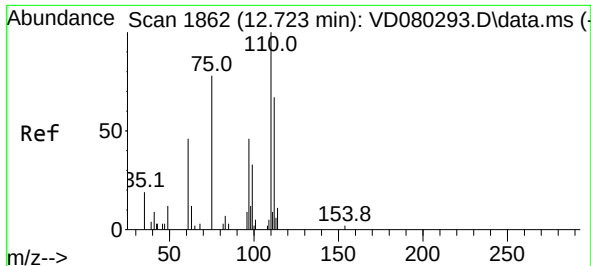

#76
1,2,3-Trichloropropane
Concen: 47.074 ug/l
RT: 12.570 min Scan# 1836
Delta R.T. -0.153 min
Lab File: VD080296.D
Acq: 06 May 2025 16:15

Instrument :
MSVOA_D
ClientSampleId :
IBLK

Tgt Ion: 75 Resp: 50412
Ion Ratio Lower Upper
75 100
77 1.5 0.0 0.0#

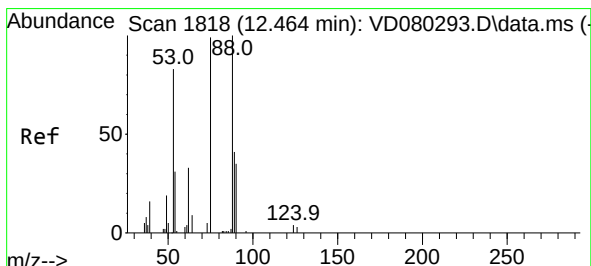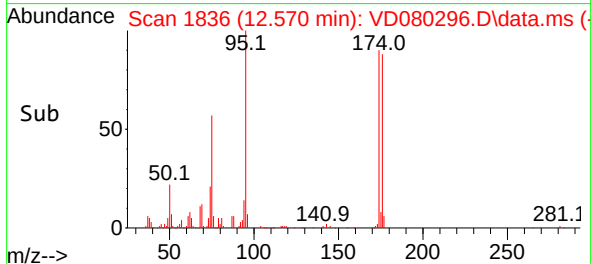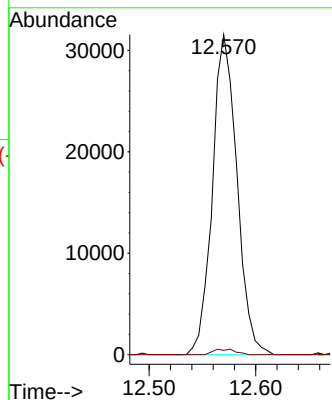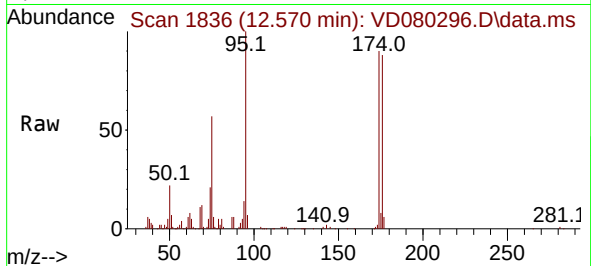

#81
trans-1,4-Dichloro-2-butene
Concen: 89.354 ug/l
RT: 12.570 min Scan# 1836
Delta R.T. 0.106 min
Lab File: VD080296.D
Acq: 06 May 2025 16:15

Tgt Ion: 75 Resp: 50412
Ion Ratio Lower Upper
75 100
53 0.1 70.8 106.2#
89 0.0 35.9 53.9#

