
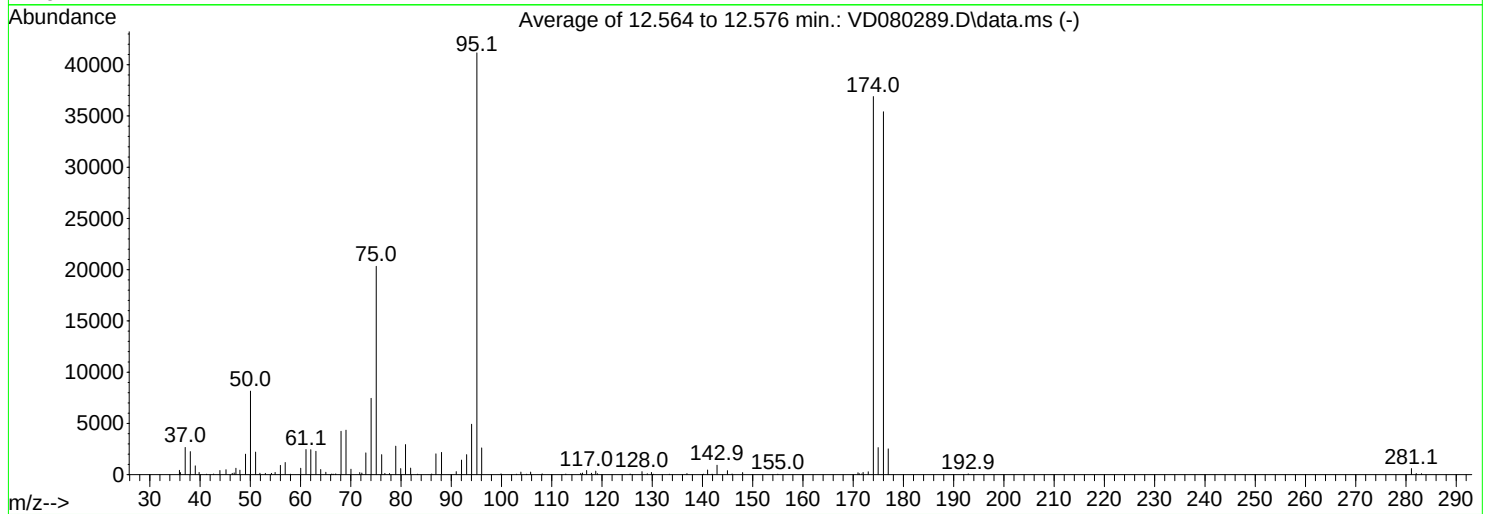


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050625\
Data File : VD080289.D
Acq On : 06 May 2025 09:57
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050625S.M
Title : SW846 8260
Last Update : Wed May 07 08:57:11 2025

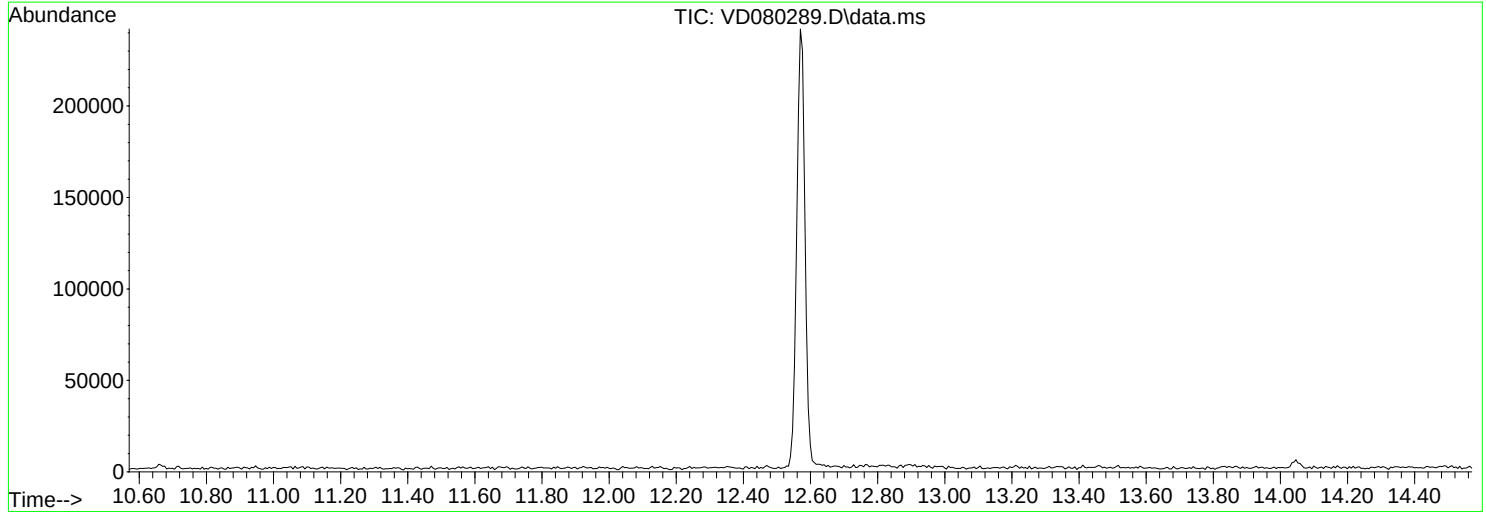

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.8	8144	PASS
75	95	30	60	49.4	20333	PASS
95	95	100	100	100.0	41160	PASS
96	95	5	9	6.3	2612	PASS
173	174	0.00	2	0.8	289	PASS
174	95	50	100	89.6	36896	PASS
175	174	5	9	7.2	2640	PASS
176	174	95	101	96.0	35413	PASS
177	176	5	9	7.1	2518	PASS