
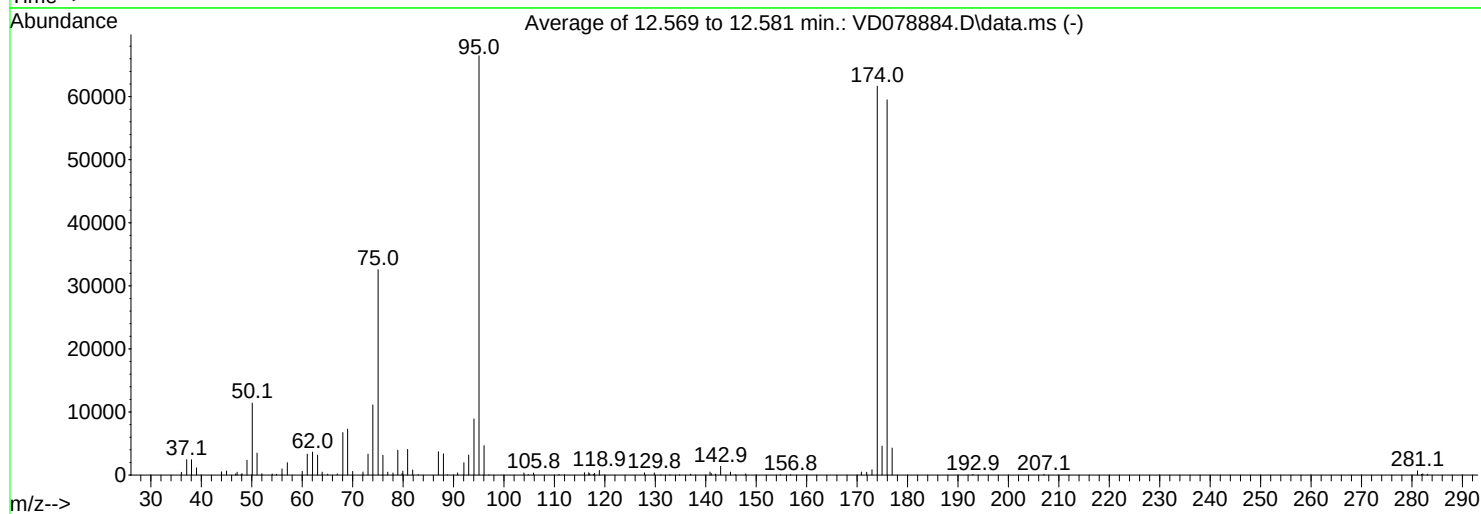


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD050824\
Data File : VD078884.D
Acq On : 08 May 2024 10:08
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050124S.M
Title : SW846 8260
Last Update : Wed May 08 19:40:18 2024

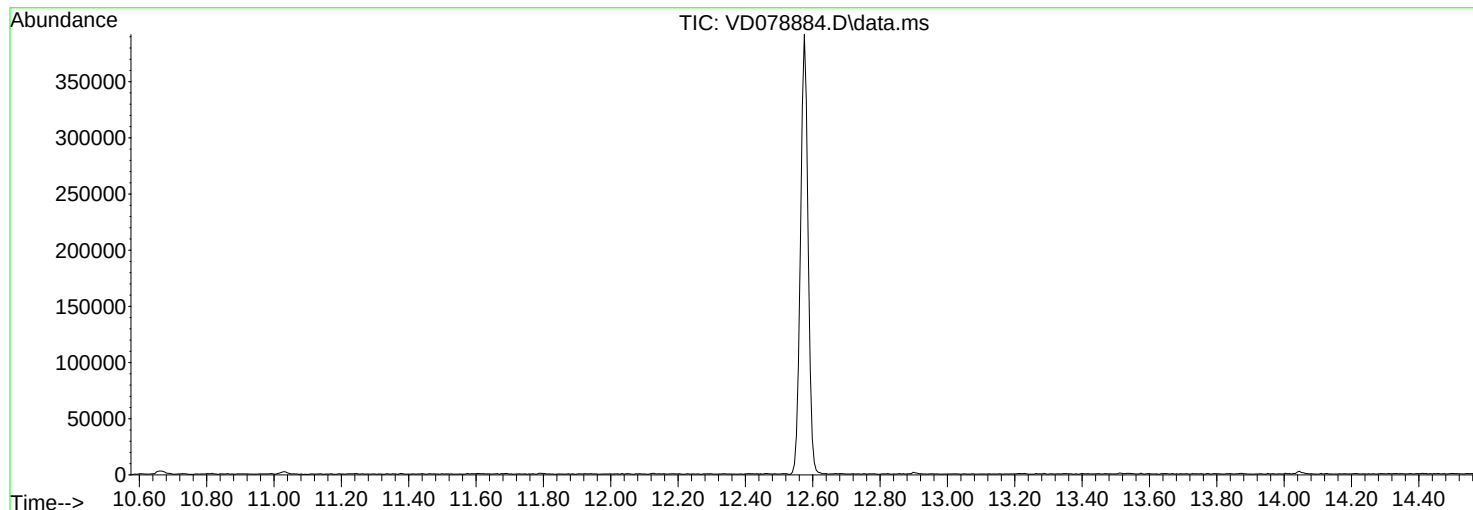

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.2	11426	PASS
75	95	30	60	49.0	32568	PASS
95	95	100	100	100.0	66480	PASS
96	95	5	9	7.0	4682	PASS
173	174	0.00	2	1.4	847	PASS
174	95	50	100	92.7	61659	PASS
175	174	5	9	7.4	4590	PASS
176	174	95	101	96.5	59496	PASS
177	176	5	9	7.2	4290	PASS