

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051122\
 Data File : VD072938.D
 Acq On : 11 May 2022 18:41
 Operator : VA/SY
 Sample : N2749-16
 Misc : 4.33G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 TP-6

Quant Time: May 12 04:15:07 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050222S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 03 08:33:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.973	168	370577	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	661882	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	661001	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	311211	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	204829	42.581	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	85.160%
35) Dibromofluoromethane	7.909	113	213918	46.019	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	92.040%
50) Toluene-d8	10.332	98	808018	48.458	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	96.920%
62) 4-Bromofluorobenzene	12.620	95	301478	48.489	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	96.980%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051122\
Data File : VD072938.D
Acq On : 11 May 2022 18:41
Operator : VA/SY
Sample : N2749-16
Misc : 4.33G/5.00ml/MSVOA_D/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
TP-6

Quant Time: May 12 04:15:07 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050222S.M
Quant Title : SW846 8260
QLast Update : Tue May 03 08:33:49 2022
Response via : Initial Calibration

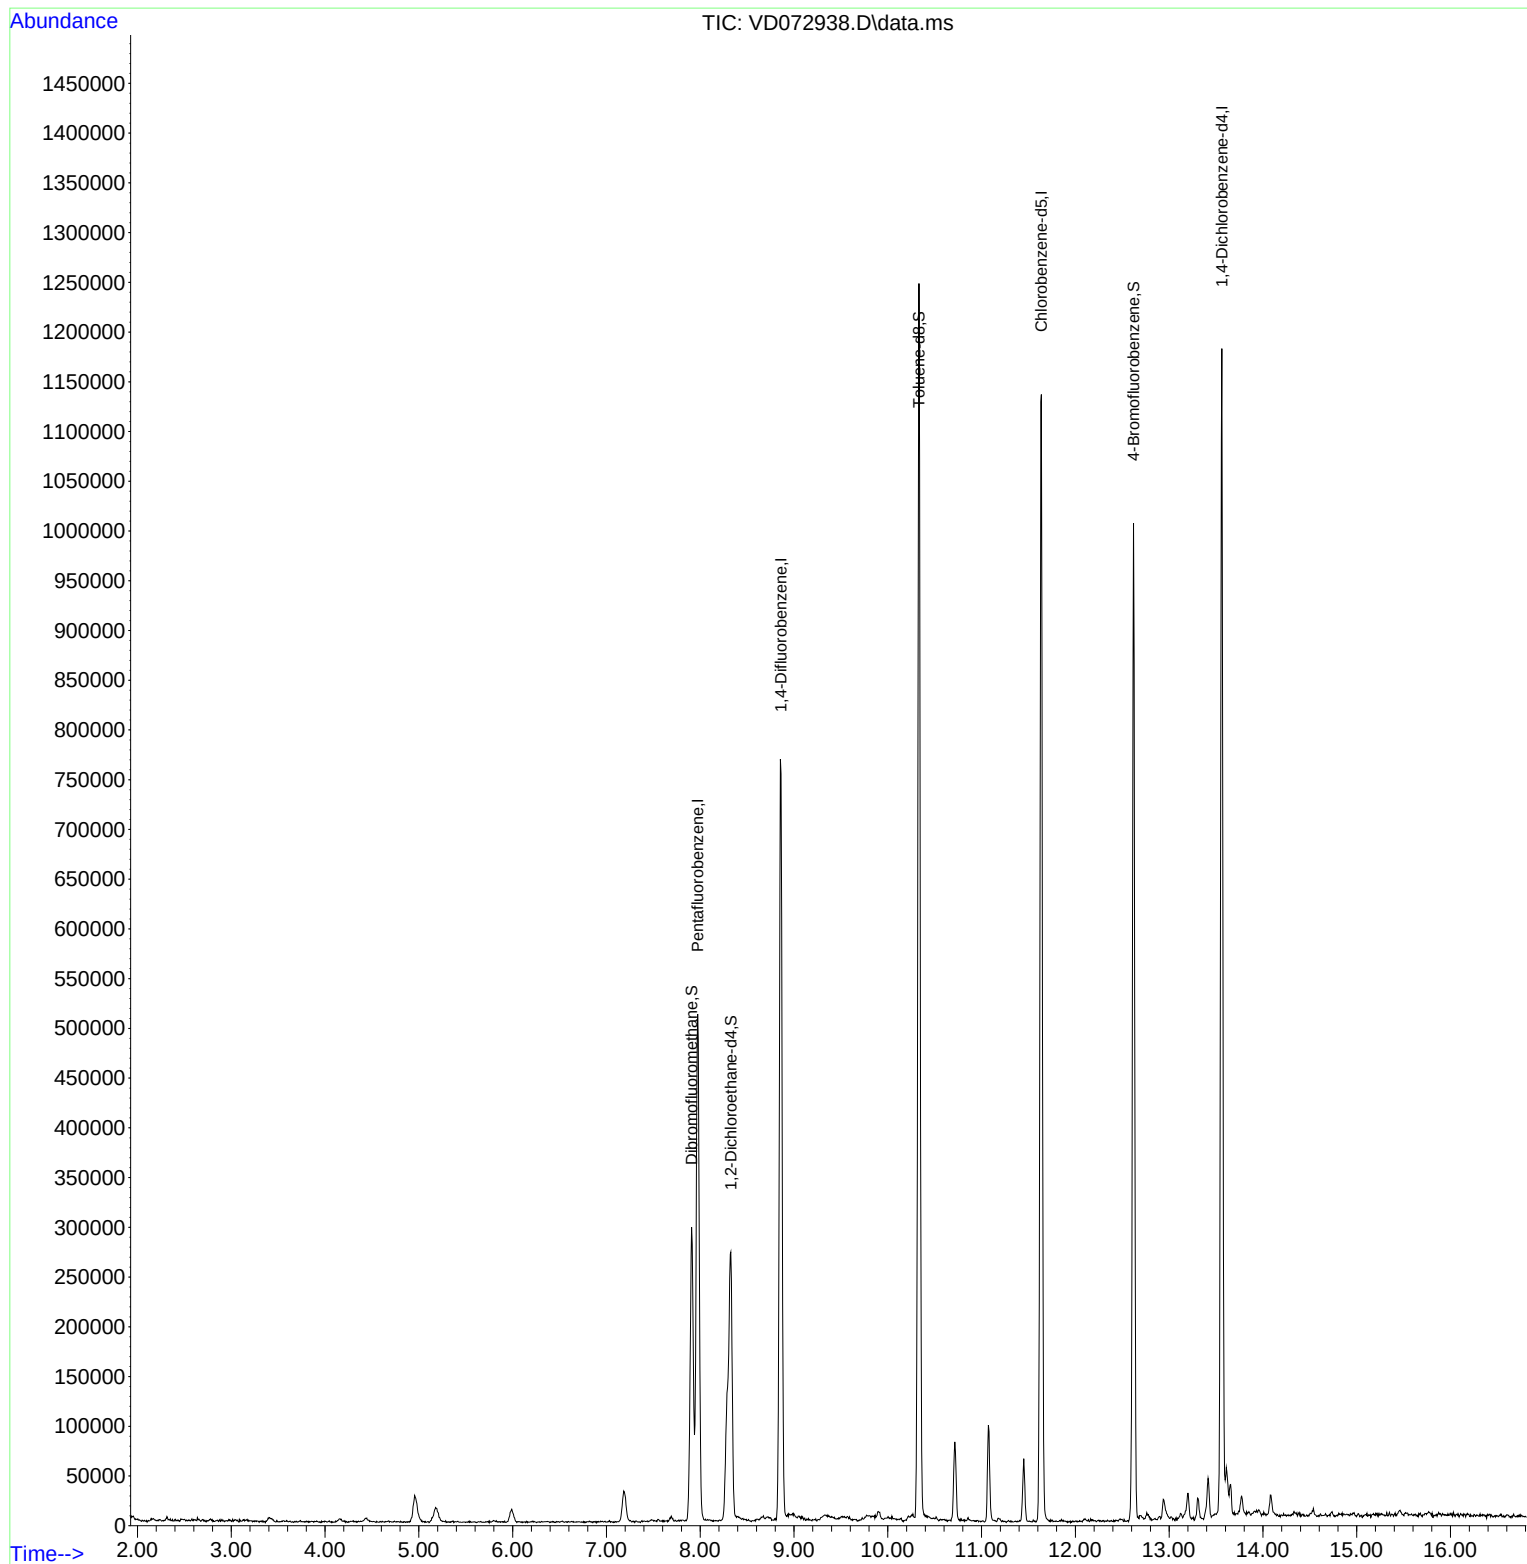

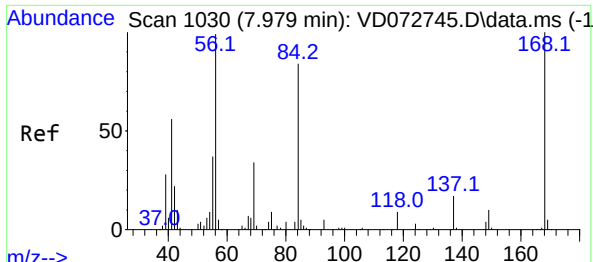

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.973 min Scan# 1029

Delta R.T. -0.006 min

Lab File: VD072938.D

Acq: 11 May 2022 18:41

Instrument :

MSVOA_D

ClientSampleId :





TP-6

Tgt Ion:168 Resp: 370577

Ion Ratio Lower Upper

168 100

99 60.7 49.8 74.6

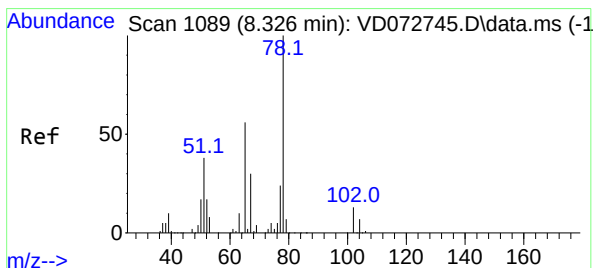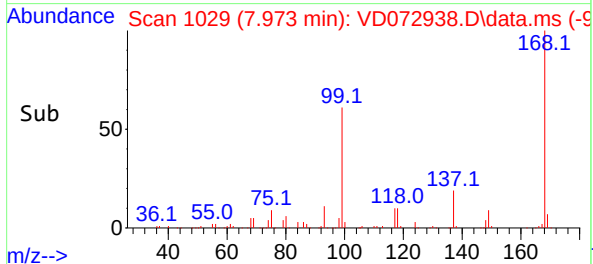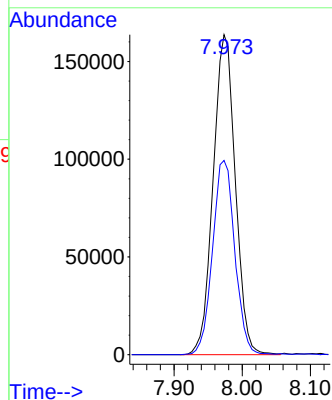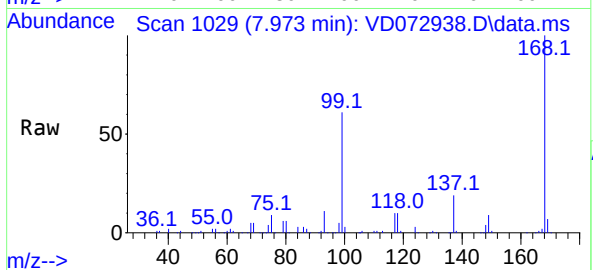

1,2-Dichloroethane-d4

Concen: 42.581 ug/l

RT: 8.326 min Scan# 1089

Delta R.T. 0.000 min

Lab File: VD072938.D




Acq: 11 May 2022 18:41


Tgt Ion: 65 Resp: 204829

Ion Ratio Lower Upper

65 100

67 53.1 0.0 101.4

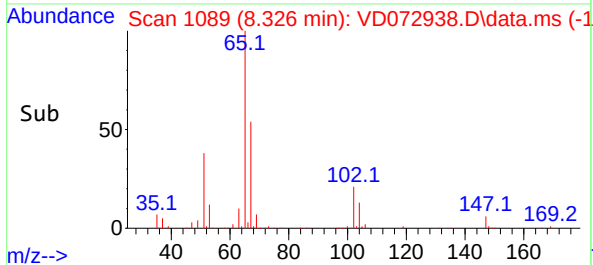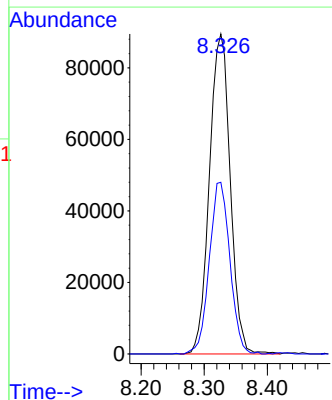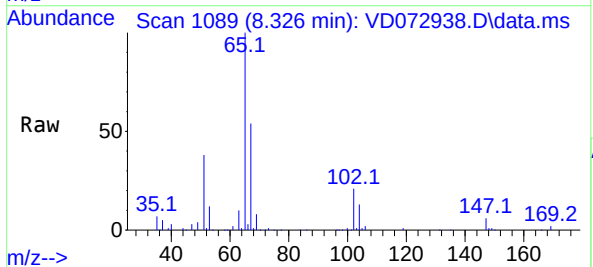

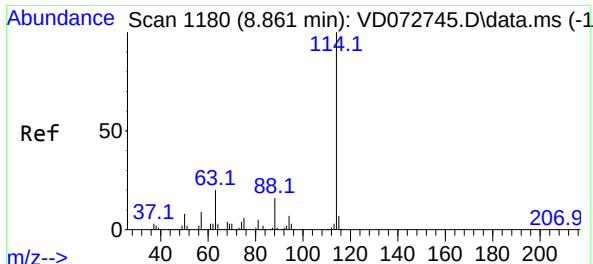

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.861 min Scan# 1180

Delta R.T. 0.000 min

Lab File: VD072938.D

Acq: 11 May 2022 18:41

Instrument :

MSVOA_D

ClientSampleId :

TP-6





Tgt Ion:114 Resp: 661882

Ion Ratio Lower Upper

114 100

63 19.5 0.0 46.6

88 14.7 0.0 33.2

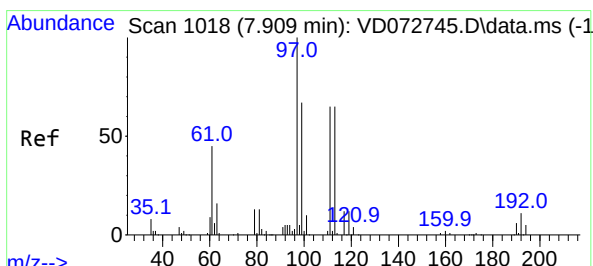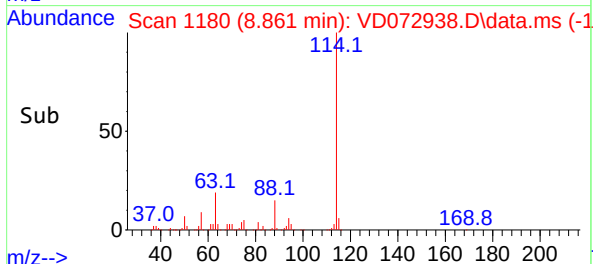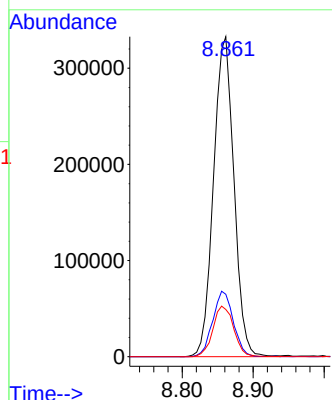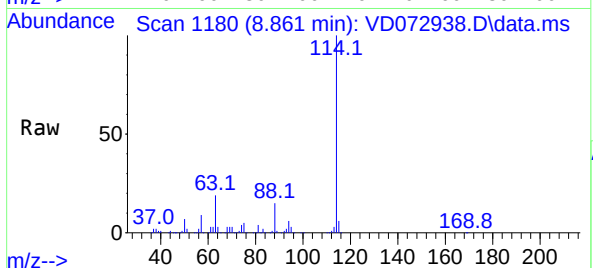

#35

Dibromofluoromethane

Concen: 46.019 ug/l

RT: 7.909 min Scan# 1018

Delta R.T. -0.000 min

Lab File: VD072938.D

Acq: 11 May 2022 18:41




Tgt Ion:113 Resp: 213918


Ion Ratio Lower Upper

113 100

111 102.4 83.8 125.6

192 17.8 14.6 21.8


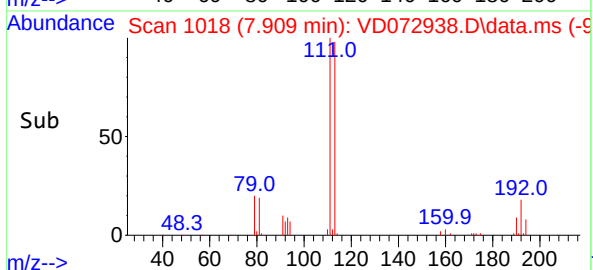
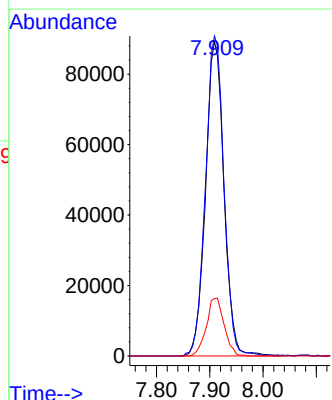
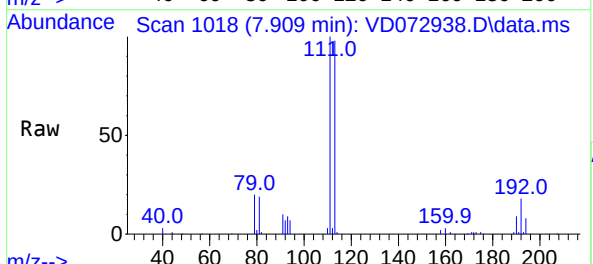


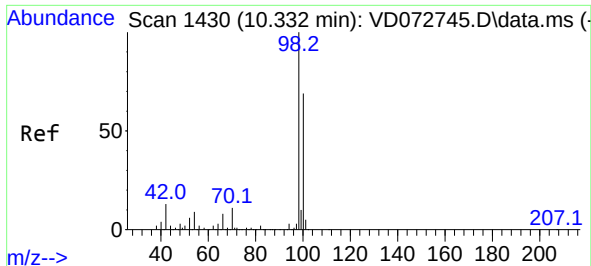

#50
Toluene-d8
Concen: 48.458 ug/l
RT: 10.332 min Scan# 1430
Delta R.T. -0.000 min
Lab File: VD072938.D
Acq: 11 May 2022 18:41




Instrument :
MSVOA_D
ClientSampleId :
TP-6


Tgt Ion: 98 Resp: 808018
Ion Ratio Lower Upper
98 100
100 66.9 52.4 78.6

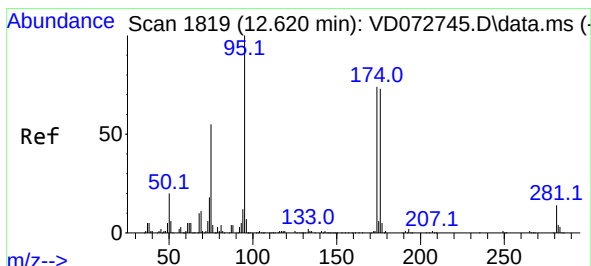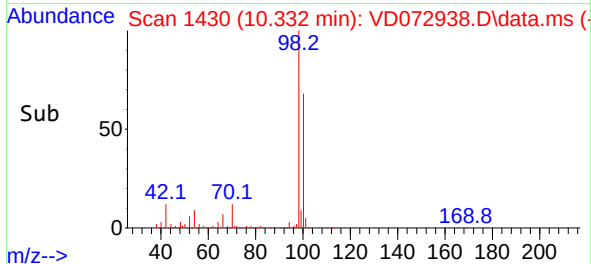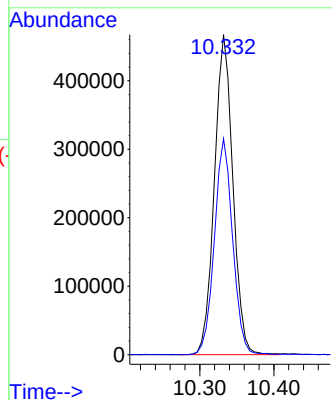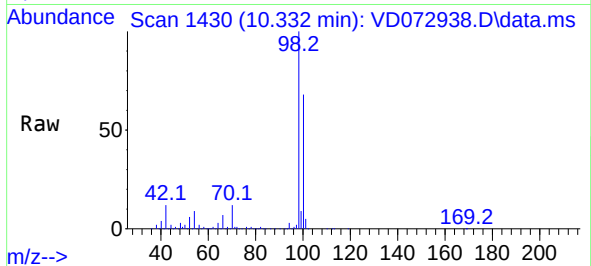

#62
4-Bromofluorobenzene
Concen: 48.489 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. 0.000 min
Lab File: VD072938.D
Acq: 11 May 2022 18:41

Tgt Ion: 95 Resp: 301478
Ion Ratio Lower Upper
95 100
174 75.7 0.0 152.8
176 73.8 0.0 145.4


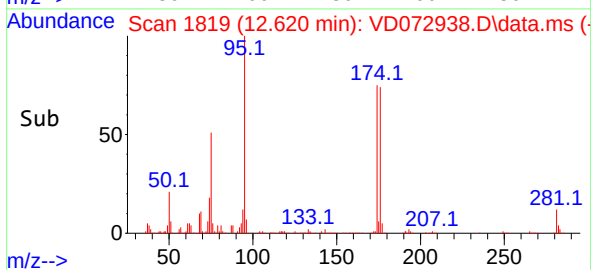
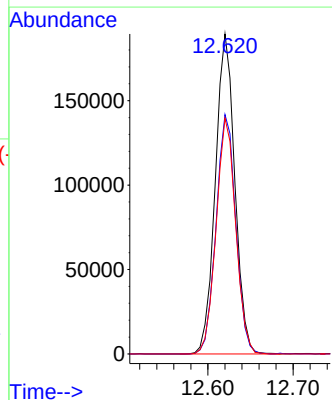
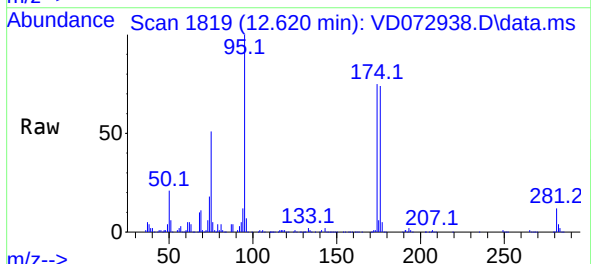


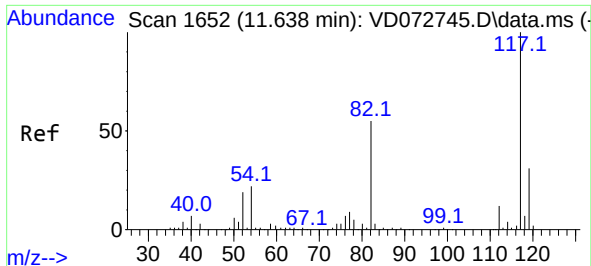

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1
Delta R.T. -0.000 min
Lab File: VD072938.D
Acq: 11 May 2022 18:41

Instrument :
MSVOA_D
ClientSampleId :
TP-6

Tgt Ion:117 Resp: 661001
Ion Ratio Lower Upper
117 100
82 53.4 45.3 67.9
119 32.4 26.6 40.0

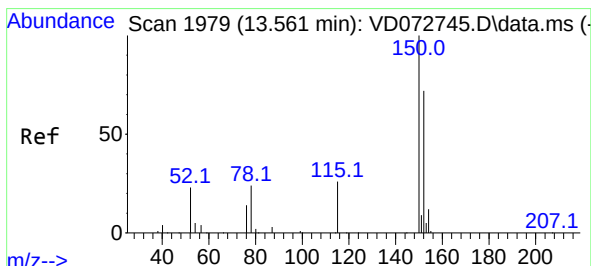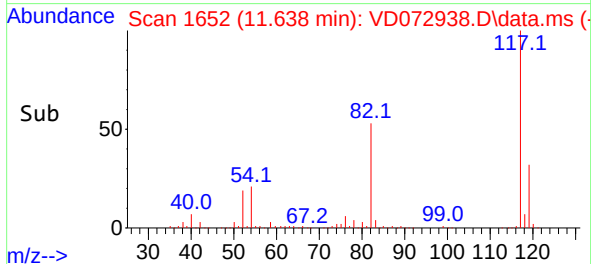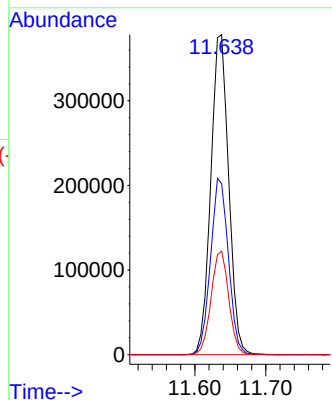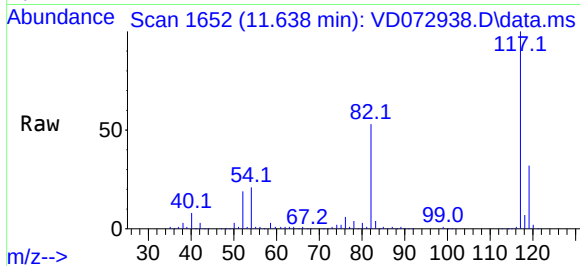

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. 0.000 min
Lab File: VD072938.D
Acq: 11 May 2022 18:41

Tgt Ion:152 Resp: 311211
Ion Ratio Lower Upper
152 100
115 60.0 31.3 93.8
150 157.3 0.0 348.6

