

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051122\
 Data File : VD072942.D
 Acq On : 11 May 2022 20:37
 Operator : VA/SY
 Sample : N2776-02
 Misc : 7.68G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 CF-280MER-9-5

Quant Time: May 12 04:16:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050222S.M
 Quant Title : SW846 8260
 QLast Update : Tue May 03 08:33:49 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.973	168	350554	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.855	114	645465	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	629749	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	286669	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	212142	46.620	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	93.240%
35) Dibromofluoromethane	7.908	113	211163	46.582	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	93.160%
50) Toluene-d8	10.332	98	783569	48.187	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	96.380%
62) 4-Bromofluorobenzene	12.620	95	317898	52.430	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	104.860%


Target Compounds	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051122\
Data File : VD072942.D
Acq On : 11 May 2022 20:37
Operator : VA/SY
Sample : N2776-02
Misc : 7.68G/5.00ml/MSVOA_D/SOIL
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
CF-280MER-9-5

Quant Time: May 12 04:16:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050222S.M
Quant Title : SW846 8260
QLast Update : Tue May 03 08:33:49 2022
Response via : Initial Calibration

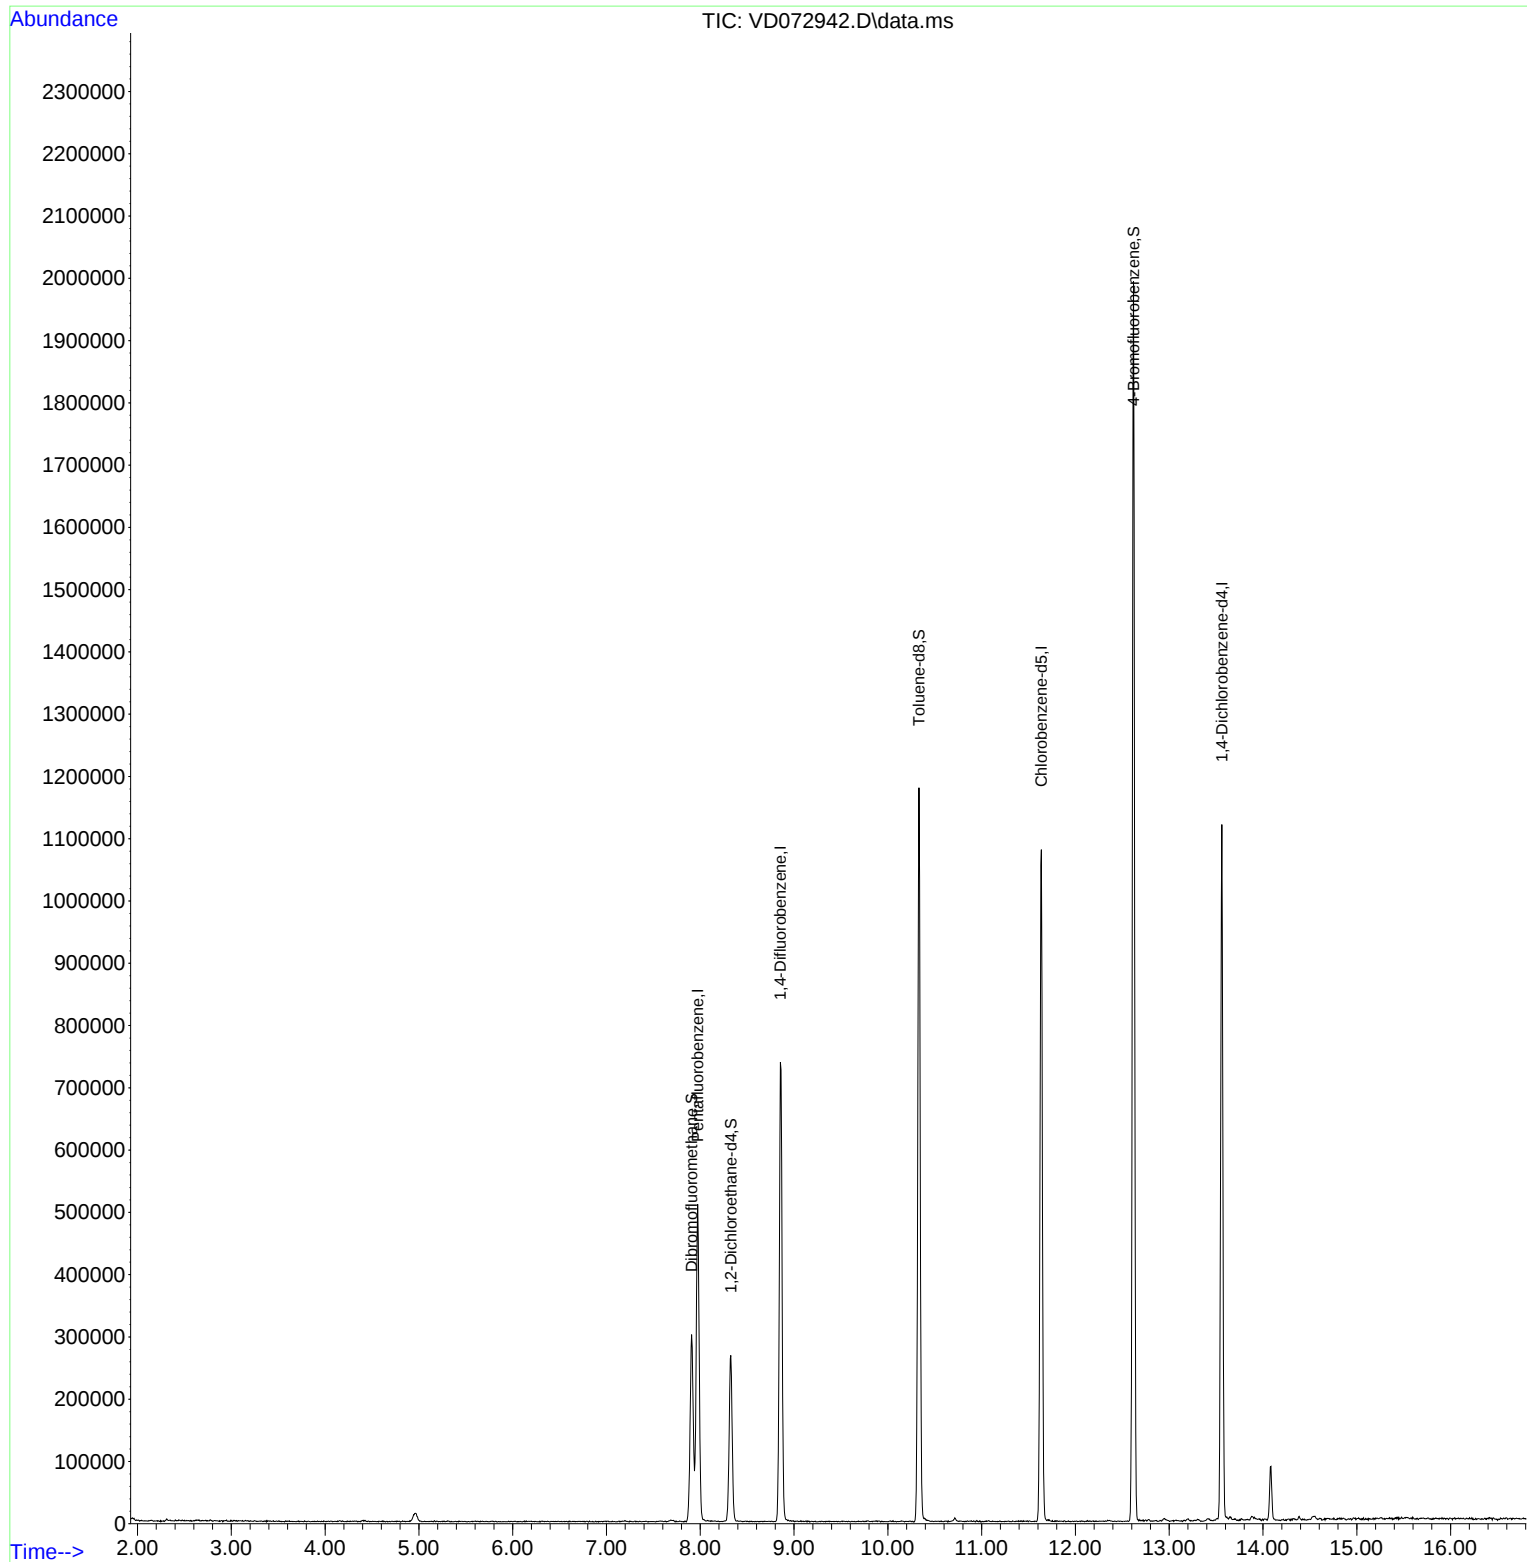



Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.973 min Scan# 1029

Delta R.T. -0.006 min

Lab File: VD072942.D

Acq: 11 May 2022 20:37

Instrument :

MSVOA_D

ClientSampleId :





CF-280MER-9-5

Tgt Ion:168 Resp: 350554

Ion Ratio Lower Upper

168 100

99 60.5 49.8 74.6

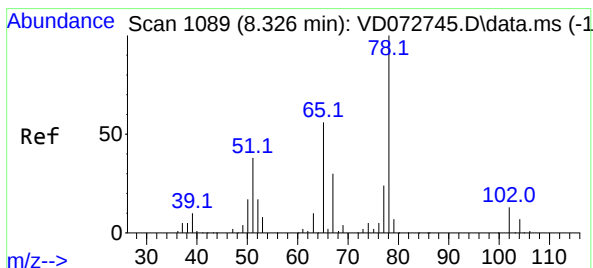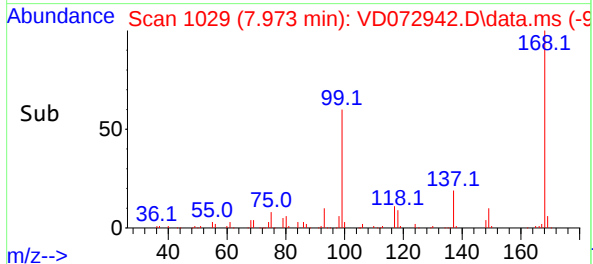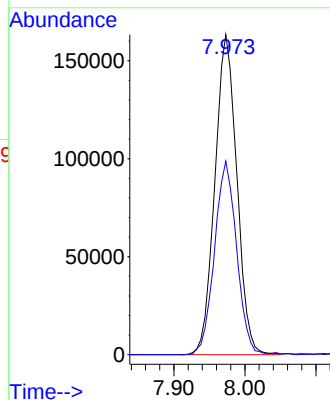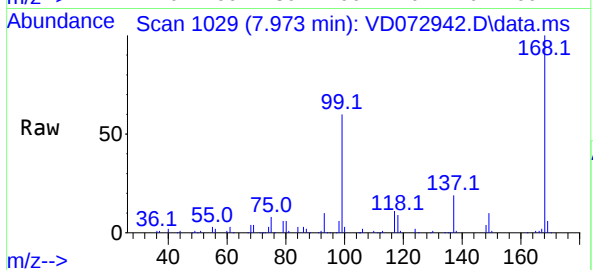

1,2-Dichloroethane-d4

Concen: 46.620 ug/l

RT: 8.326 min Scan# 1089

Delta R.T. 0.000 min

Lab File: VD072942.D




Acq: 11 May 2022 20:37


Tgt Ion: 65 Resp: 212142

Ion Ratio Lower Upper

65 100

67 52.3 0.0 101.4

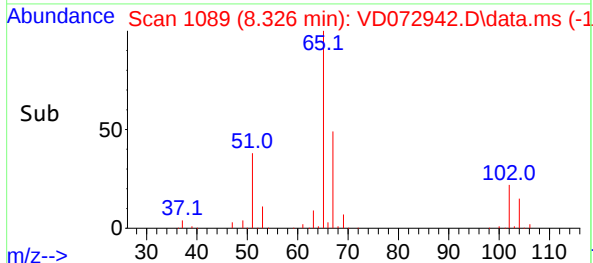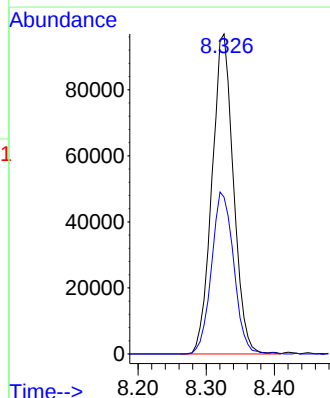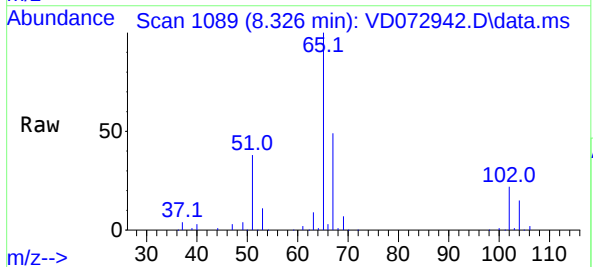



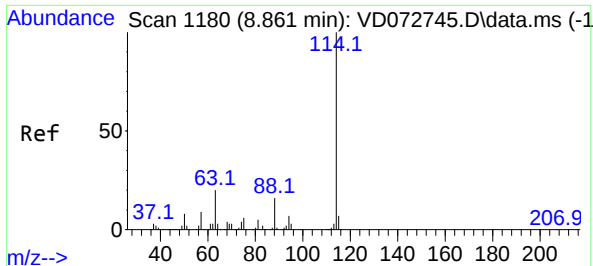


#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.855 min Scan# 1180
Delta R.T. -0.006 min
Lab File: VD072942.D
Acq: 11 May 2022 20:37

Instrument :
MSVOA_D
ClientSampleId :
CF-280MER-9-5

Tgt Ion:114 Resp: 645465




Ion	Ratio	Lower	Upper
114	100		
63	20.6	0.0	46.6
88	15.4	0.0	33.2

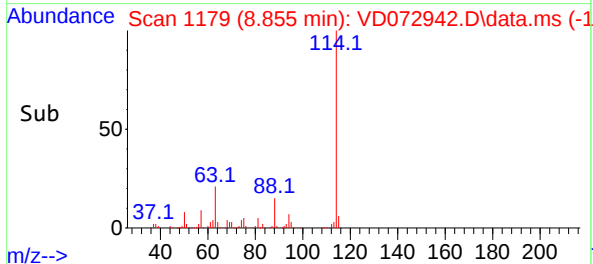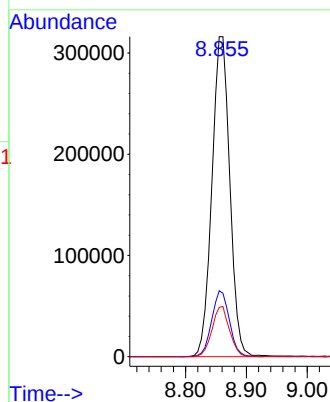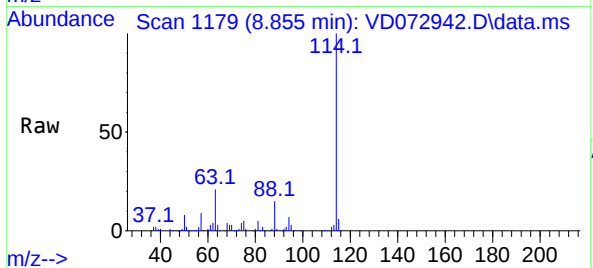


#35
Dibromofluoromethane
Concen: 46.582 ug/l
RT: 7.908 min Scan# 1018
Delta R.T. -0.001 min
Lab File: VD072942.D
Acq: 11 May 2022 20:37

Tgt Ion:113 Resp: 211163

Ion	Ratio	Lower	Upper
113	100		
111	103.9	83.8	125.6
192	18.5	14.6	21.8


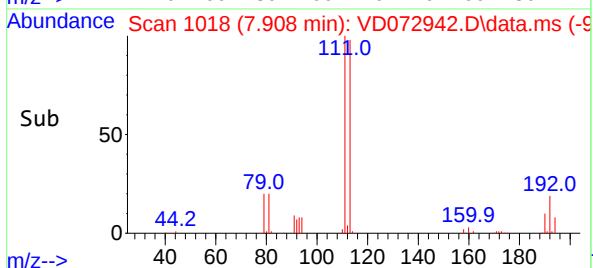
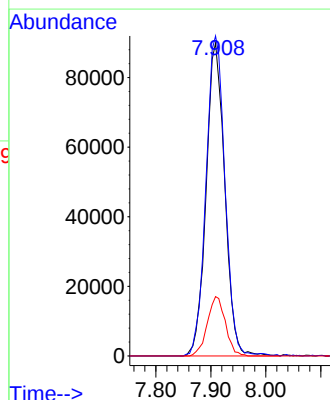
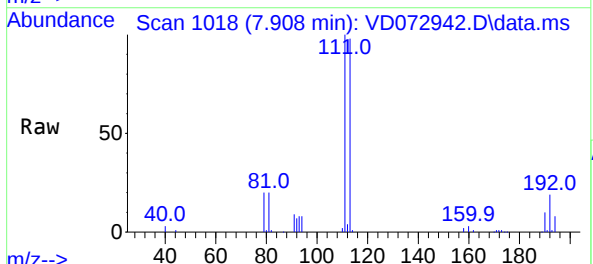


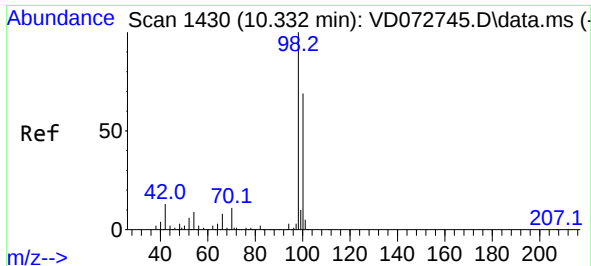

#50
Toluene-d8
Concen: 48.187 ug/l
RT: 10.332 min Scan# 1430
Delta R.T. -0.000 min
Lab File: VD072942.D
Acq: 11 May 2022 20:37




Instrument :
MSVOA_D
ClientSampleId :
CF-280MER-9-5


Tgt Ion: 98 Resp: 783569
Ion Ratio Lower Upper
98 100
100 65.7 52.4 78.6

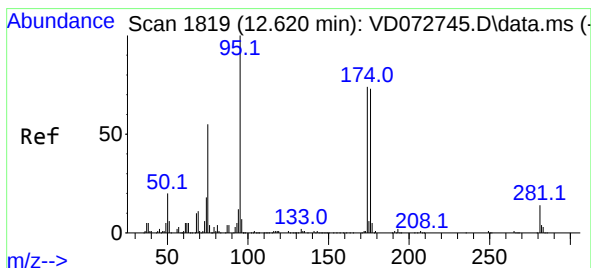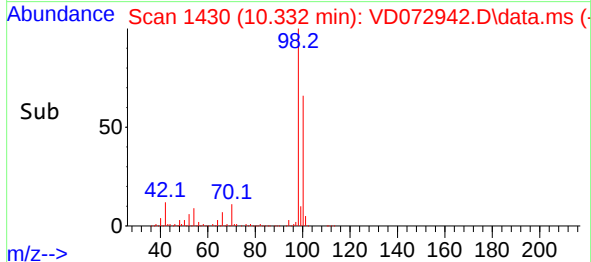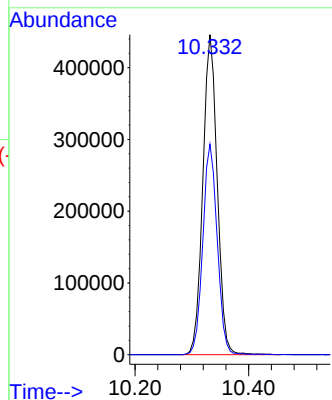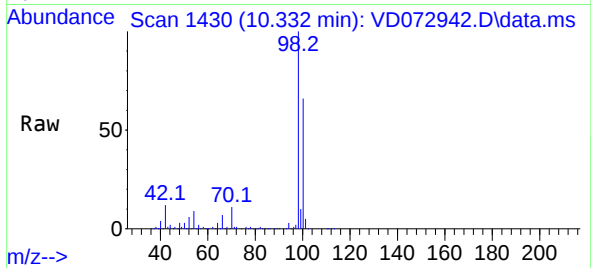

#62
4-Bromofluorobenzene
Concen: 52.430 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. -0.000 min
Lab File: VD072942.D
Acq: 11 May 2022 20:37

Tgt Ion: 95 Resp: 317898
Ion Ratio Lower Upper
95 100
174 73.8 0.0 152.8
176 72.5 0.0 145.4


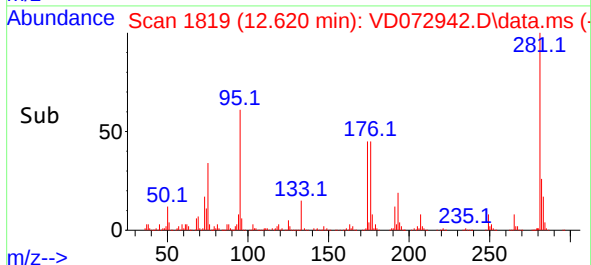
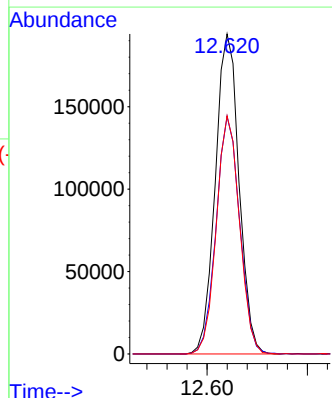
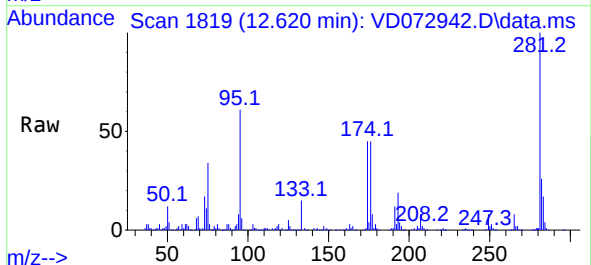


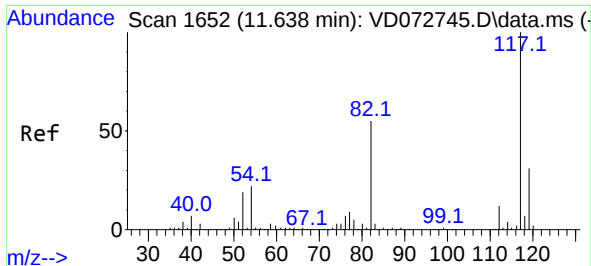

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 1
Delta R.T. -0.000 min
Lab File: VD072942.D
Acq: 11 May 2022 20:37

Instrument :
MSVOA_D
ClientSampleId :
CF-280MER-9-5

Tgt Ion:117 Resp: 629749
Ion Ratio Lower Upper
117 100
82 54.4 45.3 67.9
119 31.3 26.6 40.0

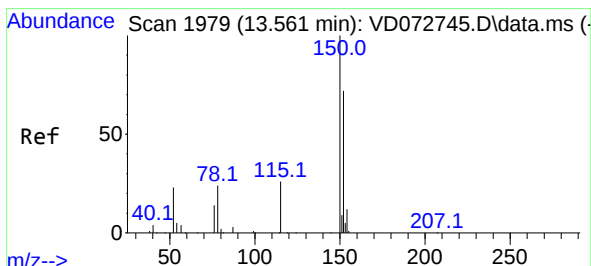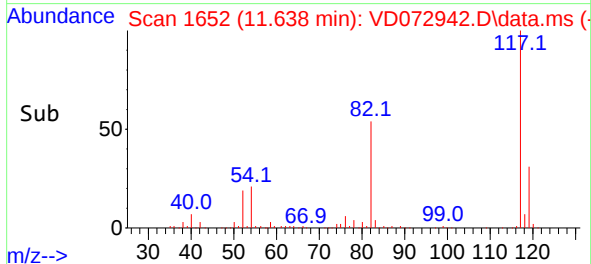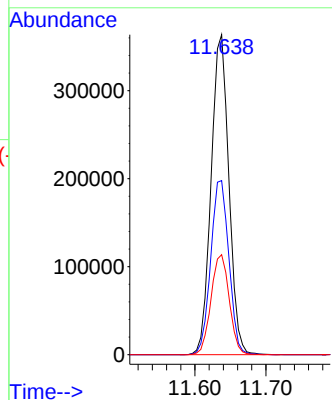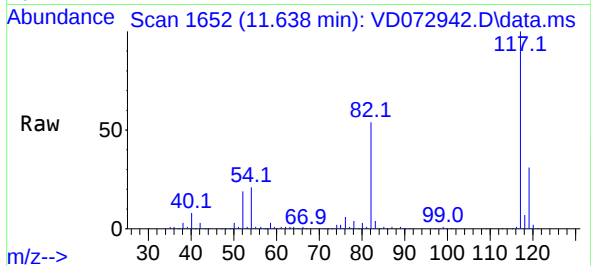

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. 0.000 min
Lab File: VD072942.D
Acq: 11 May 2022 20:37

Tgt Ion:152 Resp: 286669
Ion Ratio Lower Upper
152 100
115 62.0 31.3 93.8
150 161.9 0.0 348.6

