
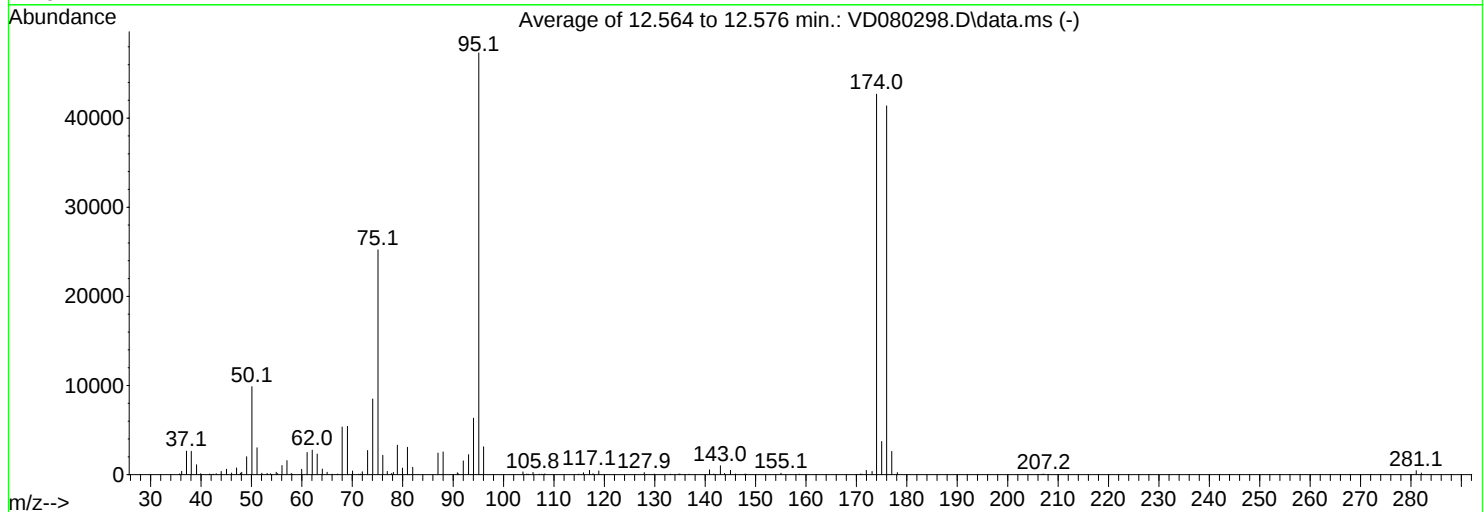


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051325\
Data File : VD080298.D
Acq On : 13 May 2025 09:45
Operator : RP/MD
Sample : BFB
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050625S.M
Title : SW846 8260
Last Update : Wed May 07 08:57:11 2025

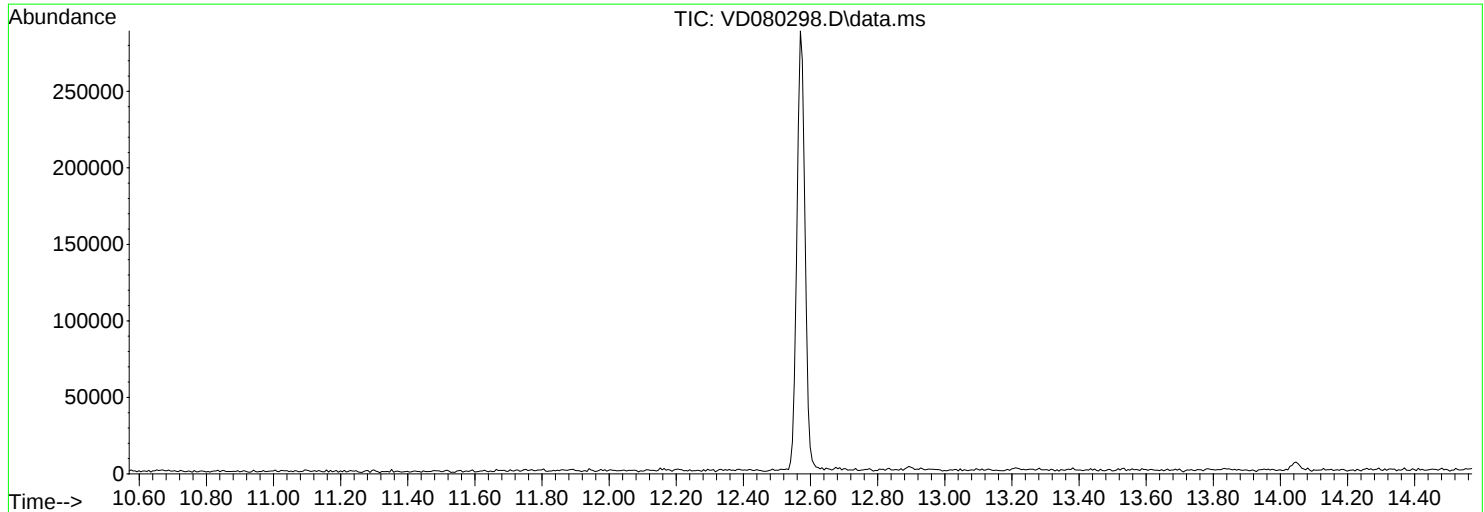

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	20.9	9881	PASS
75	95	30	60	53.3	25224	PASS
95	95	100	100	100.0	47325	PASS
96	95	5	9	6.6	3129	PASS
173	174	0.00	2	0.9	368	PASS
174	95	50	100	90.2	42685	PASS
175	174	5	9	8.7	3710	PASS
176	174	95	101	96.9	41373	PASS
177	176	5	9	6.3	2604	PASS