
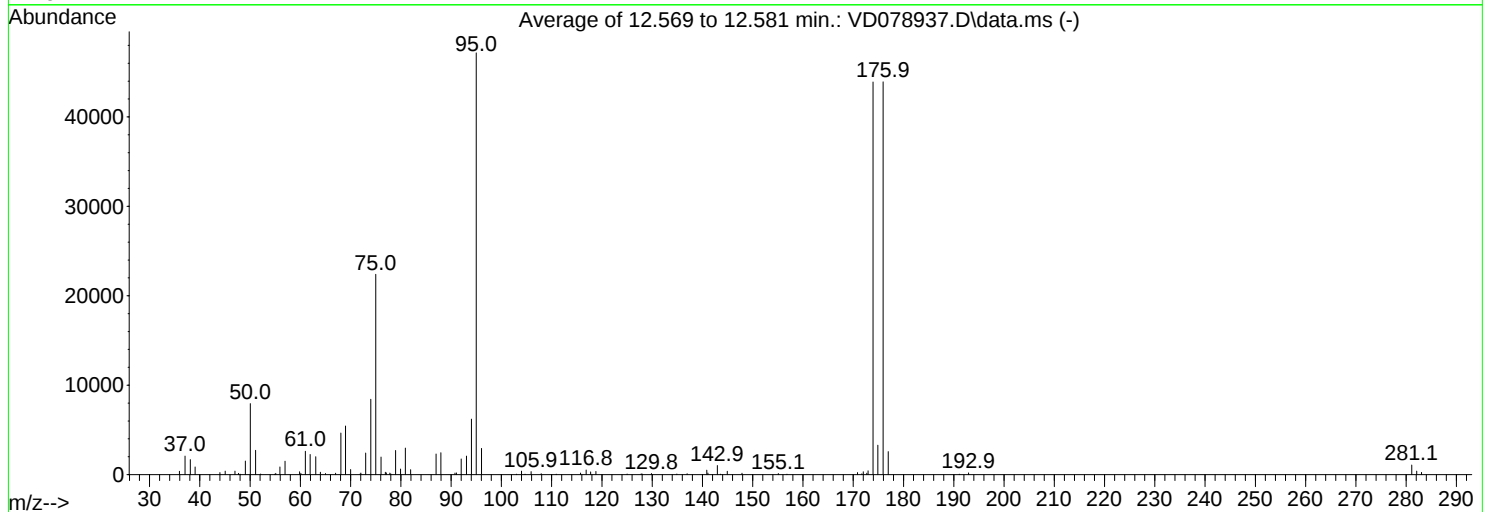


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051624\
Data File : VD078937.D
Acq On : 16 May 2024 08:40
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051324S.M
Title : SW846 8260
Last Update : Tue May 14 06:21:28 2024

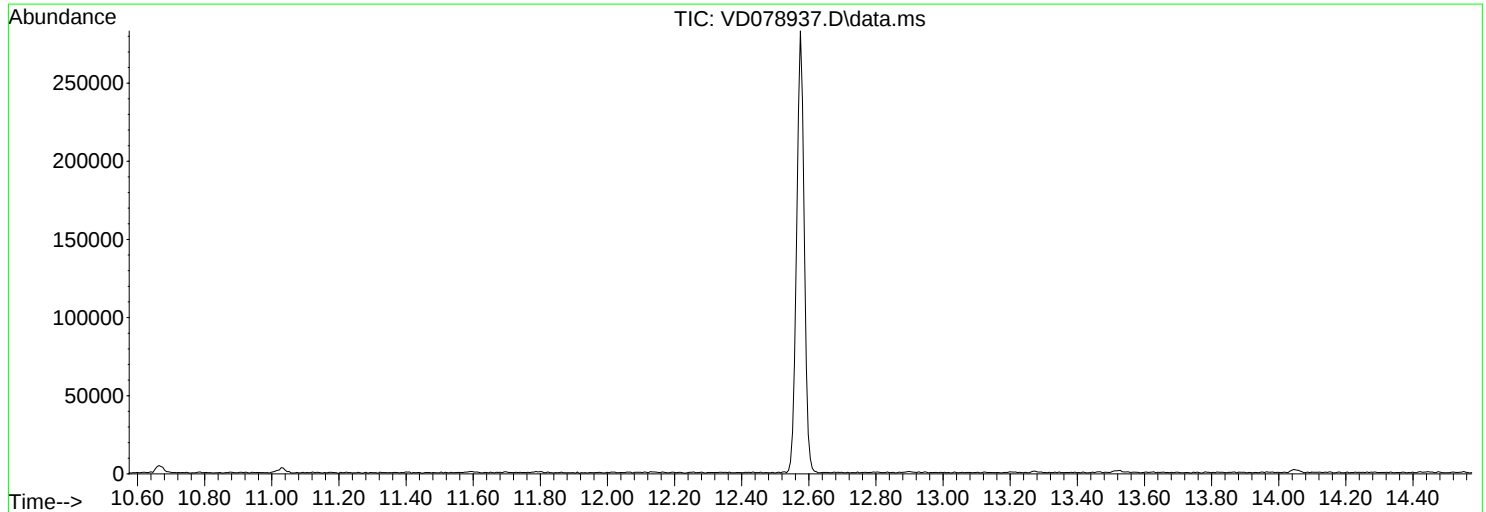

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.9	7952	PASS
75	95	30	60	47.5	22395	PASS
95	95	100	100	100.0	47163	PASS
96	95	5	9	6.2	2930	PASS
173	174	0.00	2	1.0	427	PASS
174	95	50	100	93.1	43899	PASS
175	174	5	9	7.5	3298	PASS
176	174	95	101	100.1	43923	PASS
177	176	5	9	5.9	2583	PASS