

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD051625\  
 Data File : VD080364.D  
 Acq On : 16 May 2025 12:02  
 Operator : RP/MD  
 Sample : Q2039-01  
 Misc : 5.06G/5.0ml/MSVOA\_D/SOIL/B  
 ALS Vial : 6 Sample Multiplier: 1

Instrument :  
 MSVOA\_D  
 ClientSampleId :  
 TR-05-05142025

Quant Time: May 17 01:18:02 2025  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D050625S.M  
 Quant Title : SW846 8260  
 QLast Update : Wed May 07 08:57:11 2025  
 Response via : Initial Calibration

| Compound                   | R.T.   | QIon | Response | Conc   | Units | Dev(Min) |
|----------------------------|--------|------|----------|--------|-------|----------|
| -----                      |        |      |          |        |       |          |
| Internal Standards         |        |      |          |        |       |          |
| 1) Pentafluorobenzene      | 7.876  | 168  | 12190    | 50.000 | ug/l  | 0.00     |
| 34) 1,4-Difluorobenzene    | 8.770  | 114  | 22438    | 50.000 | ug/l  | 0.00     |
| 63) Chlorobenzene-d5       | 11.582 | 117  | 25262    | 50.000 | ug/l  | 0.00     |
| 72) 1,4-Dichlorobenzene-d4 | 13.517 | 152  | 18074    | 50.000 | ug/l  | 0.00     |

|                             |        |       |          |          |      |           |
|-----------------------------|--------|-------|----------|----------|------|-----------|
| System Monitoring Compounds |        |       |          |          |      |           |
| 33) 1,2-Dichloroethane-d4   | 8.229  | 65    | 11226    | 71.214   | ug/l | 0.00      |
| Spiked Amount               | 50.000 | Range | 50 - 163 | Recovery | =    | 142.420%  |
| 35) Dibromofluoromethane    | 7.806  | 113   | 10531    | 70.026   | ug/l | 0.00      |
| Spiked Amount               | 50.000 | Range | 54 - 147 | Recovery | =    | 140.060%  |
| 50) Toluene-d8              | 10.270 | 98    | 29338    | 49.512   | ug/l | 0.00      |
| Spiked Amount               | 50.000 | Range | 58 - 134 | Recovery | =    | 99.020%   |
| 62) 4-Bromofluorobenzene    | 12.570 | 95    | 16405    | 86.256   | ug/l | 0.00      |
| Spiked Amount               | 50.000 | Range | 30 - 143 | Recovery | =    | 172.520%# |


| Target Compounds | Qvalue |
|------------------|--------|
| -----            |        |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_D\Data\VD051625\  
Data File : VD080364.D  
Acq On : 16 May 2025 12:02  
Operator : RP/MD  
Sample : Q2039-01  
Misc : 5.06G/5.0ml/MSVOA\_D/SOIL/B  
ALS Vial : 6 Sample Multiplier: 1

Instrument :  
MSVOA\_D  
ClientSampleId :  
TR-05-05142025

Quant Time: May 17 01:18:02 2025  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_D\Method\82D050625S.M  
Quant Title : SW846 8260  
QLast Update : Wed May 07 08:57:11 2025  
Response via : Initial Calibration




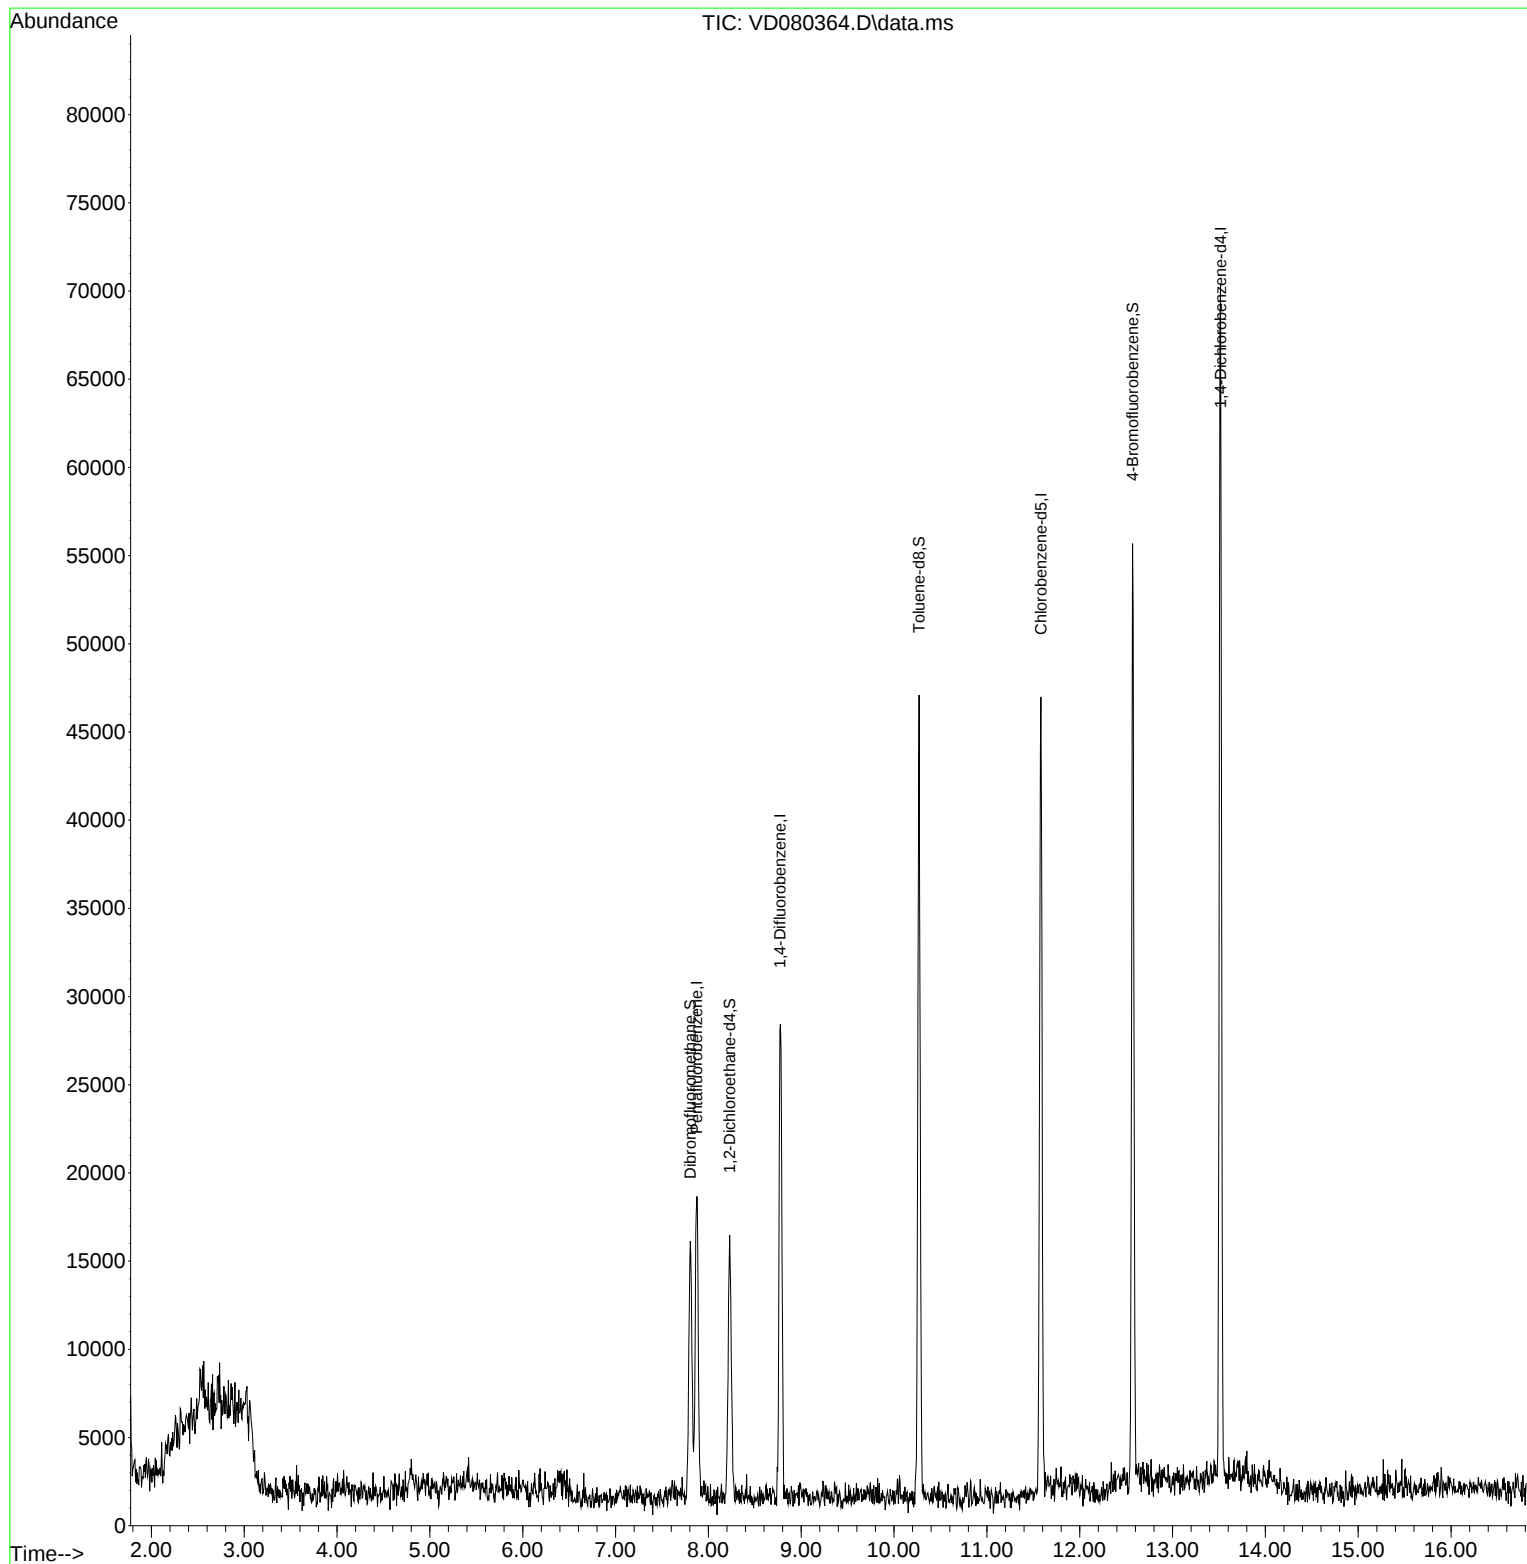


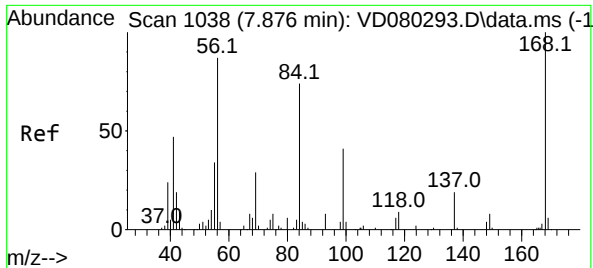

#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 7.876 min Scan# 1038  
Delta R.T. 0.001 min  
Lab File: VD080364.D  
Acq: 16 May 2025 12:02




Instrument :  
MSVOA\_D  
ClientSampleId :  
TR-05-05142025


Tgt Ion:168 Resp: 12190  
Ion Ratio Lower Upper  
168 100  
99 55.9 46.0 69.0

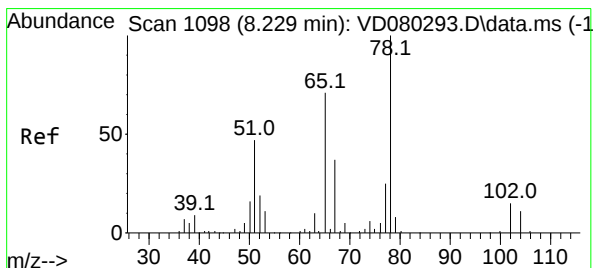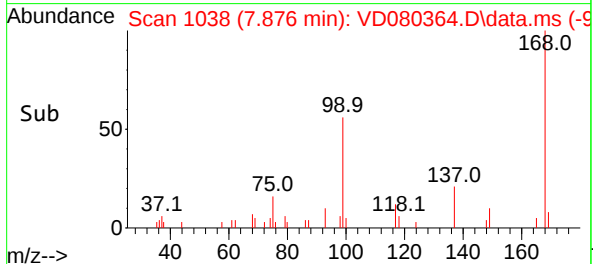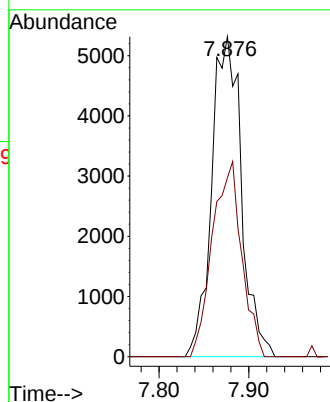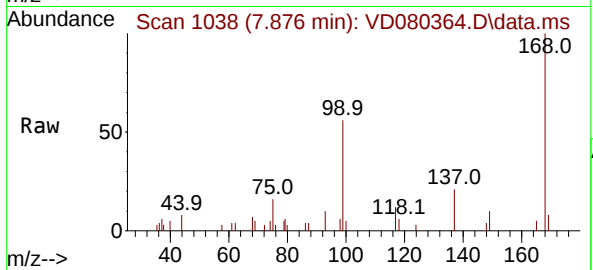

#33  
1,2-Dichloroethane-d4  
Concen: 71.214 ug/l  
RT: 8.229 min Scan# 1098  
Delta R.T. 0.001 min  
Lab File: VD080364.D  
Acq: 16 May 2025 12:02

Tgt Ion: 65 Resp: 11226  
Ion Ratio Lower Upper  
65 100  
67 54.5 0.0 109.2

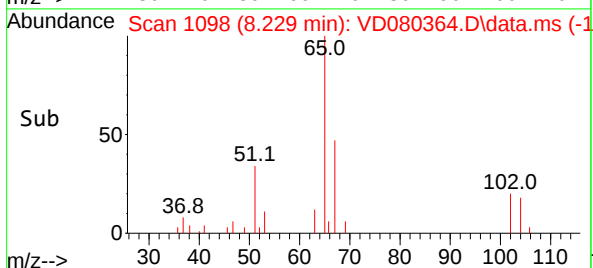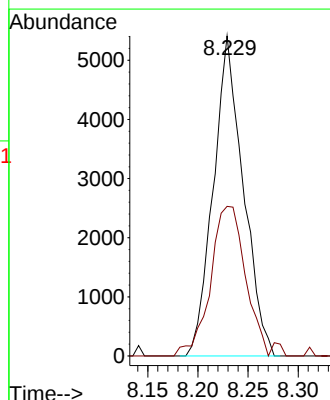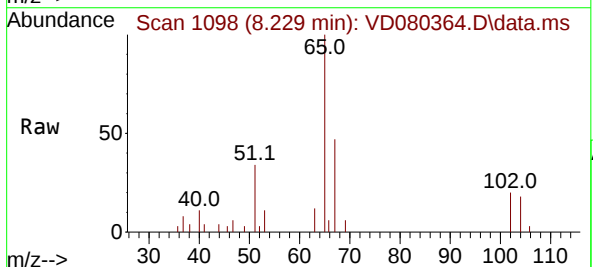

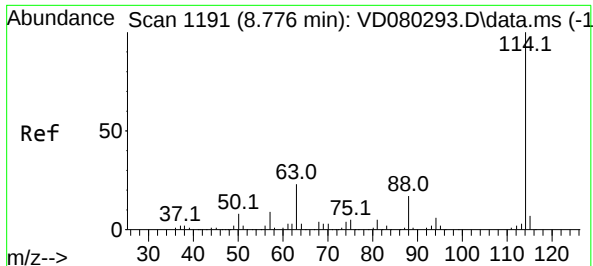

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.770 min Scan# 1191

Delta R.T. -0.005 min

Lab File: VD080364.D

Acq: 16 May 2025 12:02

Instrument :

MSVOA\_D

ClientSampleId :

TR-05-05142025





Tgt Ion:114 Resp: 22438

Ion Ratio Lower Upper

114 100

63 15.7 0.0 38.8

88 14.4 0.0 30.6

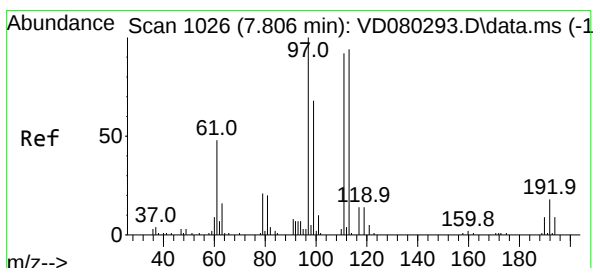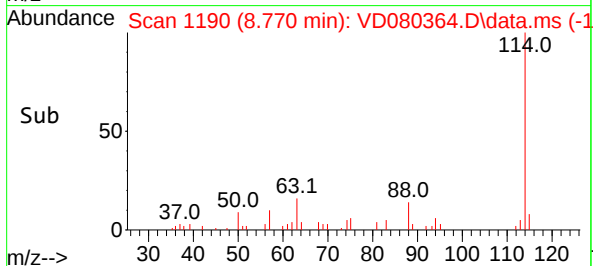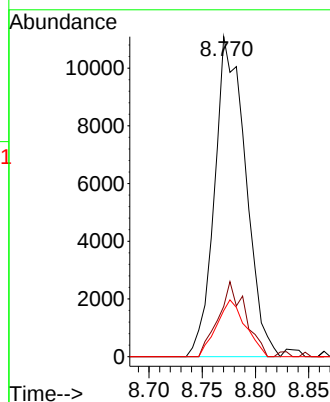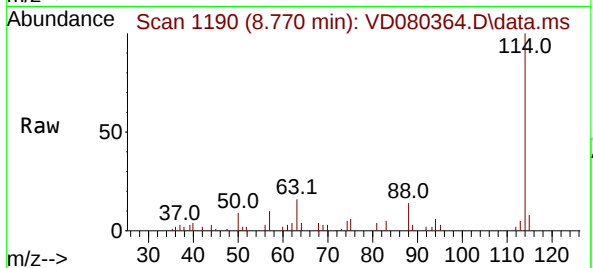

#35

Dibromofluoromethane

Concen: 70.026 ug/l

RT: 7.806 min Scan# 1026

Delta R.T. 0.001 min

Lab File: VD080364.D

Acq: 16 May 2025 12:02




Tgt Ion:113 Resp: 10531


Ion Ratio Lower Upper

113 100

111 104.3 82.5 123.7

192 20.7 16.6 25.0


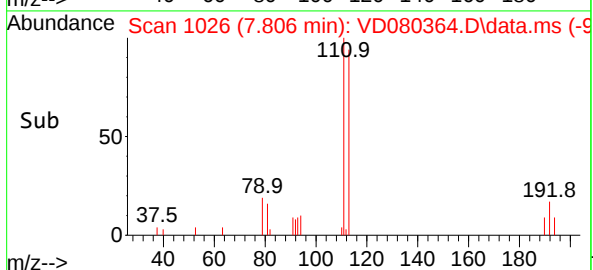
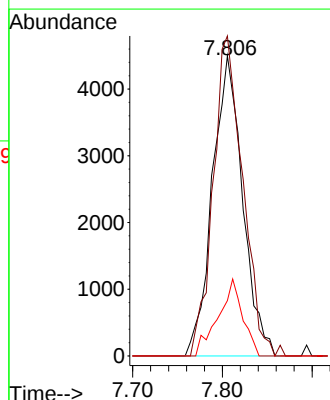
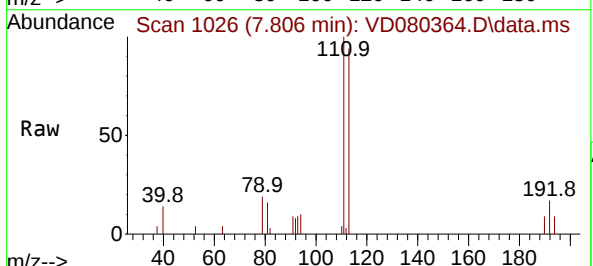


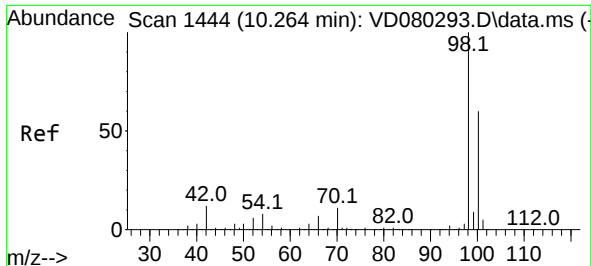

#50  
Toluene-d8  
Concen: 49.512 ug/l  
RT: 10.270 min Scan# 1444  
Delta R.T. 0.001 min  
Lab File: VD080364.D  
Acq: 16 May 2025 12:02




Instrument :  
MSVOA\_D  
ClientSampleId :  
TR-05-05142025


Tgt Ion: 98 Resp: 29338  
Ion Ratio Lower Upper  
98 100  
100 61.1 50.2 75.4

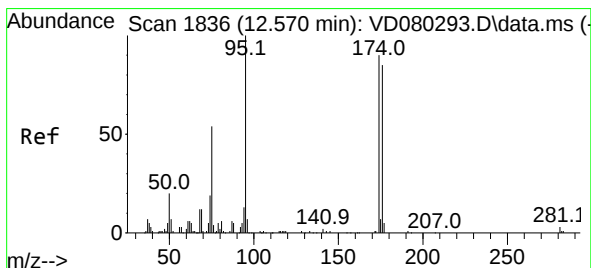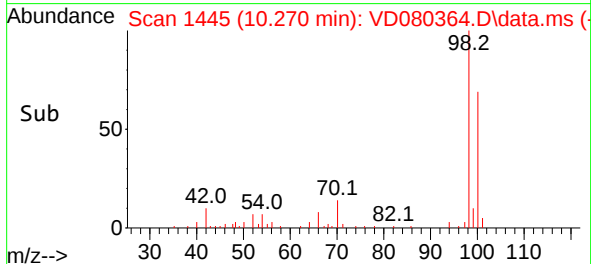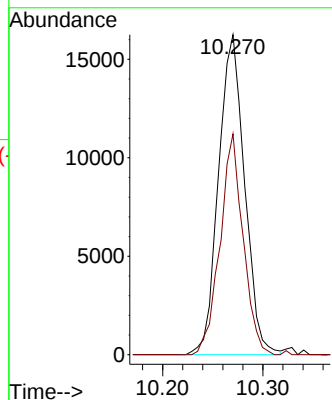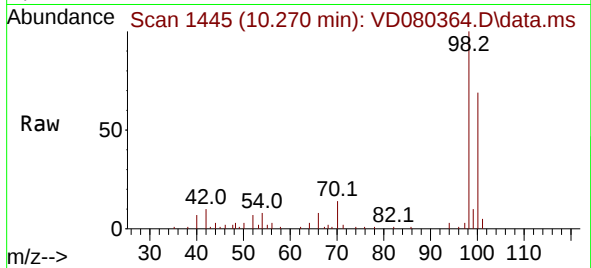

#62  
4-Bromofluorobenzene  
Concen: 86.256 ug/l  
RT: 12.570 min Scan# 1836  
Delta R.T. 0.001 min  
Lab File: VD080364.D  
Acq: 16 May 2025 12:02

Tgt Ion: 95 Resp: 16405  
Ion Ratio Lower Upper  
95 100  
174 82.9 0.0 173.4  
176 85.0 0.0 166.6


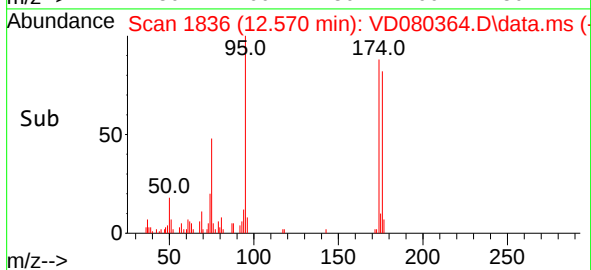
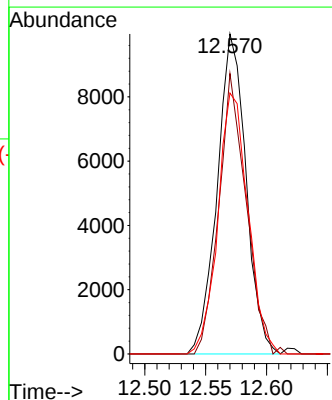
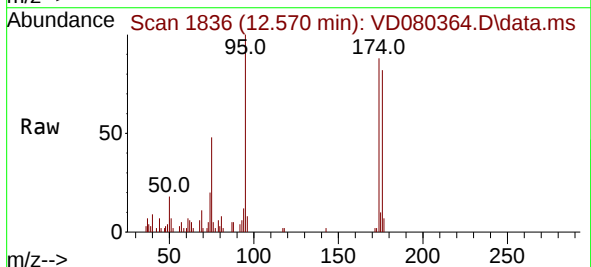


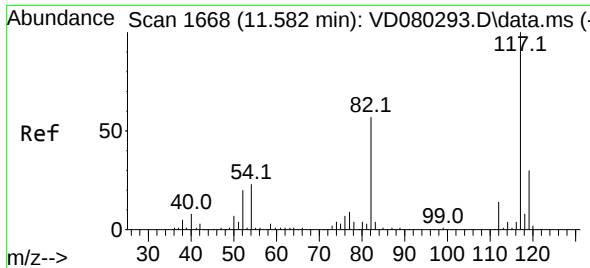

#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.582 min Scan# 117  
Delta R.T. 0.001 min  
Lab File: VD080364.D  
Acq: 16 May 2025 12:02

Instrument :  
MSVOA\_D  
ClientSampleId :  
TR-05-05142025

Tgt Ion:117 Resp: 25262  
Ion Ratio Lower Upper  
117 100  
82 53.0 45.8 68.6  
119 26.2 26.2 39.2

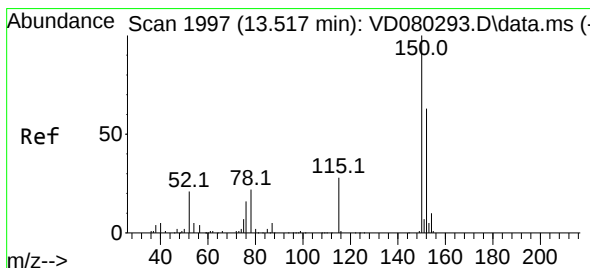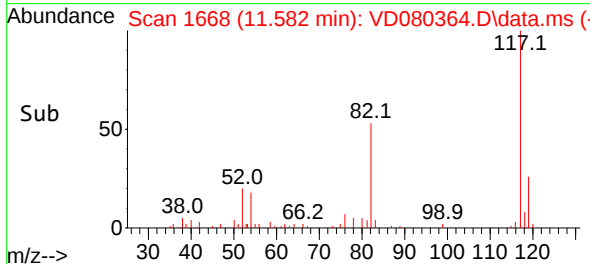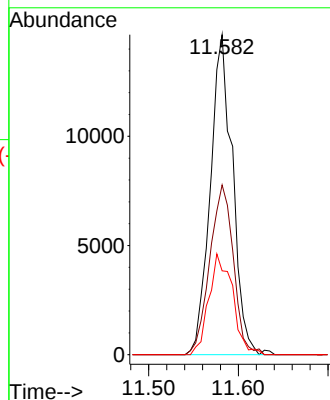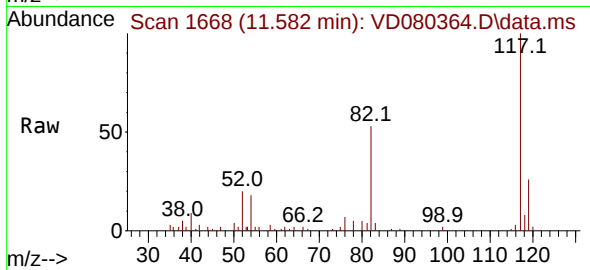

#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 13.517 min Scan# 1997  
Delta R.T. 0.001 min  
Lab File: VD080364.D  
Acq: 16 May 2025 12:02

Tgt Ion:152 Resp: 18074  
Ion Ratio Lower Upper  
152 100  
115 57.3 28.9 86.8  
150 160.1 0.0 354.8

