
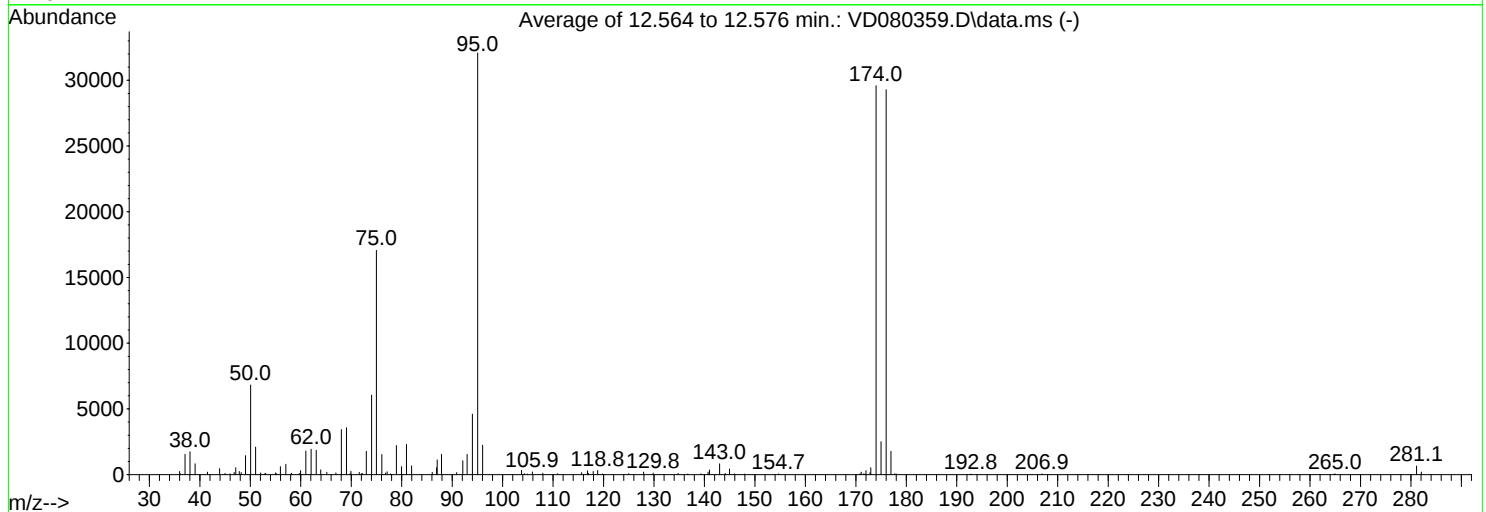


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD051625\
Data File : VD080359.D
Acq On : 16 May 2025 08:11
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5.0ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D050625S.M
Title : SW846 8260
Last Update : Wed May 07 08:57:11 2025

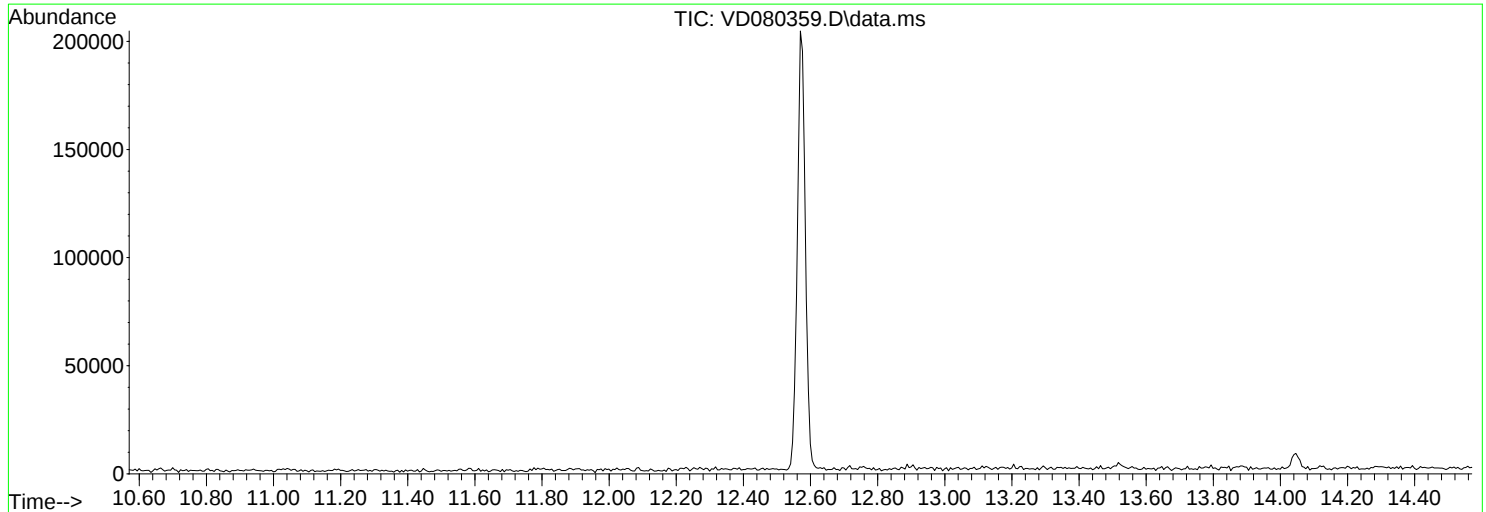

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.2	6812	PASS
75	95	30	60	53.2	17070	PASS
95	95	100	100	100.0	32088	PASS
96	95	5	9	7.0	2244	PASS
173	174	0.00	2	1.8	527	PASS
174	95	50	100	92.2	29597	PASS
175	174	5	9	8.5	2503	PASS
176	174	95	101	99.0	29288	PASS
177	176	5	9	6.1	1776	PASS