
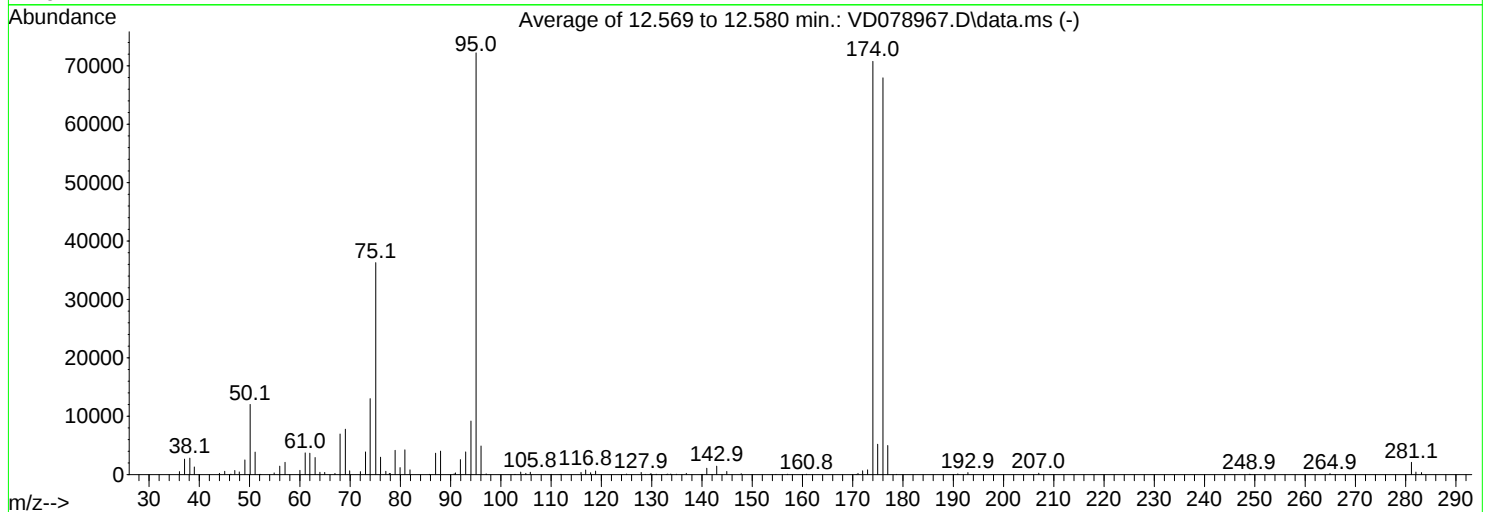


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052024\
Data File : VD078967.D
Acq On : 20 May 2024 09:32
Operator : RP/MD
Sample : BFB213
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB213

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051724SMA.M
Title : SFAM01.0
Last Update : Tue May 21 01:03:15 2024

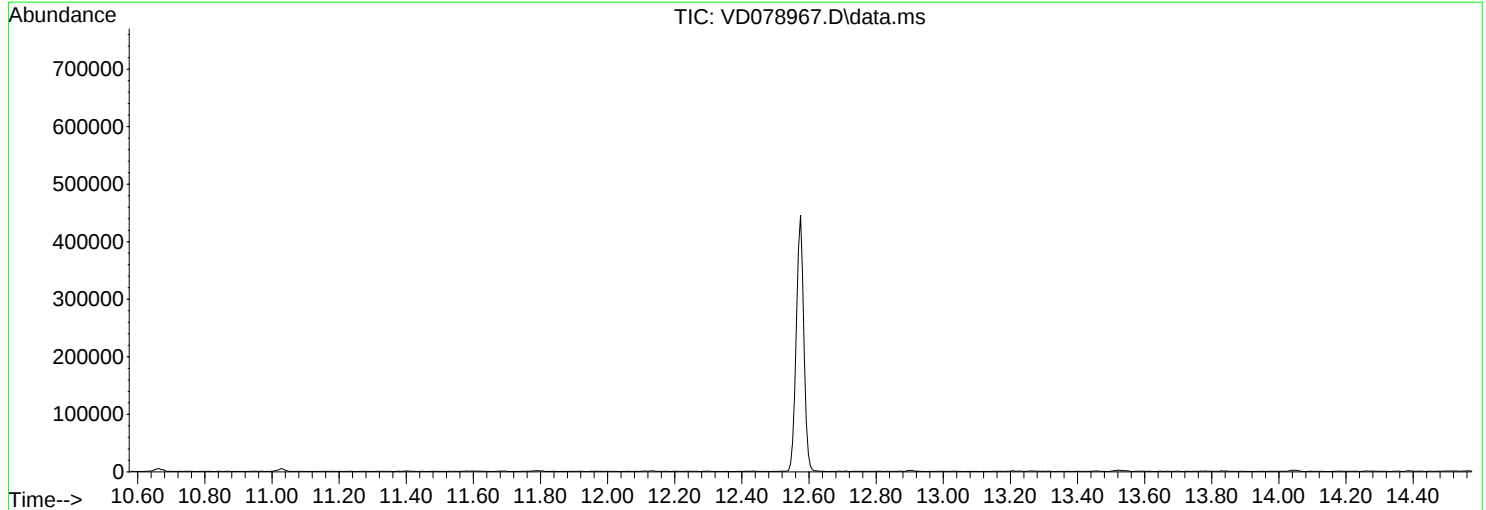

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.6	12023	PASS
75	95	30	80	50.3	36307	PASS
95	95	100	100	100.0	72229	PASS
96	95	5	9	6.8	4909	PASS
173	174	0.00	2	1.2	838	PASS
174	95	50	120	98.0	70773	PASS
175	174	5	9	7.4	5209	PASS
176	174	95	105	96.0	67947	PASS
177	176	5	10	7.4	4999	PASS

Scan 1860 (12.528 min): VD078967.D\data.ms
BFB213

m/z	Abundance
40.00	758.0
44.10	322.0

Instrument :
MSVOA_D
ClientSampleId :
BFB213

m/z	Abundance
36.00	448.0
37.10	2687.0
38.10	2725.0
39.00	1320.0
40.10	944.0
44.00	466.0
45.10	577.0
46.10	175.0
47.00	624.0
48.00	380.0
49.10	2260.0
50.10	12552.0
51.10	3738.0
52.00	192.0
54.90	292.0
56.00	1088.0
57.10	2747.0
60.00	709.0
61.00	3803.0
62.00	3467.0
63.10	3329.0
64.00	371.0
64.90	639.0
67.10	153.0
68.00	7152.0
69.10	7890.0
69.90	690.0
72.10	551.0
73.10	3798.0
74.00	12689.0
75.10	35912.0
76.00	2824.0
77.10	441.0
77.80	626.0
79.00	4159.0
79.90	1274.0
80.90	4512.0
81.90	776.0
87.00	3967.0
88.00	3671.0
90.90	500.0
92.00	2655.0
93.00	4080.0
94.00	8507.0
95.10	72944.0
96.00	5121.0
97.00	249.0
104.00	429.0
105.00	180.0
105.90	576.0
110.00	153.0
115.90	364.0
117.00	959.0
118.00	228.0
118.90	482.0
125.00	181.0
127.90	409.0
129.70	294.0
136.90	230.0
140.00	182.0
140.90	1069.0
143.00	1517.0
145.00	847.0
171.20	178.0
172.00	709.0
173.00	1028.0
174.00	69104.0
175.00	5418.0
176.00	64664.0
176.90	4543.0
192.90	337.0
207.10	248.0
248.90	247.0
281.20	1687.0
282.10	266.0
283.20	350.0

Instrument :
MSVOA_D
ClientSampleId :
BFB213

m/z	Abundance
36.10	552.0
37.00	2926.0
38.10	3555.0
39.00	1585.0
40.00	586.0
43.90	539.0
45.00	708.0
46.30	228.0
47.10	905.0
47.90	508.0
49.00	2763.0
50.10	13139.0
51.10	4248.0
52.20	166.0
55.00	334.0
56.00	1606.0
57.00	2142.0
60.00	715.0
61.00	4332.0
62.00	4308.0
63.00	2905.0
63.90	461.0
65.00	330.0
66.90	316.0
68.00	7968.0
69.10	9170.0
69.90	616.0
72.00	536.0
73.00	4758.0
74.00	14457.0
75.10	42024.0
76.00	3158.0
77.10	966.0
78.00	614.0
78.90	4426.0
80.00	1250.0
80.90	4434.0
81.90	863.0
85.80	203.0
87.00	3912.0
88.00	5158.0
91.00	444.0
92.00	2665.0
93.00	4166.0
94.10	10680.0
95.00	81344.0
96.10	5087.0
97.10	184.0
102.80	175.0
104.00	512.0
105.00	178.0
105.90	204.0
111.80	159.0
115.90	450.0
116.80	763.0
117.80	438.0
118.80	654.0
125.00	182.0
127.90	398.0
128.70	207.0
129.90	412.0
133.20	316.0
133.80	313.0
134.90	277.0
137.00	217.0
140.90	1084.0
143.00	1438.0
144.90	625.0
147.80	287.0
154.70	180.0
157.00	243.0
160.80	247.0
171.00	491.0
172.00	717.0
172.90	907.0
174.00	79352.0
174.90	6027.0
176.00	78064.0
176.90	6059.0
178.70	176.0
190.90	247.0
192.90	506.0
207.00	273.0
249.10	171.0
264.90	290.0
281.20	2635.0
282.00	523.0
283.20	415.0

Instrument :
MSVOA_D
ClientSampleId :
BFB213

m/z	Abundance
36.00	575.0
37.10	2389.0
38.10	2203.0
39.00	1061.0
40.00	807.0
43.90	613.0
45.00	451.0
47.00	594.0
47.90	518.0
49.00	2544.0
50.10	10378.0
51.10	3584.0
54.80	295.0
56.00	1677.0
57.10	1451.0
60.00	841.0
61.10	3091.0
62.00	3262.0
63.10	2539.0
64.10	427.0
65.00	171.0
67.10	235.0
68.00	5737.0
69.00	6267.0
69.90	661.0
72.00	479.0
73.00	3124.0
74.00	11922.0
75.10	30984.0
76.10	2992.0
77.00	306.0
79.00	3881.0
79.90	1083.0
80.90	3807.0
81.90	833.0
87.00	3172.0
88.00	3286.0
90.70	399.0
91.90	2410.0
93.00	3400.0
94.00	8335.0
95.10	62400.0
96.10	4519.0
103.80	352.0
104.90	282.0
105.80	437.0
112.00	173.0
116.00	344.0
116.80	684.0
117.90	289.0
118.90	654.0
127.90	319.0
129.80	192.0
130.90	278.0
132.90	201.0
136.80	189.0
141.00	1172.0
142.90	1409.0
144.80	183.0
147.80	216.0
170.70	157.0
171.80	590.0
173.00	579.0
174.00	63864.0
175.00	4182.0
176.00	61112.0
177.00	4394.0
190.90	155.0
192.90	268.0
206.90	236.0
265.00	303.0
281.10	1993.0
282.10	494.0
283.00	338.0

Instrument :
MSVOA_D
ClientSampleId :
BFB213