

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052322\
 Data File : VD073286.D
 Acq On : 23 May 2022 16:44
 Operator : VA/SY
 Sample : N2870-04
 Misc : 5.65G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 P033-SS001-1824-01

Quant Time: May 24 03:27:42 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051922S.M
 Quant Title : SW846 8260
 QLast Update : Thu May 19 15:13:42 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.973	168	320449	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.856	114	569787	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.632	117	600928	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	279405	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	180464	50.958	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	101.920%
35) Dibromofluoromethane	7.909	113	193783	51.540	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	103.080%
50) Toluene-d8	10.332	98	707631	51.057	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	102.120%
62) 4-Bromofluorobenzene	12.620	95	266134	54.716	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	109.440%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052322\
Data File : VD073286.D
Acq On : 23 May 2022 16:44
Operator : VA/SY
Sample : N2870-04
Misc : 5.65G/5.00ml/MSVOA_D/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
P033-SS001-1824-01

Quant Time: May 24 03:27:42 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051922S.M
Quant Title : SW846 8260
QLast Update : Thu May 19 15:13:42 2022
Response via : Initial Calibration




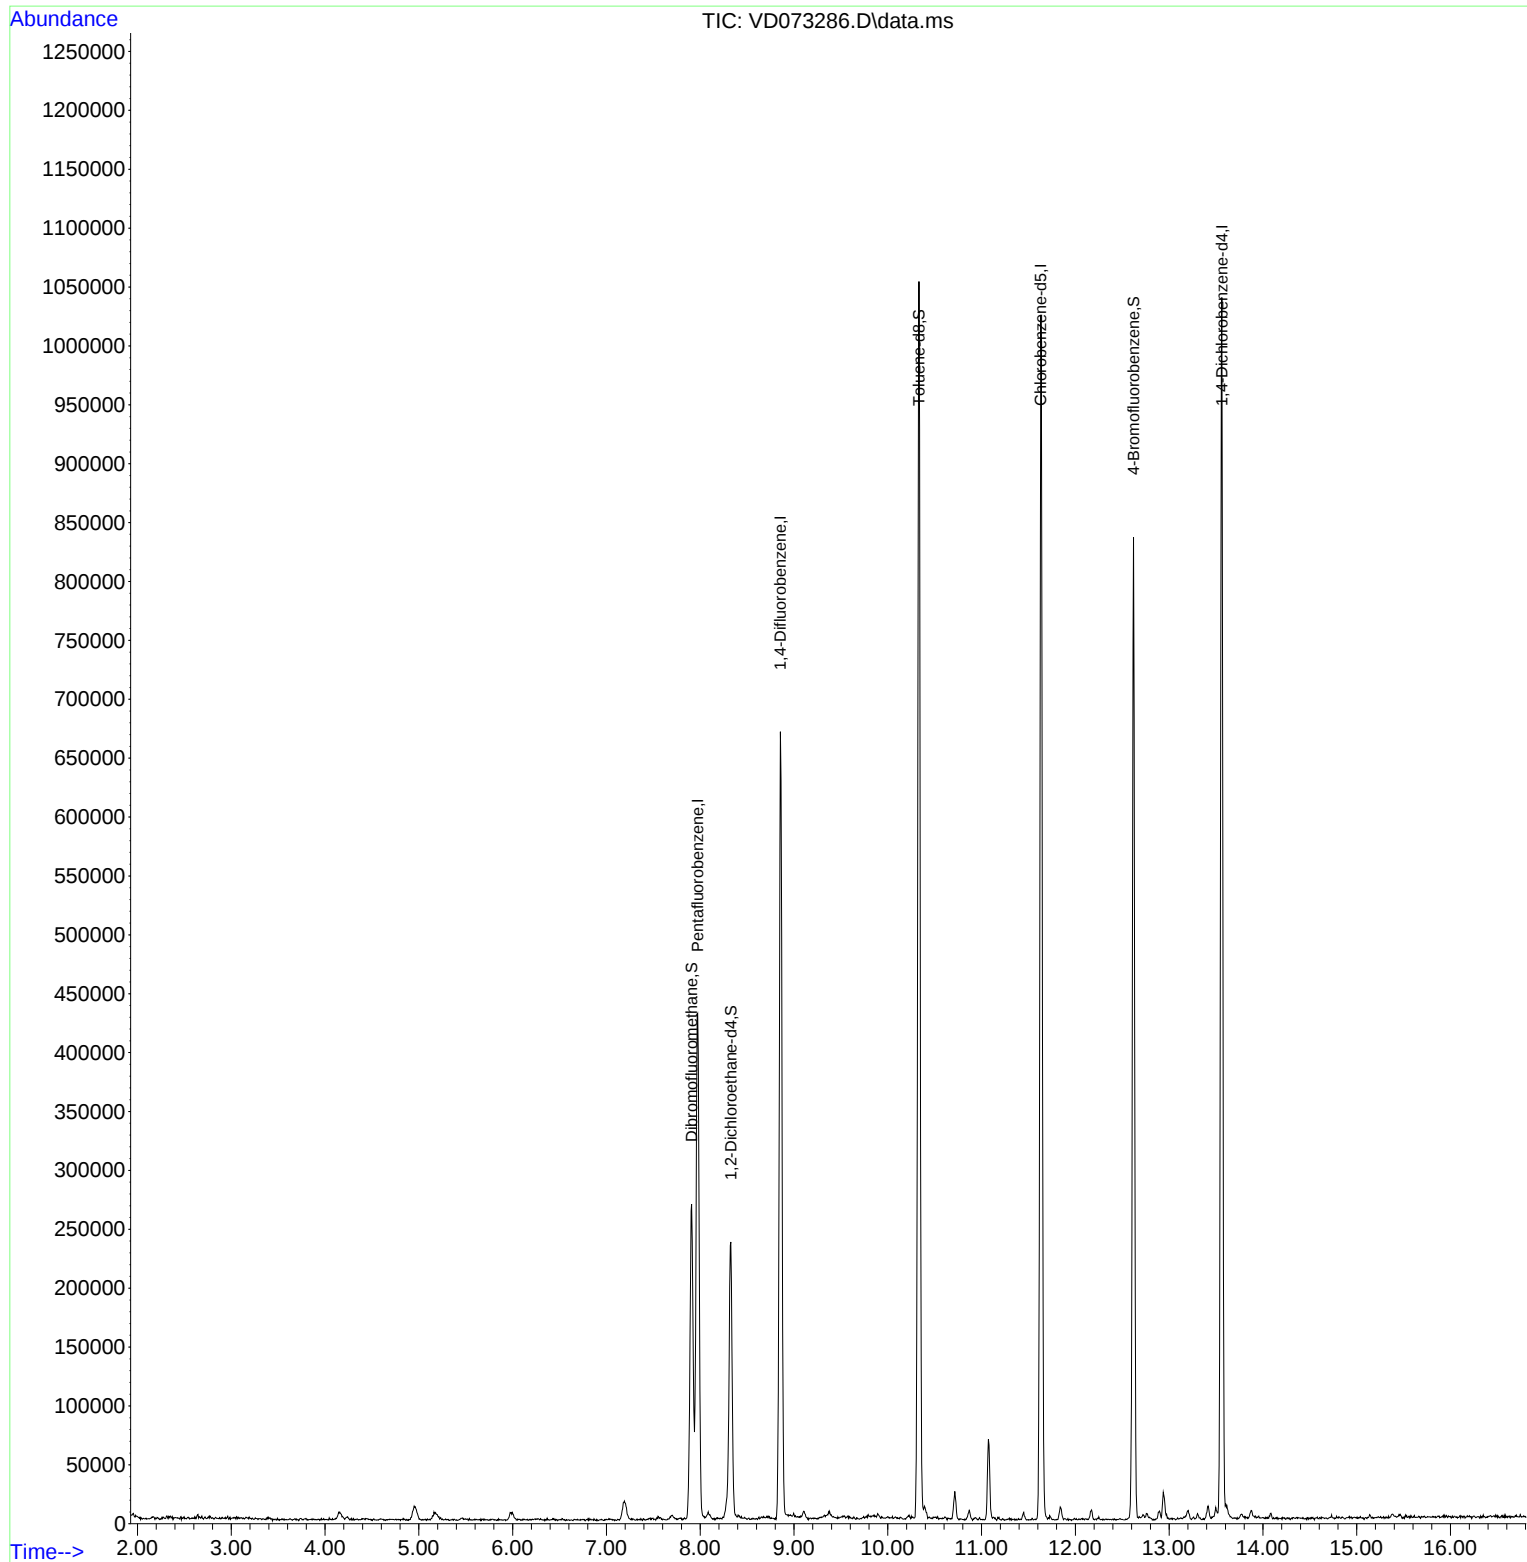


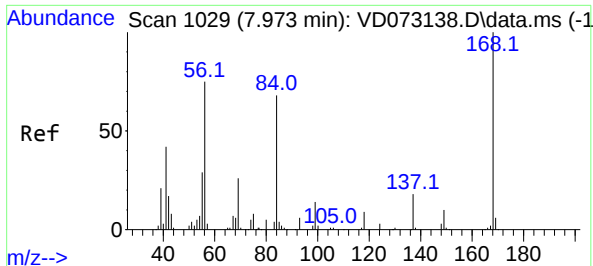

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.973 min Scan# 1029
Delta R.T. 0.000 min
Lab File: VD073286.D
Acq: 23 May 2022 16:44




Instrument :
MSVOA_D
ClientSampleId :
P033-SS001-1824-01


Tgt Ion:168 Resp: 320449
Ion Ratio Lower Upper
168 100
99 59.9 49.8 74.6

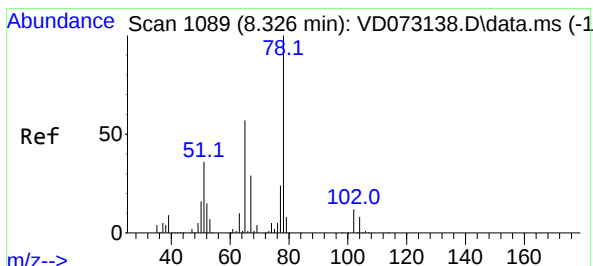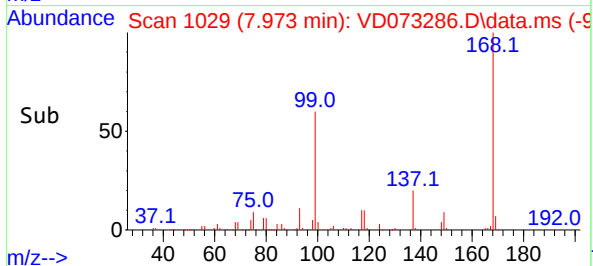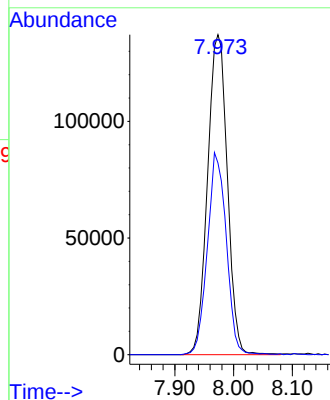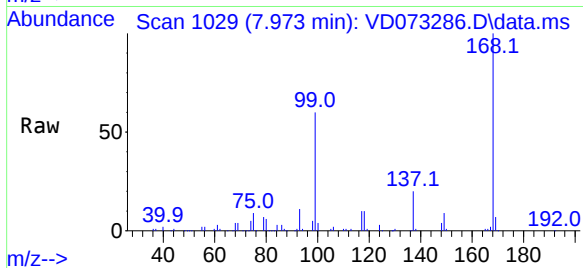

#33
1,2-Dichloroethane-d4
Concen: 50.958 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. 0.000 min
Lab File: VD073286.D
Acq: 23 May 2022 16:44

Tgt Ion: 65 Resp: 180464
Ion Ratio Lower Upper
65 100
67 52.5 0.0 101.4

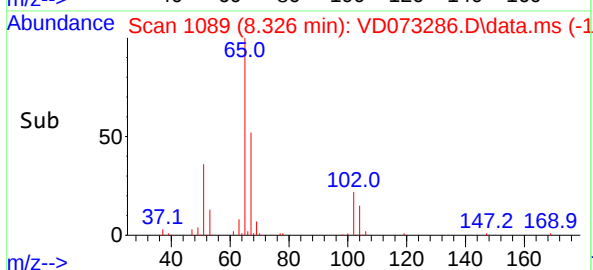
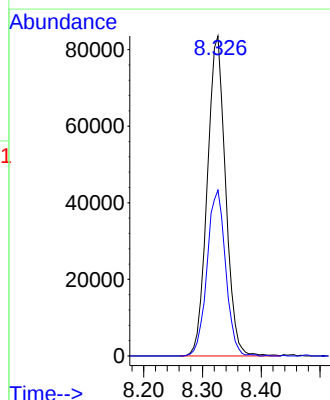
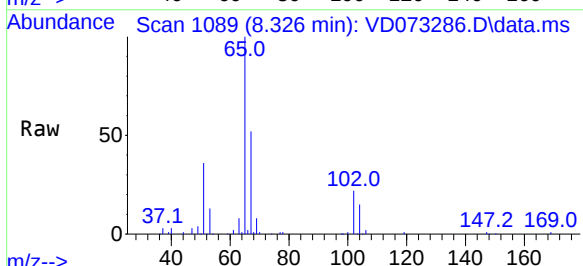


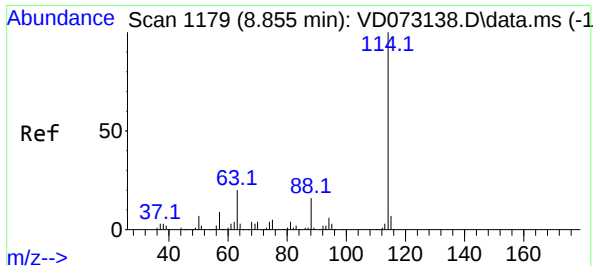

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.856 min Scan# 1179
Delta R.T. 0.001 min
Lab File: VD073286.D
Acq: 23 May 2022 16:44




Instrument :
MSVOA_D
ClientSampleId :
P033-SS001-1824-01

Tgt Ion:114 Resp: 569787
Ion Ratio Lower Upper
114 100
63 19.7 0.0 46.6
88 15.6 0.0 33.2

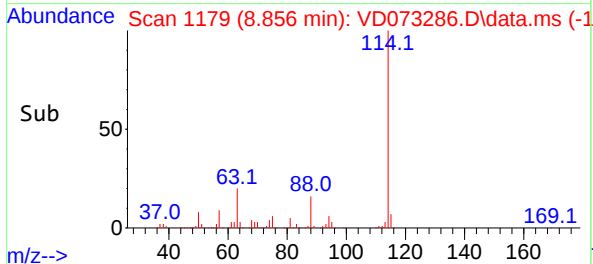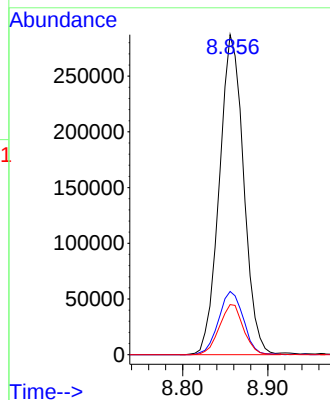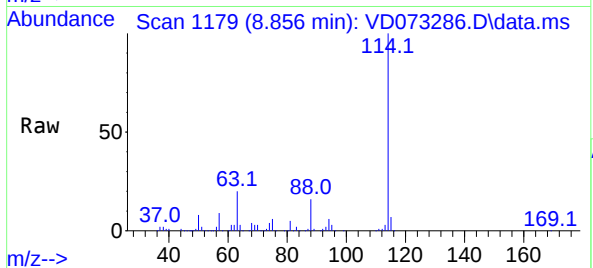

#35
Dibromofluoromethane
Concen: 51.540 ug/l
RT: 7.909 min Scan# 1018
Delta R.T. -0.005 min
Lab File: VD073286.D
Acq: 23 May 2022 16:44

Tgt Ion:113 Resp: 193783
Ion Ratio Lower Upper
113 100
111 104.1 83.8 125.6
192 17.8 14.6 21.8


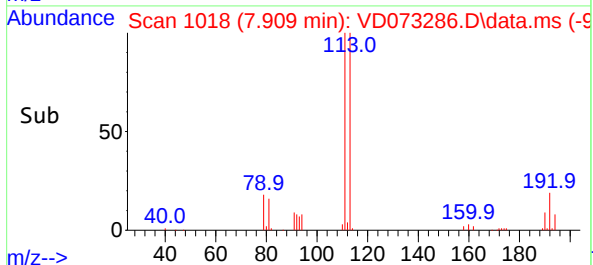
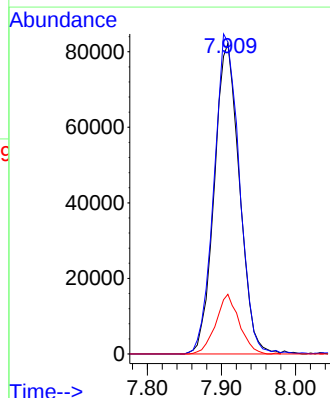
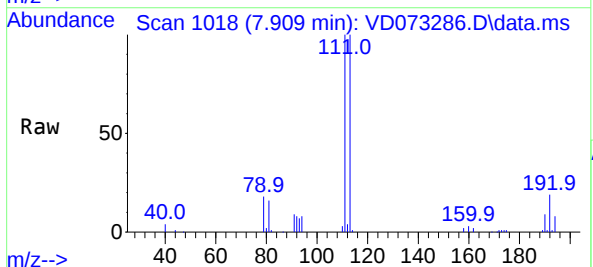




#50
Toluene-d8
Concen: 51.057 ug/l
RT: 10.332 min Scan# 1430
Delta R.T. -0.000 min
Lab File: VD073286.D
Acq: 23 May 2022 16:44




Instrument :
MSVOA_D
ClientSampleId :
P033-SS001-1824-01


Tgt Ion: 98 Resp: 707631
Ion Ratio Lower Upper
98 100
100 66.5 52.4 78.6

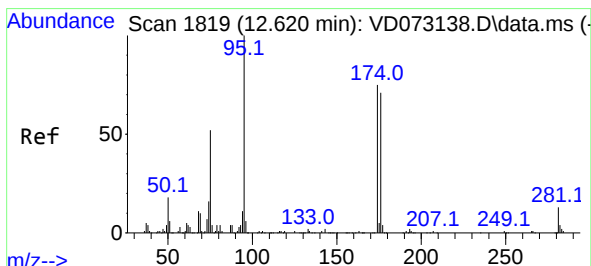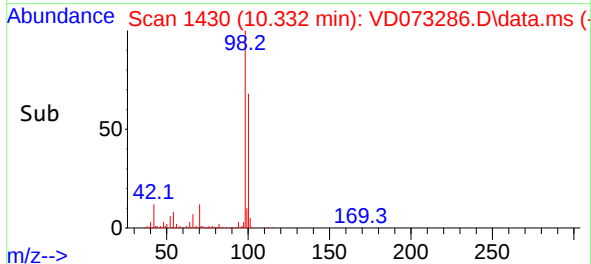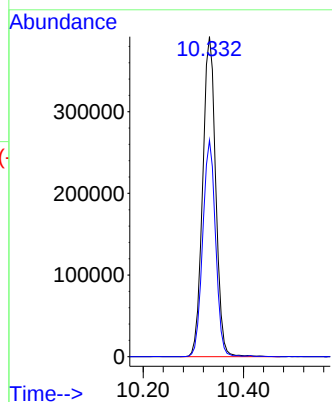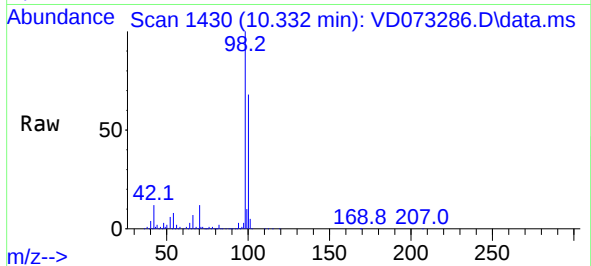

#62
4-Bromofluorobenzene
Concen: 54.716 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. 0.000 min
Lab File: VD073286.D
Acq: 23 May 2022 16:44

Tgt Ion: 95 Resp: 266134
Ion Ratio Lower Upper
95 100
174 78.6 0.0 152.8
176 73.1 0.0 145.4

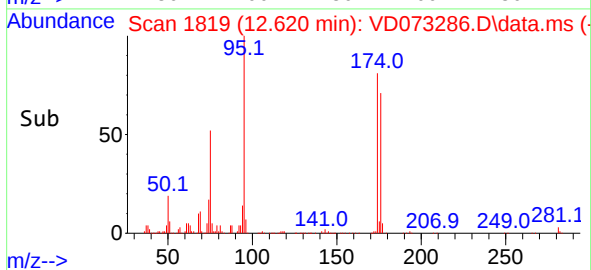
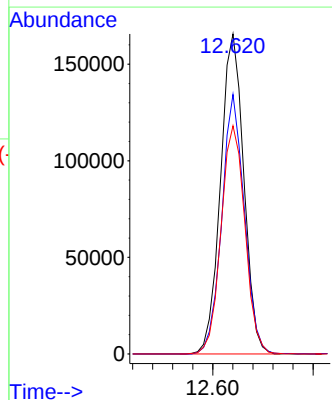
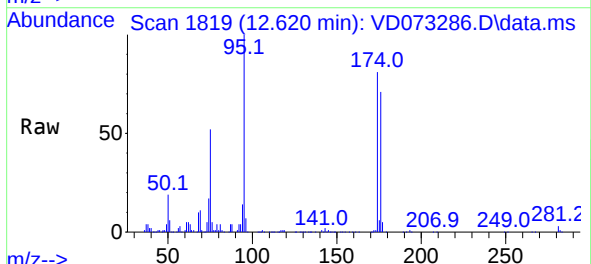


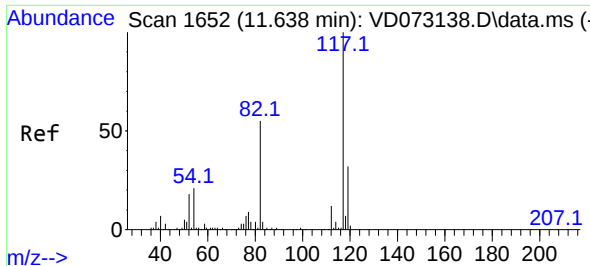

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.632 min Scan# 117
Delta R.T. -0.006 min
Lab File: VD073286.D
Acq: 23 May 2022 16:44

Instrument :
MSVOA_D
ClientSampleId :
P033-SS001-1824-01

Tgt Ion:117 Resp: 600928
Ion Ratio Lower Upper
117 100
82 56.5 45.3 67.9
119 32.0 26.6 40.0

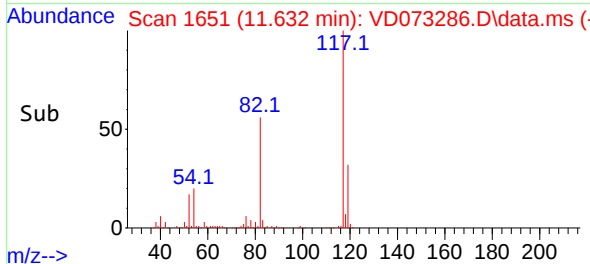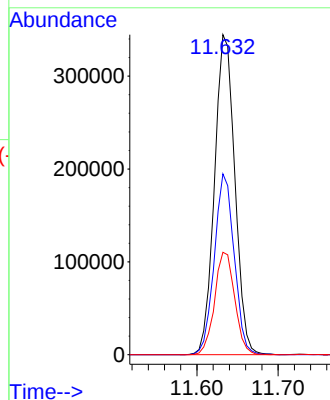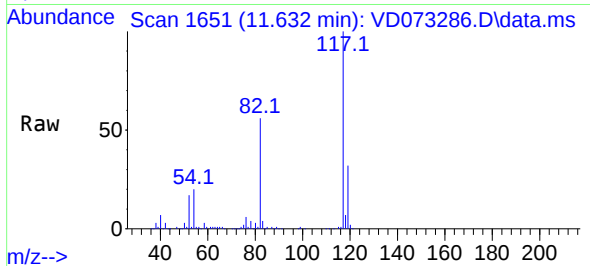

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. 0.000 min
Lab File: VD073286.D
Acq: 23 May 2022 16:44

Tgt Ion:152 Resp: 279405
Ion Ratio Lower Upper
152 100
115 61.2 31.3 93.8
150 159.8 0.0 348.6

