
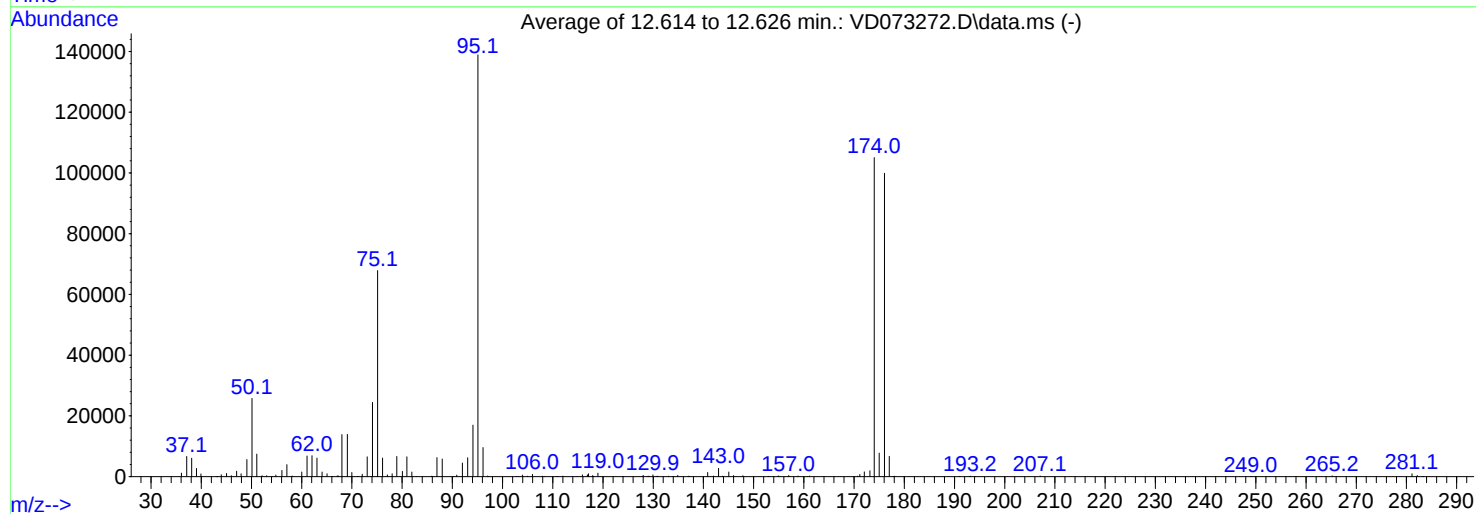


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052322\
Data File : VD073272.D
Acq On : 23 May 2022 08:48
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D051922S.M
Title : SW846 8260
Last Update : Thu May 19 15:13:42 2022

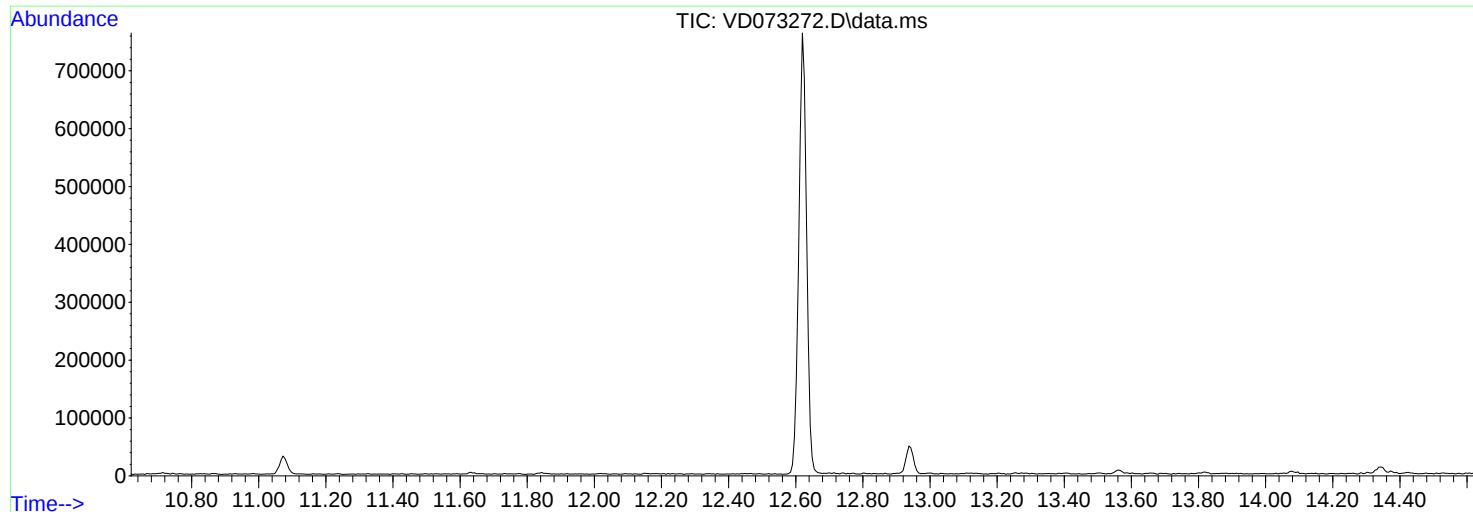

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1809

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.5	25755	PASS
75	95	30	60	48.9	67859	PASS
95	95	100	100	100.0	138891	PASS
96	95	5	9	6.9	9568	PASS
173	174	0.00	2	1.8	1943	PASS
174	95	50	100	75.6	105061	PASS
175	174	5	9	7.4	7766	PASS
176	174	95	101	95.1	99912	PASS
177	176	5	9	6.7	6691	PASS