




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052324\
Data File : VD079000.D
Acq On : 23 May 2024 13:18
Operator : RP/MD
Sample : P2570-02
Misc : 4.59G/10ml/MSVOA_D/SOIL/A
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BH6B0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/27/2024
Supervised By :Mahesh Dadoda 05/27/2024

Quant Time: May 24 02:14:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051724SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 24 02:12:30 2024
Response via : Initial Calibration

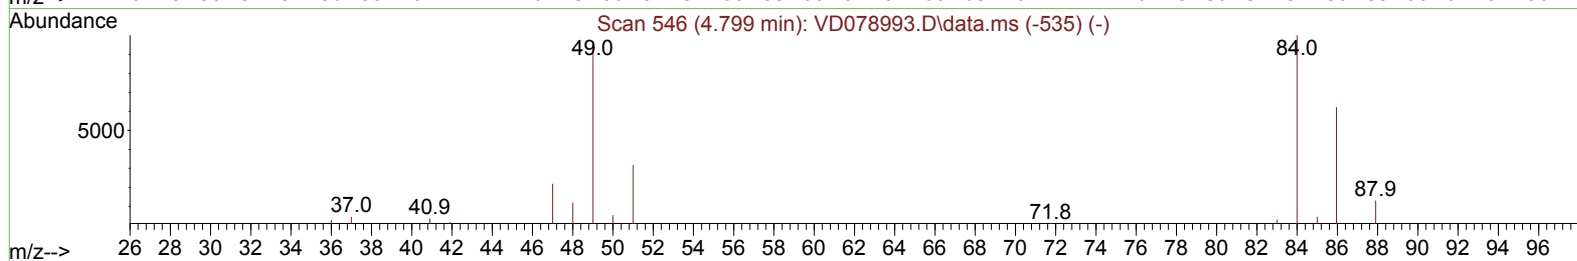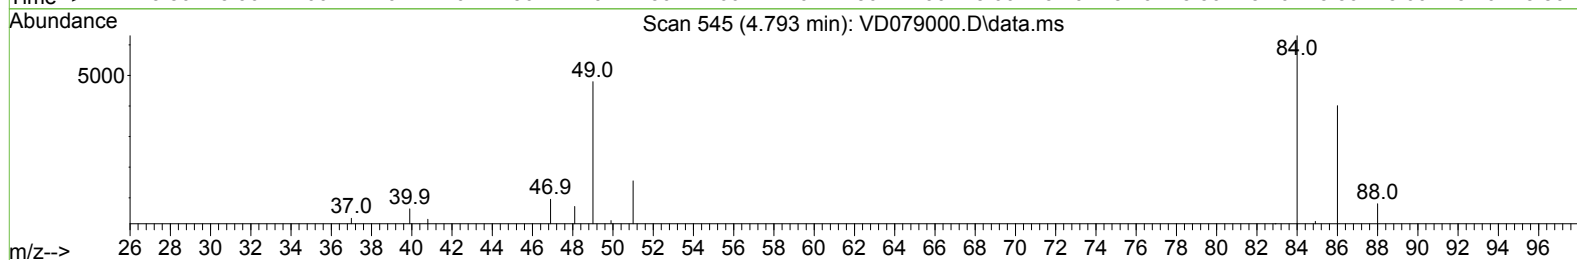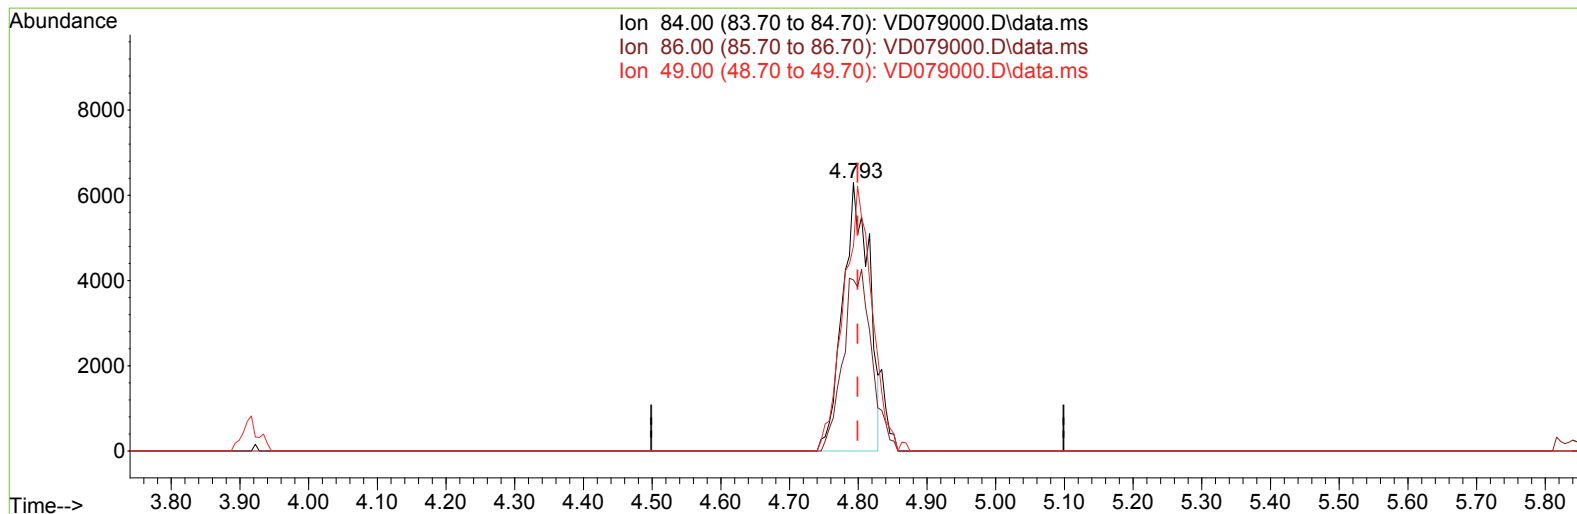

TIC: VD079000.D\data.ms

(16) Methylene chloride (T)

4.793min (-0.006) 6.58 ug/L

response 16714

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.40	63.72
49.00	91.50	76.20
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052324\
Data File : VD079000.D
Acq On : 23 May 2024 13:18
Operator : RP/MD
Sample : P2570-02
Misc : 4.59G/10ml/MSVOA_D/SOIL/A
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BH6B0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/27/2024
Supervised By :Mahesh Dadoda 05/27/2024

Quant Time: May 24 02:14:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051724SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 24 02:12:30 2024
Response via : Initial Calibration

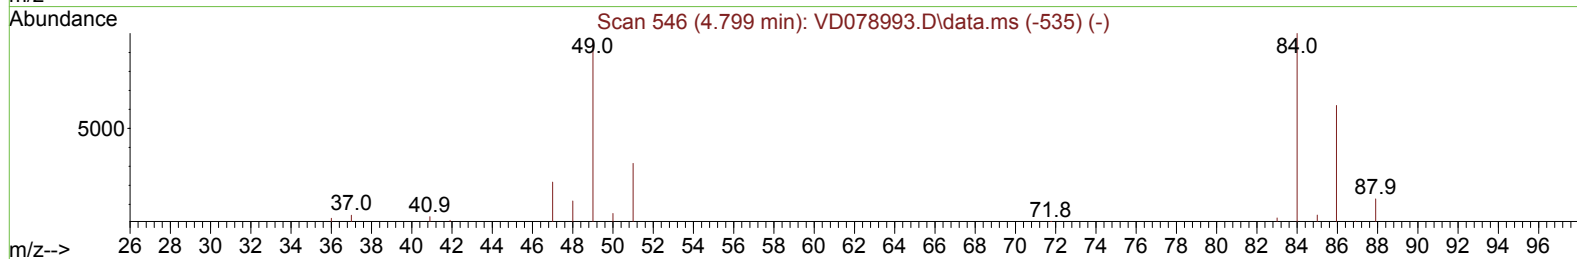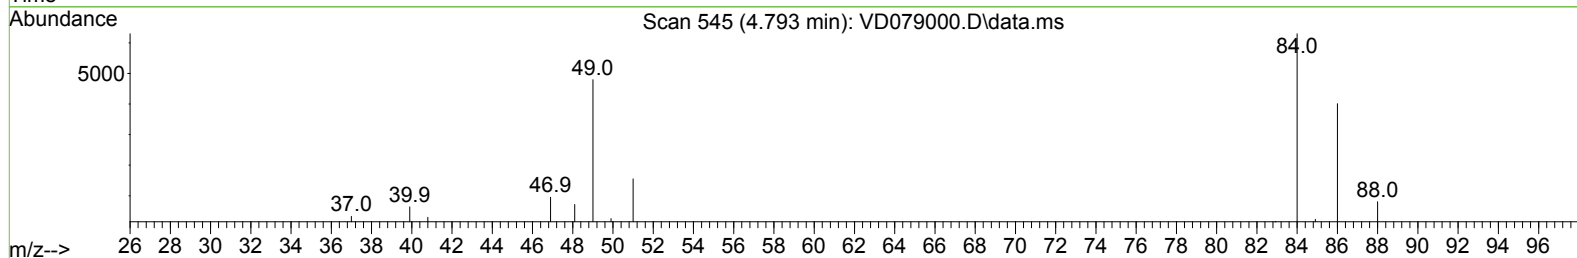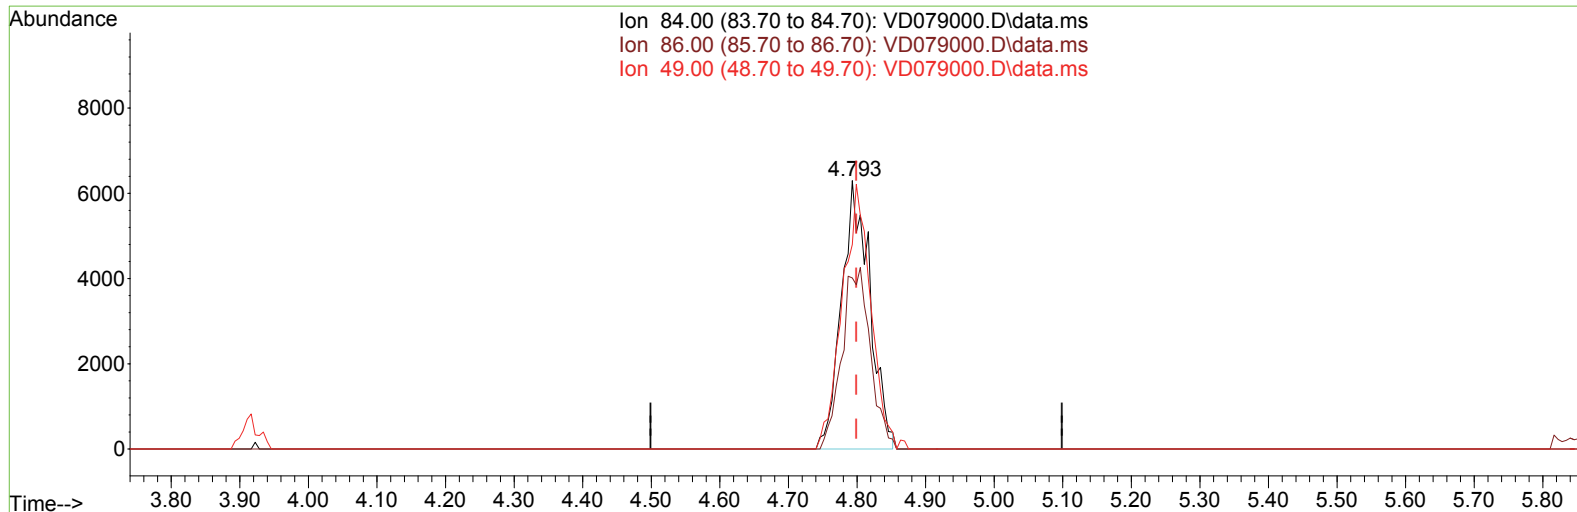

TIC: VD079000.D\data.ms

(16) Methylene chloride (T)

4.793min (-0.006) 7.09 ug/L m

response 18029

Ion	Exp%	Act%
84.00	100.00	100.00
86.00	62.40	63.72
49.00	91.50	76.20
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052324\
 Data File : VD079000.D
 Acq On : 23 May 2024 13:18
 Operator : RP/MD
 Sample : P2570-02
 Misc : 4.59G/10ml/MSVOA_D/SOIL/A
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BH6B0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/27/2024
 Supervised By :Mahesh Dadoda 05/27/2024

Quant Time: May 24 02:14:50 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 24 02:12:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.781	114	107312	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	102665	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152	35161	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.270	65	80431	30.574	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	122.280%
7) Chloroethane-d5	2.799	69	79565	28.254	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	113.000%
11) 1,1-Dichloroethene-d2	3.911	65	12497	24.353	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	97.400%
21) 2-Butanone-d5	6.987	46	13759	36.951	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	73.900%
24) Chloroform-d	7.569	84	72110	22.572	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.280%
26) 1,2-Dichloroethane-d4	8.228	65	38024	25.063	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	100.240%
32) Benzene-d6	8.199	84	140277	26.778	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	107.120%
36) 1,2-Dichloropropane-d6	9.210	67	42718	26.763	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	107.040%
41) Toluene-d8	10.269	98	118299	24.500	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.000%
43) trans-1,3-Dichloroprop...	10.522	79	17605	23.944	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	95.760%
47) 2-Hexanone-d5	10.881	63	11866	37.094	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	74.180%
56) 1,1,2,2-Tetrachloroeth...	12.646	84	38842	21.392	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	85.560%
66) 1,2-Dichlorobenzene-d4	13.816	152	30040	25.171	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.680%
Target Compounds						Qvalue
16) Methylene chloride	4.793	84	18029m	7.093	ug/L	
25) Chloroform	7.593	83	2542	0.666	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052324\
Data File : VD079000.D
Acq On : 23 May 2024 13:18
Operator : RP/MD
Sample : P2570-02
Misc : 4.59G/10ml/MSVOA_D/SOIL/A
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BH6B0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 05/27/2024
Supervised By :Mahesh Dadoda 05/27/2024

Quant Time: May 24 02:14:50 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051724SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 24 02:12:30 2024
Response via : Initial Calibration

