

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052324\
Data File : VD079002.D
Acq On : 23 May 2024 14:12
Operator : RP/MD
Sample : P2570-03
Misc : 4.02G/10ml/MSVOA_D/SOIL/A
ALS Vial : 12 Sample Multiplier: 1




Instrument :
MSVOA_D
ClientSampleId :
BH6B1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
Yesilyurt

05/27/2024
Supervised By :Mahesh
Dadoda
05/27/2024
Supervised By :Mahesh
Dadoda

Quant Time: May 24 02:15:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051724SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 24 02:12:30 2024
Response via : Initial Calibration

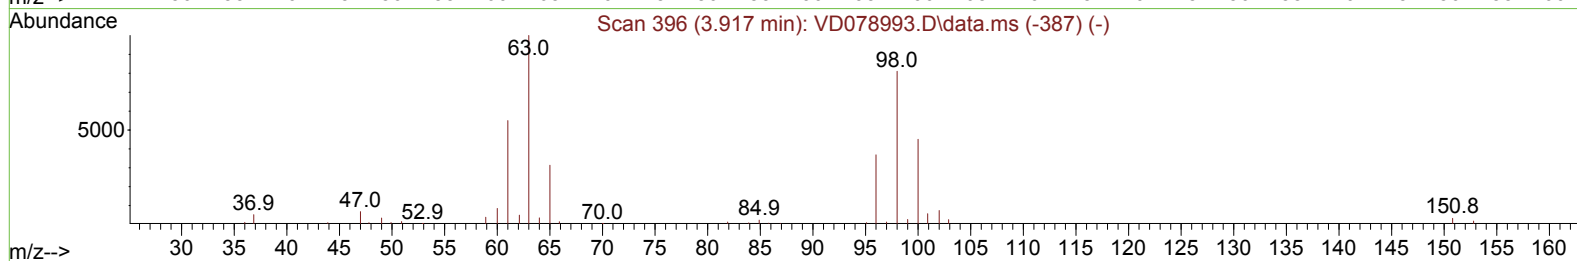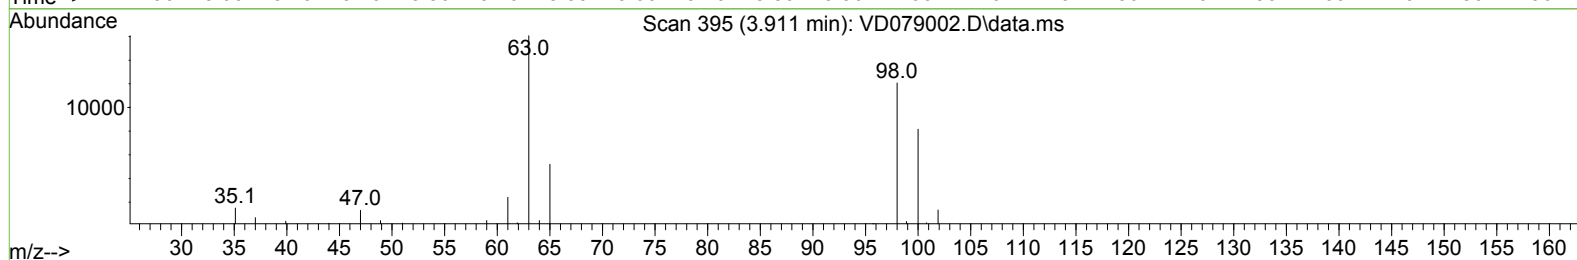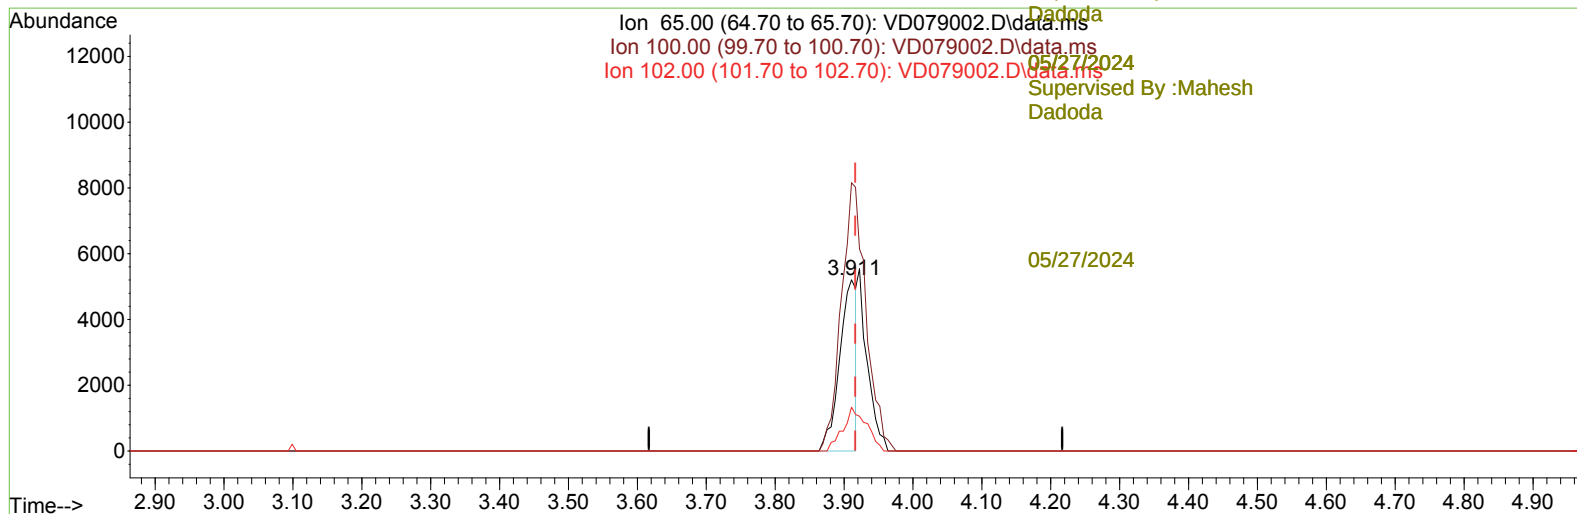

TIC: VD079002.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

3.911min (-0.006) 12.64 ug/L

response 8776

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	100.80	230.46#
102.00	11.10	35.85#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052324\
Data File : VD079002.D
Acq On : 23 May 2024 14:12
Operator : RP/MD
Sample : P2570-03
Misc : 4.02G/10ml/MSVOA_D/SOIL/A
ALS Vial : 12 Sample Multiplier: 1




Instrument :
MSVOA_D
ClientSampleId :
BH6B1

Manual IntegrationsAPPROVED

Quant Time: May 24 02:15:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051724SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 24 02:12:30 2024
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

05/27/2024
Supervised By :Mahesh
Dadoda
05/27/2024
Supervised By :Mahesh
Dadoda

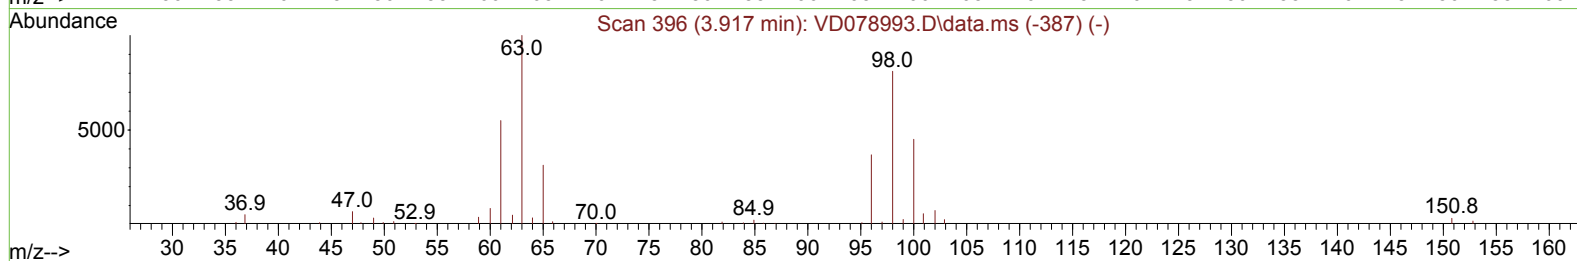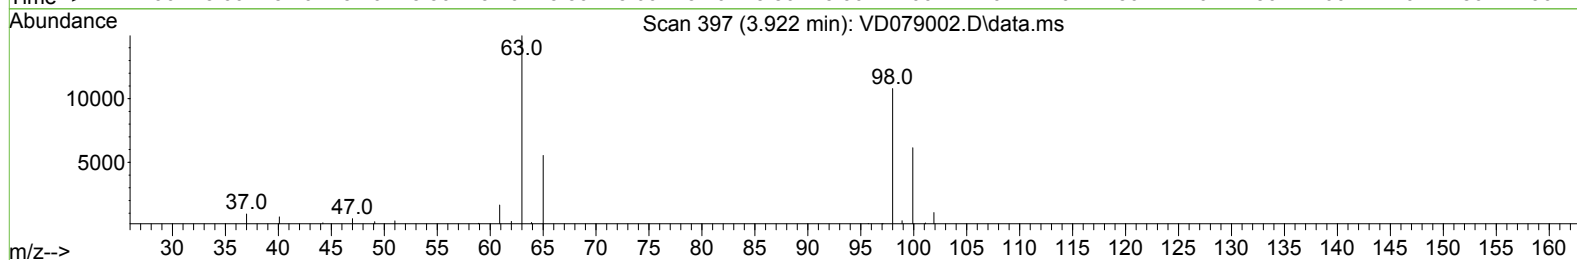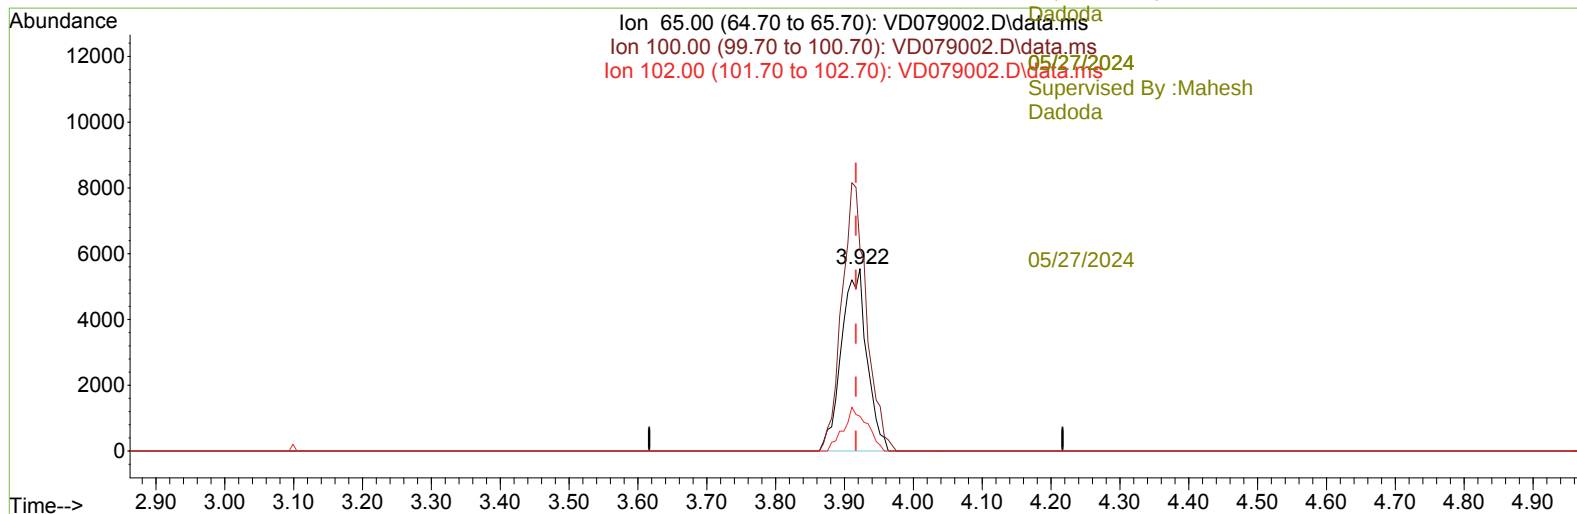

TIC: VD079002.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

3.922min (+ 0.006) 20.39 ug/L m

response 14162

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	100.80	142.81#
102.00	11.10	22.21#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052324\
Data File : VD079002.D
Acq On : 23 May 2024 14:12
Operator : RP/MD
Sample : P2570-03
Misc : 4.02G/10ml/MSVOA_D/SOIL/A
ALS Vial : 12 Sample Multiplier: 1




Instrument :
MSVOA_D
ClientSampleId :
BH6B1

Manual IntegrationsAPPROVED

Quant Time: May 24 02:15:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051724SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 24 02:12:30 2024
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

05/27/2024
Supervised By :Mahesh
Dadoda
05/27/2024
Supervised By :Mahesh
Dadoda

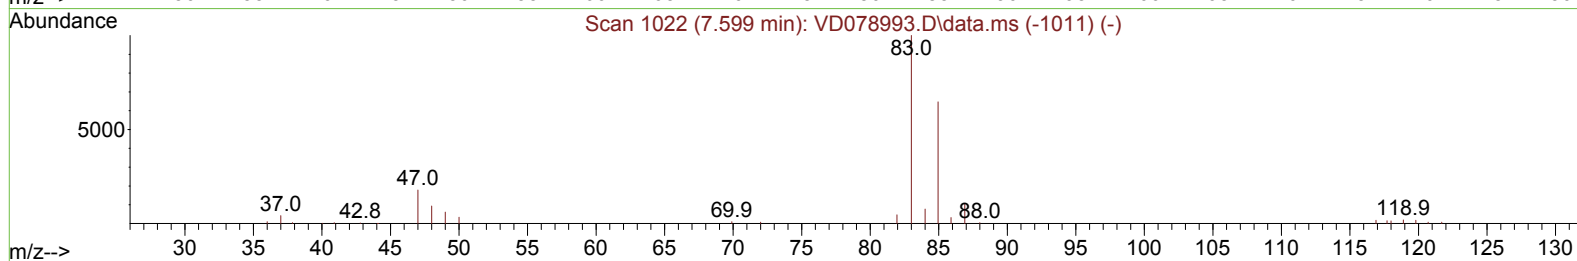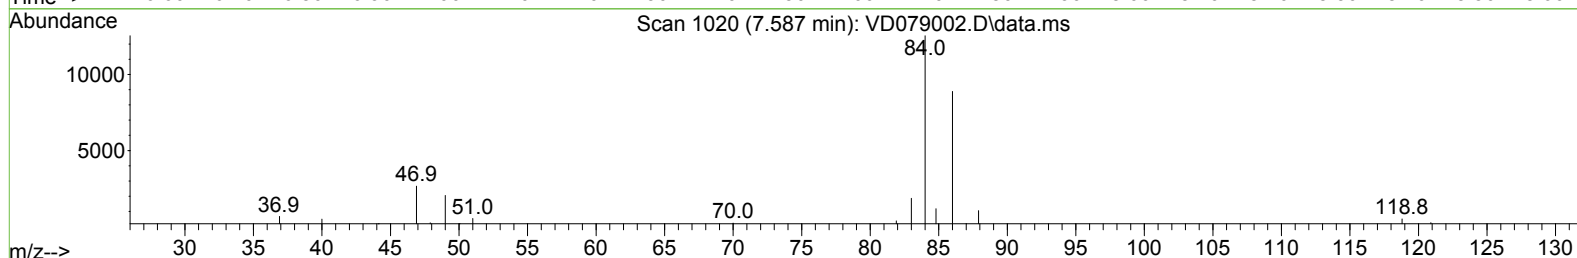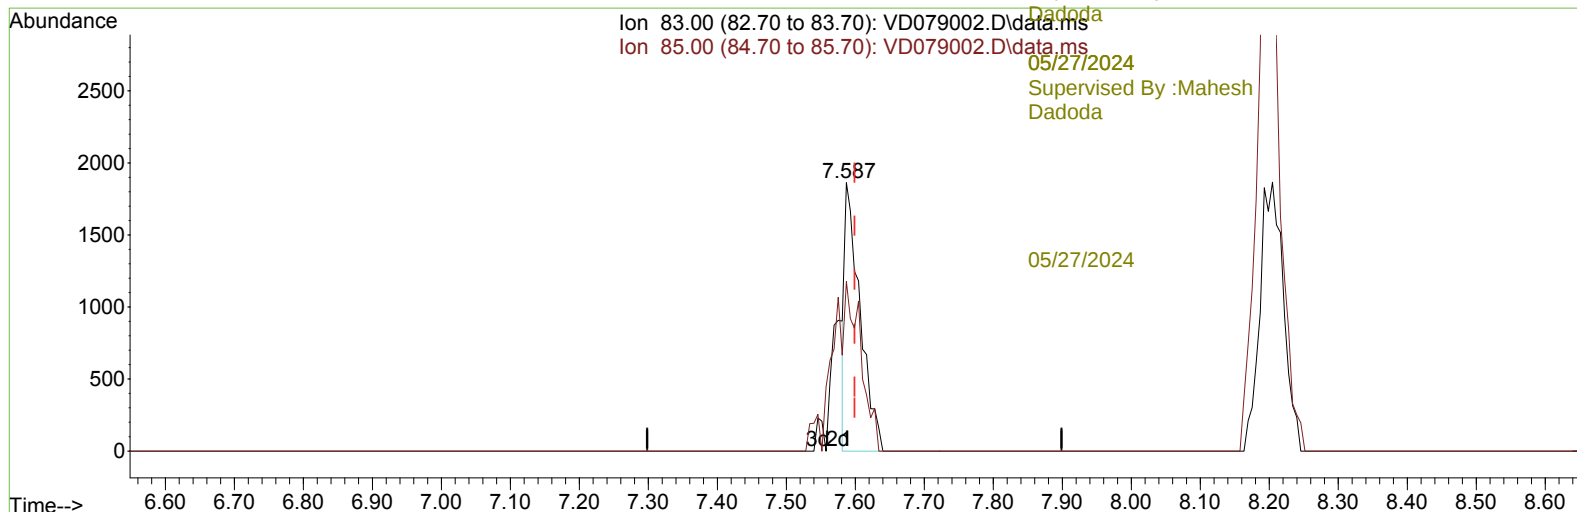

TIC: VD079002.D\data.ms

(25) Chloroform (T)

7.587min (-0.012) 0.55 ug/L

response 2852

Ion	Exp%	Act%
83.00	100.00	100.00
85.00	59.70	63.18
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052324\
Data File : VD079002.D
Acq On : 23 May 2024 14:12
Operator : RP/MD
Sample : P2570-03
Misc : 4.02G/10ml/MSVOA_D/SOIL/A
ALS Vial : 12 Sample Multiplier: 1




Instrument :
MSVOA_D
ClientSampleId :
BH6B1

Manual IntegrationsAPPROVED

Quant Time: May 24 02:15:24 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051724SMA.M
Quant Title : SFAM01.0
QLast Update : Fri May 24 02:12:30 2024
Response via : Initial Calibration

Reviewed By :Semsettin
Yesilyurt

05/27/2024
Supervised By :Mahesh
Dadoda
05/27/2024
Supervised By :Mahesh
Dadoda

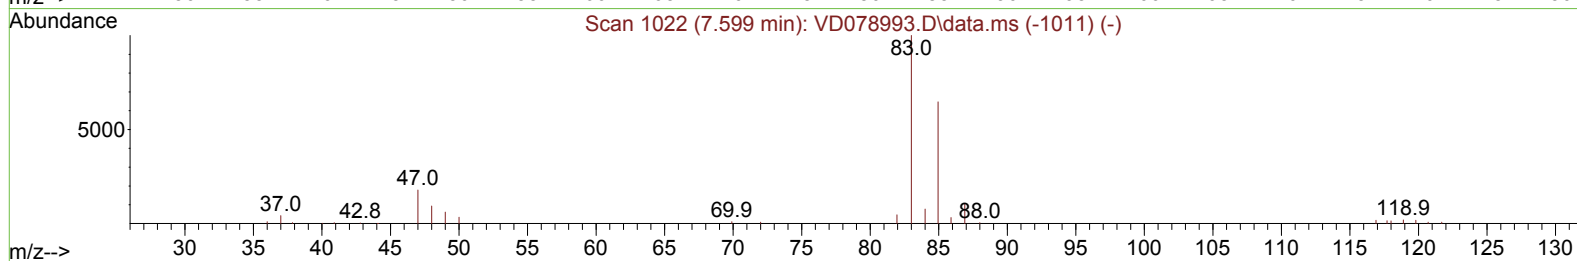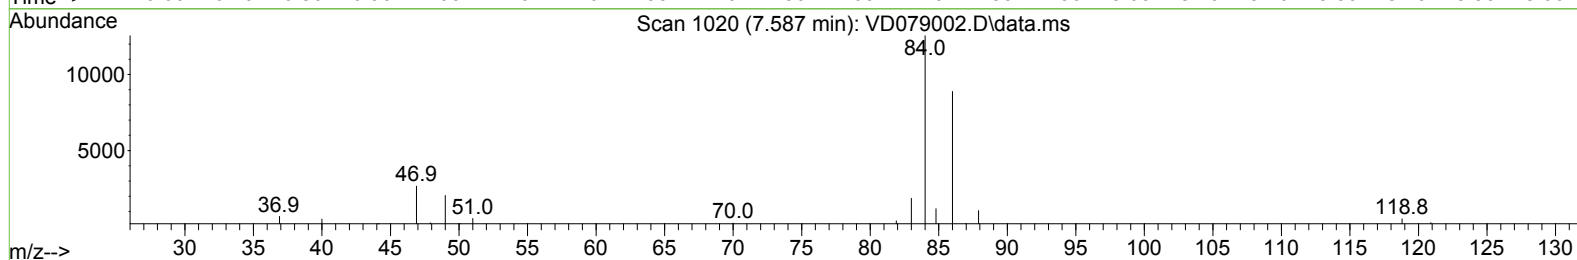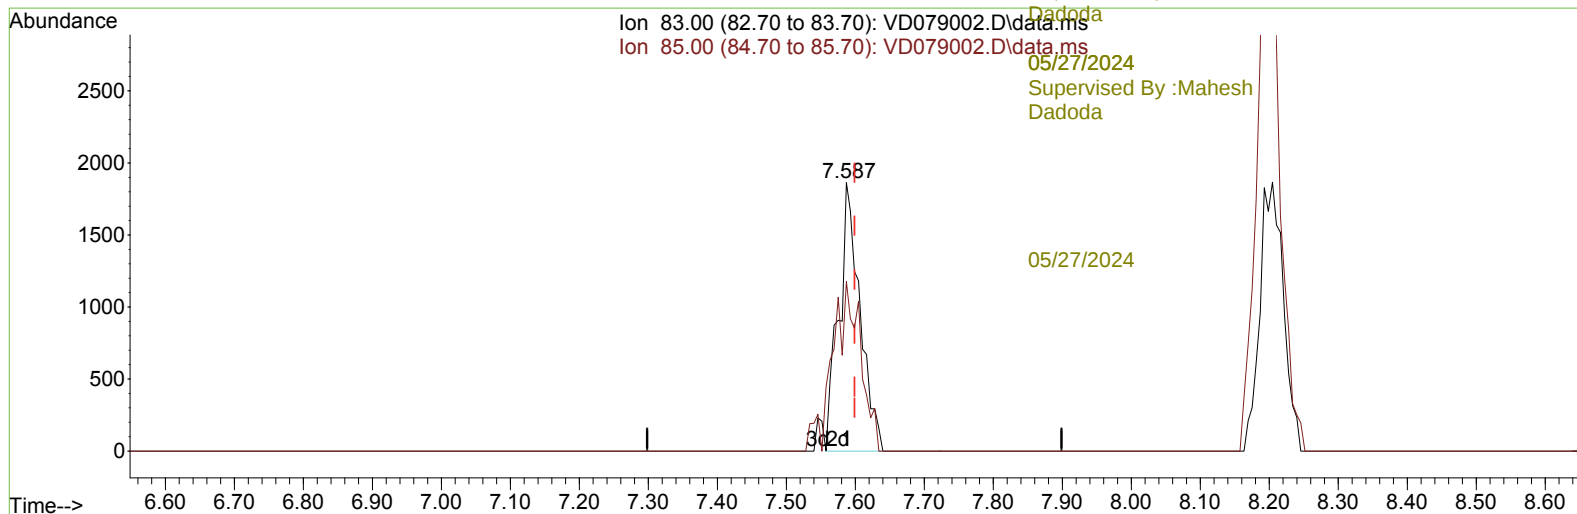

TIC: VD079002.D\data.ms

(25) Chloroform (T)

7.587min (-0.012) 0.77 ug/L m

response 3972

Ion	Exp%	Act%
83.00	100.00	100.00
85.00	59.70	63.18
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052324\
 Data File : VD079002.D
 Acq On : 23 May 2024 14:12
 Operator : RP/MD
 Sample : P2570-03
 Misc : 4.02G/10ml/MSVOA_D/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BH6B1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
 Yesilyurt

05/27/2024
 Supervised By :Mahesh
 Dadoda

05/27/2024
 Supervised By :Mahesh
 Dadoda

Quant Time: May 24 02:15:24 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051724SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri May 24 02:12:30 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)
Internal Standards							
1) 1,4-Difluorobenzene	8.781	114		145227	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117		135872	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152		44948	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.270	65		78594	22.076	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.320%	
7) Chloroethane-d5	2.799	69		85132	22.339	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.360%	
11) 1,1-Dichloroethene-d2	3.922	65		14162m	20.393	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	81.560%	
21) 2-Butanone-d5	6.987	46		13977	27.737	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	55.480%	
24) Chloroform-d	7.563	84		68531	15.851	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	63.400%	
26) 1,2-Dichloroethane-d4	8.234	65		36998	18.020	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	72.080%	
32) Benzene-d6	8.199	84		140621	20.283	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	81.120%	
36) 1,2-Dichloropropane-d6	9.204	67		42499	20.119	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	80.480%	
41) Toluene-d8	10.269	98		118922	18.609	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	74.440%	
43) trans-1,3-Dichloroprop...	10.522	79		17105	17.578	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	70.320%	
47) 2-Hexanone-d5	10.875	63		11110	26.242	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	52.480%	
56) 1,1,2,2-Tetrachloroeth...	12.651	84		39189	16.308	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	65.240%	
66) 1,2-Dichlorobenzene-d4	13.810	152		30448	19.958	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	79.840%	
Target Compounds							
16) Methylene chloride	4.793	84		18872	5.486	ug/L	87
25) Chloroform	7.587	83		3972m	0.769	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052324\
Data File : VD079002.D
Acq On : 23 May 2024 14:12
Operator : RP/MD
Sample : P2570-03
Misc : 4.02G/10ml/MSVOA_D/SOIL/A
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BH6B1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin
Yesilyurt

05/27/2024
Supervised By :Mahesh
Dadoda

05/27/2024
Supervised By :Mahesh
Dadoda

05/27/2024

