
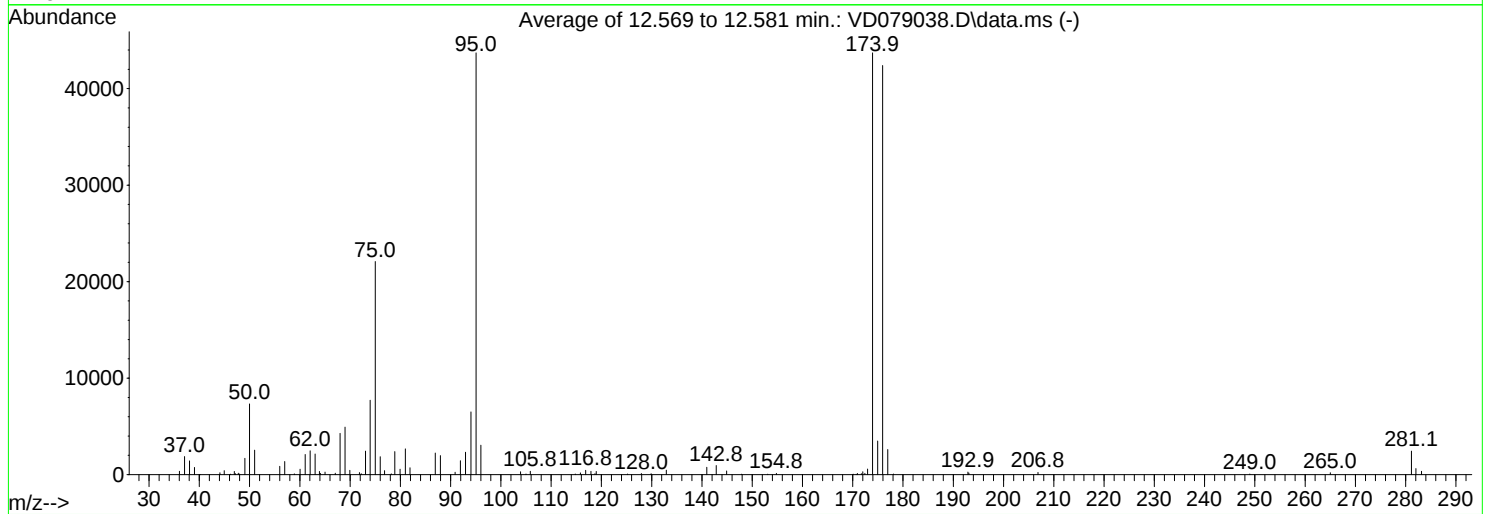


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD052824\
Data File : VD079038.D
Acq On : 28 May 2024 08:23
Operator : RP/MD
Sample : BFB216
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB216

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM051724SMA.M
Title : SFAM01.0
Last Update : Fri May 24 02:12:30 2024

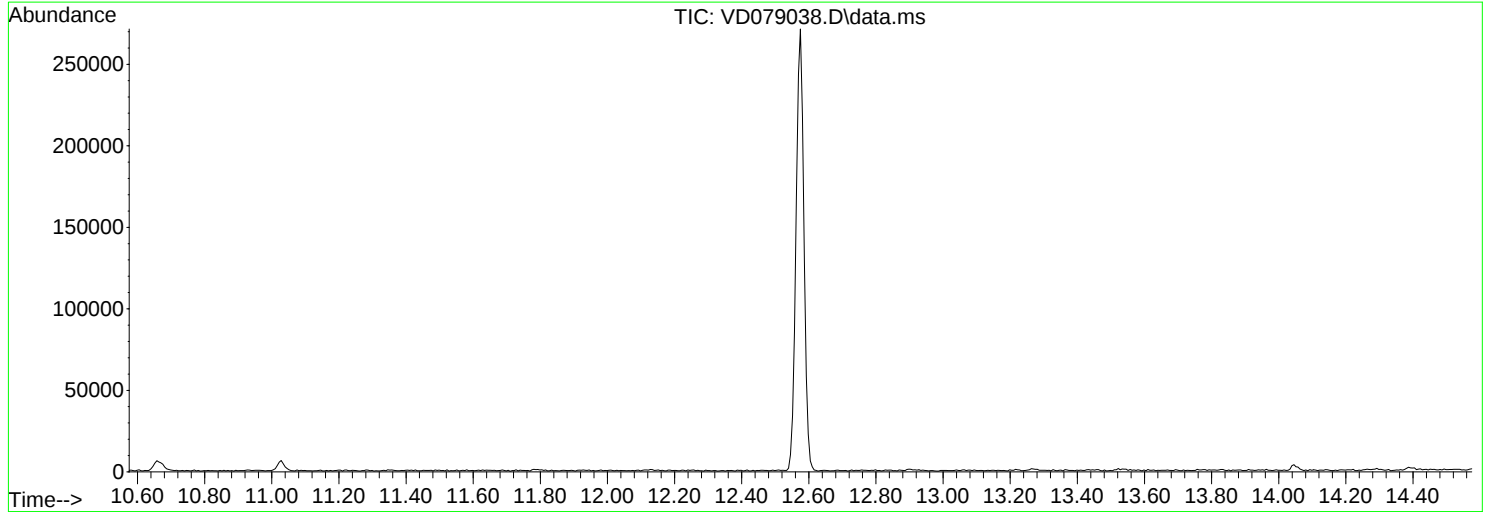

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.8	7323	PASS
75	95	30	80	50.5	22085	PASS
95	95	100	100	100.0	43696	PASS
96	95	5	9	7.0	3050	PASS
173	174	0.00	2	1.3	577	PASS
174	95	50	120	100.0	43707	PASS
175	174	5	9	8.0	3491	PASS
176	174	95	105	97.0	42389	PASS
177	176	5	10	6.1	2604	PASS

Scan 1859 (12.522 min): VD079038.D\data.ms
BFB216

m/z	Abundance
40.00	683.0
44.10	279.0

Instrument :
MSVOA_D
ClientSampleId :
BFB216

m/z	Abundance
36.10	364.0
37.00	1523.0
38.10	1577.0
39.00	947.0
40.00	573.0
44.10	404.0
44.90	435.0
46.90	460.0
47.80	275.0
49.10	1880.0
50.00	7279.0
50.90	2694.0
56.00	880.0
57.00	1409.0
60.00	536.0
61.10	2094.0
62.00	2350.0
63.10	2314.0
63.90	590.0
64.90	241.0
67.00	199.0
68.00	3943.0
69.00	4967.0
70.00	398.0
71.90	196.0
73.00	2353.0
74.00	7583.0
75.00	22888.0
76.00	2074.0
76.80	303.0
78.90	2499.0
80.00	697.0
81.00	2953.0
81.90	469.0
87.00	1934.0
88.00	2033.0
91.00	319.0
92.00	1584.0
92.90	2201.0
94.00	6829.0
95.10	44752.0
96.00	3534.0
104.00	240.0
105.90	408.0
115.80	310.0
116.90	371.0
117.90	439.0
119.00	319.0
132.90	213.0
140.90	849.0
142.80	1098.0
144.90	498.0
154.90	201.0
170.70	159.0
172.10	373.0
173.00	873.0
173.90	43656.0
175.00	3785.0
175.90	40096.0
177.00	3058.0
192.90	396.0
206.80	268.0
281.10	1945.0
282.00	351.0
283.20	432.0

Instrument :
MSVOA_D
ClientSampleId :
BFB216

m/z	Abundance
36.00	381.0
37.10	2685.0
38.00	1245.0
39.00	634.0
40.00	858.0
44.10	529.0
45.00	560.0
46.20	161.0
47.20	286.0
47.70	191.0
49.00	2113.0
50.00	8175.0
51.00	2825.0
56.00	962.0
57.00	1463.0
58.90	235.0
60.10	698.0
61.00	2686.0
62.10	2855.0
63.00	2141.0
64.10	390.0
65.00	309.0
67.10	271.0
68.00	5089.0
69.00	5474.0
70.00	458.0
71.80	280.0
72.20	284.0
73.00	2734.0
74.00	8722.0
75.00	23400.0
76.00	1945.0
76.90	751.0
78.20	242.0
78.90	2578.0
80.00	647.0
81.00	3121.0
81.90	809.0
86.90	2596.0
87.90	2194.0
90.90	258.0
91.90	1575.0
93.00	2915.0
94.00	7319.0
95.00	48920.0
96.00	3342.0
103.90	424.0
105.00	189.0
105.80	334.0
115.80	237.0
116.90	660.0
117.80	172.0
118.90	665.0
128.00	180.0
132.90	526.0
140.90	814.0
142.90	943.0
144.90	473.0
147.90	166.0
154.70	209.0
171.00	204.0
171.90	511.0
172.90	487.0
174.00	47048.0
174.90	3796.0
176.00	48448.0
176.90	2369.0
178.10	215.0
193.10	512.0
206.90	240.0
265.00	324.0
281.10	2096.0
282.10	771.0
283.20	339.0

Instrument :
MSVOA_D
ClientSampleId :
BFB216

m/z	Abundance
36.00	303.0
37.00	1418.0
38.00	1437.0
39.10	650.0
40.10	624.0
44.10	525.0
44.90	261.0
47.00	558.0
48.00	198.0
49.10	1062.0
50.00	6516.0
51.10	2105.0
56.00	756.0
57.00	1209.0
60.00	464.0
61.00	1468.0
62.10	2220.0
63.00	1953.0
63.90	386.0
65.10	246.0
68.00	3815.0
69.00	4353.0
69.90	481.0
71.90	190.0
73.10	2236.0
74.00	6823.0
75.00	19968.0
76.00	1540.0
76.70	169.0
78.90	2071.0
79.80	354.0
80.90	1950.0
81.70	444.0
82.00	421.0
87.00	2187.0
88.00	1695.0
90.80	176.0
92.00	1155.0
93.00	1840.0
94.10	5332.0
95.00	37416.0
96.00	2275.0
103.80	240.0
105.80	299.0
114.80	218.0
116.70	315.0
118.00	424.0
118.70	318.0
125.20	188.0
127.90	173.0
129.90	284.0
132.90	658.0
141.00	625.0
142.80	814.0
145.00	162.0
153.10	151.0
170.10	157.0
170.90	155.0
171.70	302.0
172.40	409.0
173.00	371.0
174.00	40416.0
174.90	2893.0
175.90	38624.0
177.00	2386.0
192.90	390.0
206.90	193.0
249.00	225.0
265.00	277.0
281.20	3263.0
282.10	785.0
283.00	292.0

Instrument :
MSVOA_D
ClientSampleId :
BFB216