


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD053025\
Data File : VD080393.D
Acq On : 30 May 2025 08:28
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D053025S.M
Title : SW846 8260
Last Update : Sat May 31 01:10:05 2025

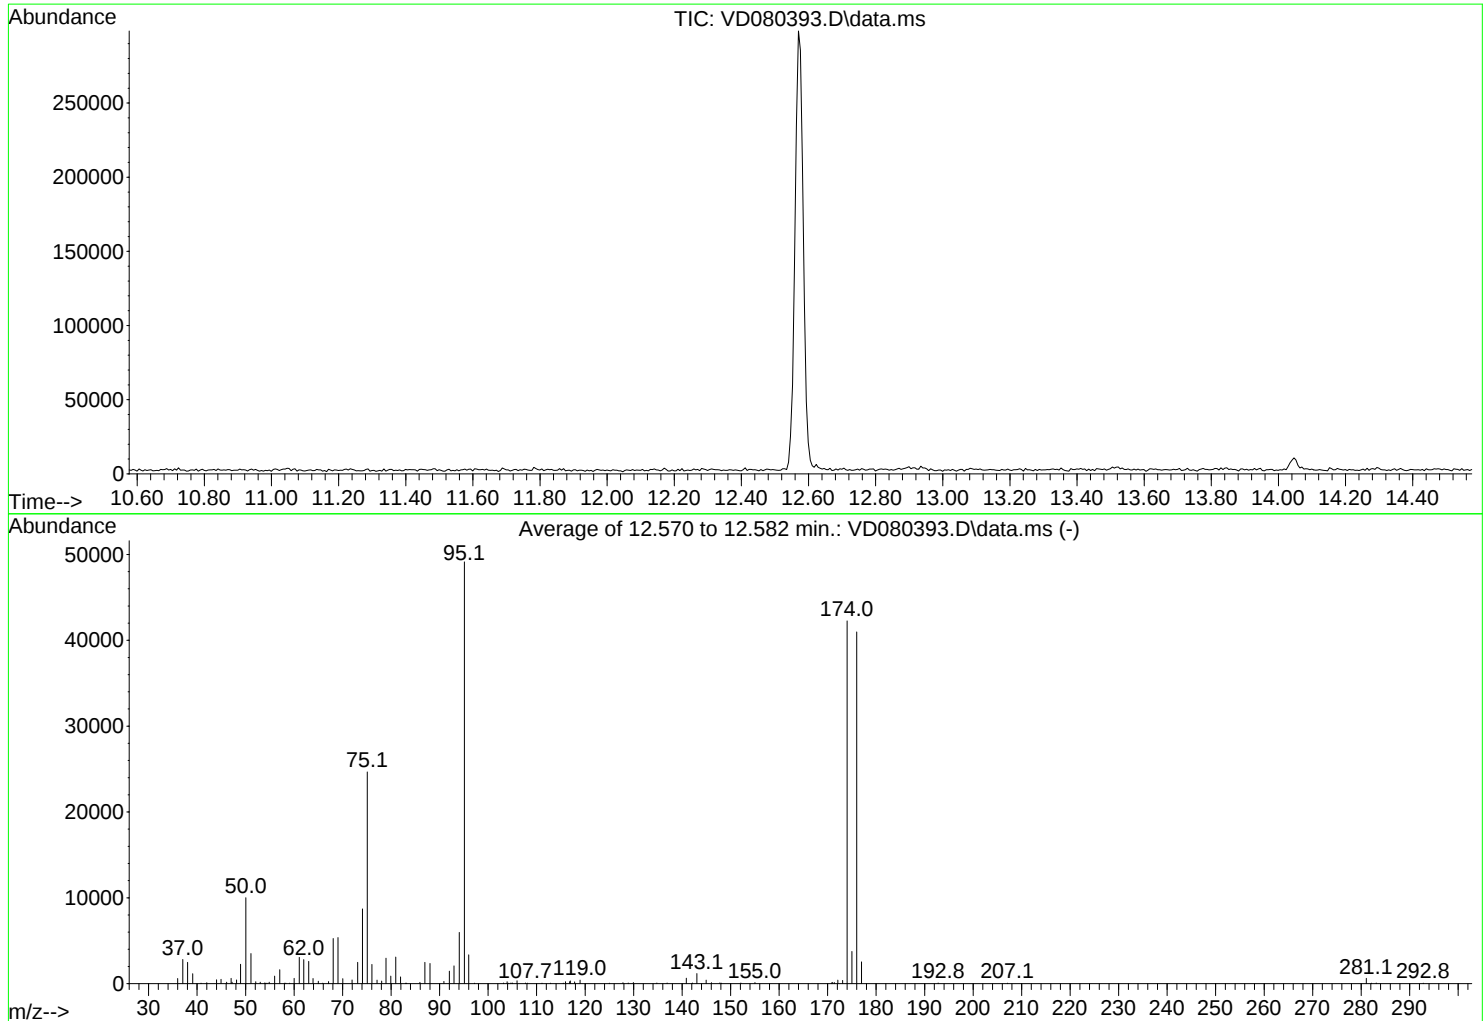

AutoFind: Scans 1836, 1837, 1838; Background Corrected with Scan 1827

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	10002	PASS
75	95	30	60	50.2	24659	PASS
95	95	100	100	100.0	49144	PASS
96	95	5	9	6.8	3356	PASS
173	174	0.00	2	0.9	372	PASS
174	95	50	100	86.0	42267	PASS
175	174	5	9	8.9	3748	PASS
176	174	95	101	96.9	40971	PASS
177	176	5	9	6.2	2530	PASS