

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD060324\
 Data File : VD079118.D
 Acq On : 03 Jun 2024 12:43
 Operator : RP/MD
 Sample : P2642-20
 Misc : 5.50G/10ml/MSVOA_D/SOIL/A
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 A4B32

Quant Time: Jun 04 05:05:18 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM052924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Jun 01 00:34:30 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.775	114	306515	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	273698	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152	91642	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.275	65	133688	14.173	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	56.680%
7) Chloroethane-d5	2.799	69	146961	16.113	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.440%
11) 1,1-Dichloroethene-d2	3.911	65	25900	15.468	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	61.880%
21) 2-Butanone-d5	6.981	46	21575	29.905	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	59.800%
24) Chloroform-d	7.569	84	143583	16.754	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	67.000%
26) 1,2-Dichloroethane-d4	8.222	65	67226	17.004	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	68.000%#
32) Benzene-d6	8.199	84	289916	19.108	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	76.440%
36) 1,2-Dichloropropane-d6	9.210	67	85797	19.630	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	78.520%
41) Toluene-d8	10.269	98	249366	17.553	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	70.200%
43) trans-1,3-Dichloroprop...	10.522	79	32198	17.527	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	70.120%
47) 2-Hexanone-d5	10.875	63	17886	31.655	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	63.320%
56) 1,1,2,2-Tetrachloroeth...	12.645	84	62273	16.086	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	64.360%
66) 1,2-Dichlorobenzene-d4	13.816	152	65889	20.833	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	83.320%
Target Compounds						
25) Chloroform	7.593	83	9735	1.161	ug/L	Qvalue 88


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD060324\
Data File : VD079118.D
Acq On : 03 Jun 2024 12:43
Operator : RP/MD
Sample : P2642-20
Misc : 5.50G/10ml/MSVOA_D/SOIL/A
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
A4B32

Quant Time: Jun 04 05:05:18 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM052924SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Jun 01 00:34:30 2024
Response via : Initial Calibration

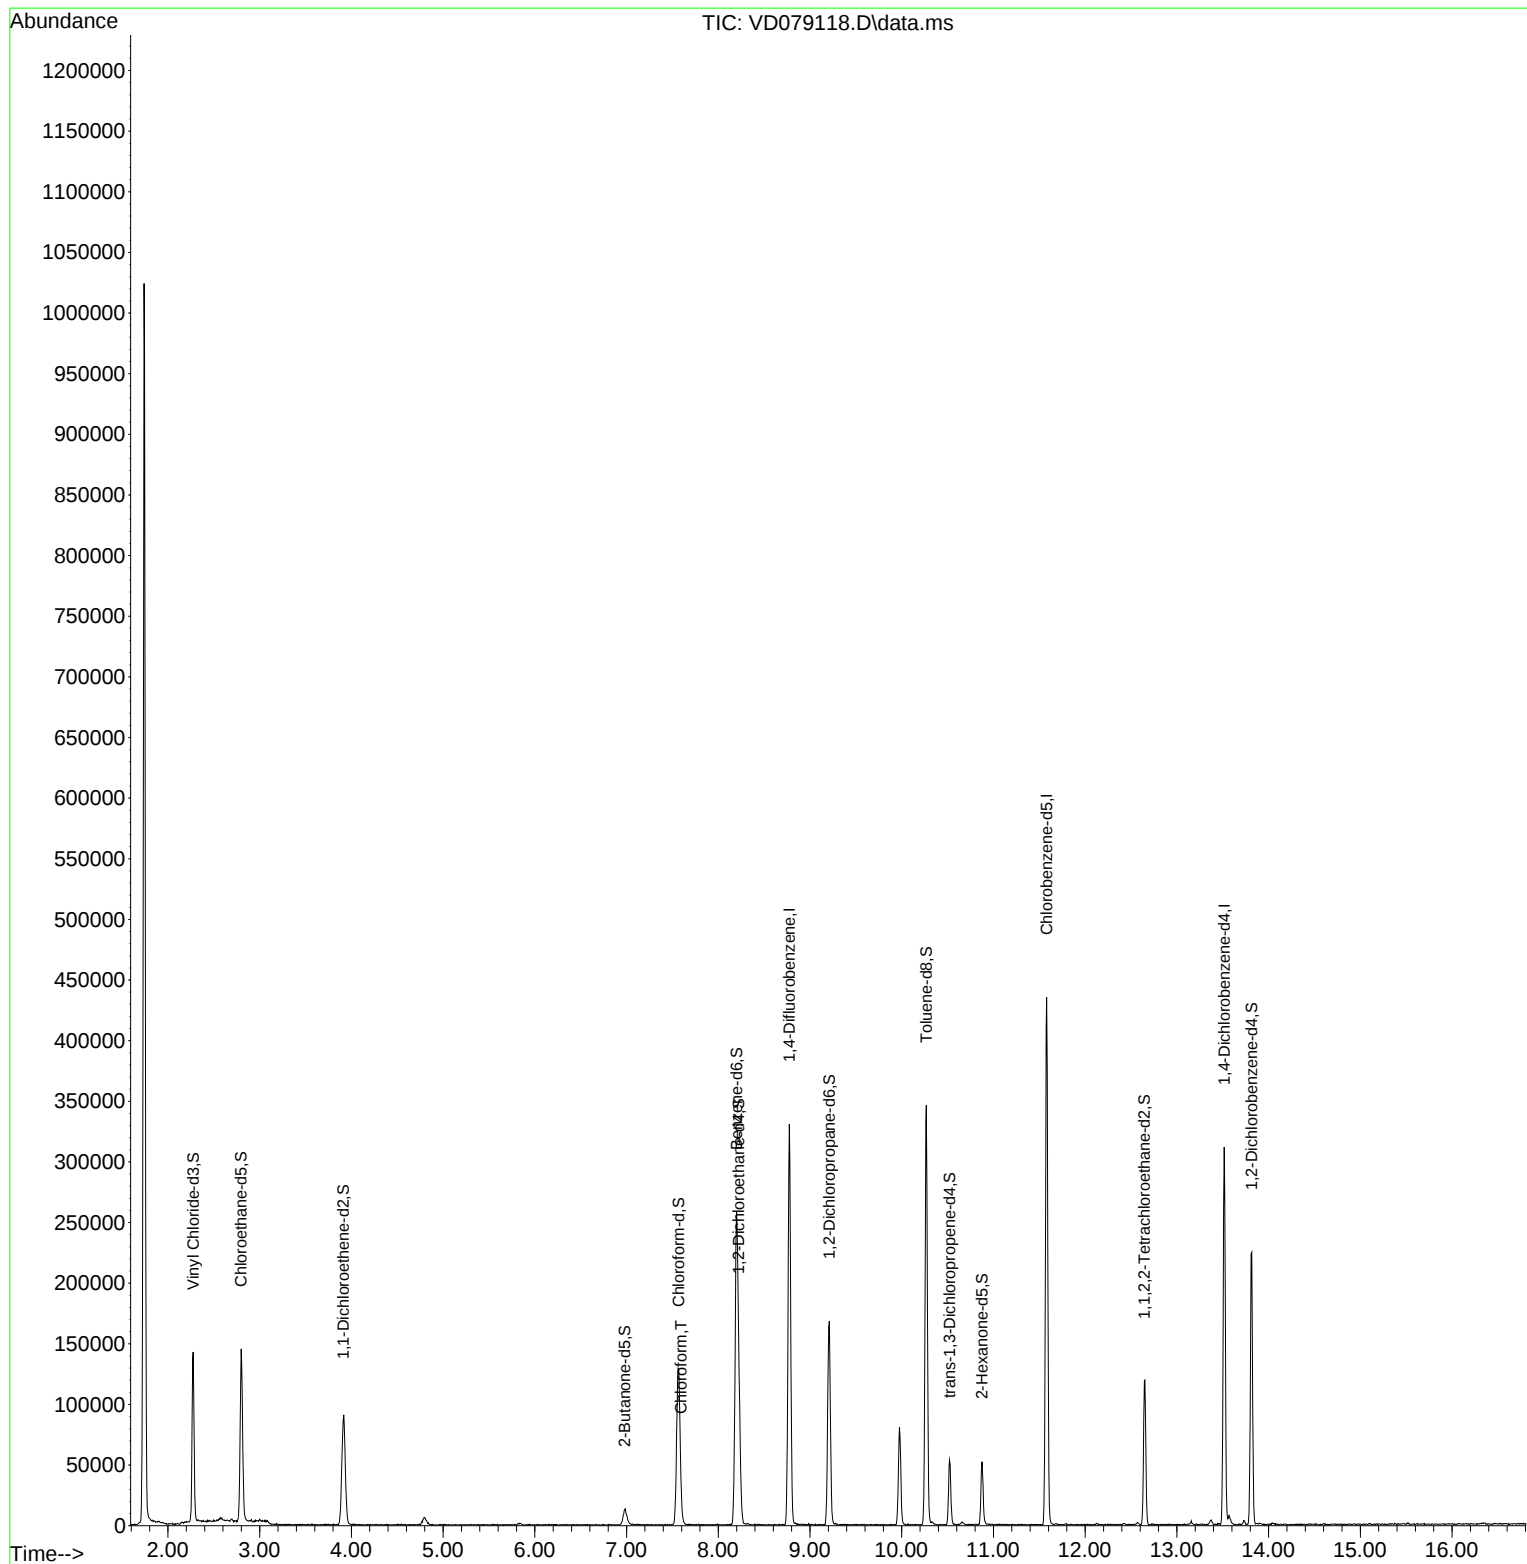

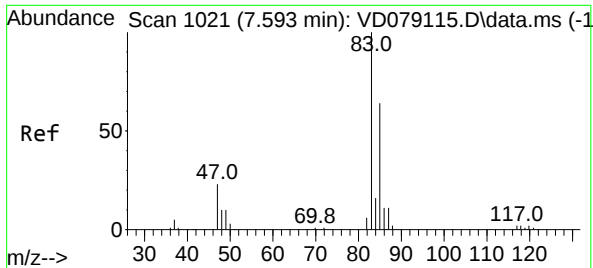

#25
 Chloroform
 Concen: 1.161 ug/L
 RT: 7.593 min Scan# 10
 Delta R.T. 0.000 min
 Lab File: VD079118.D
 Acq: 03 Jun 2024 12:43

Instrument :
 MSVOA_D
 ClientSampleId :
 A4B32

Tgt Ion: 83 Resp: 9735
 Ion Ratio Lower Upper
 83 100
 85 58.7 47.9 89.1

