
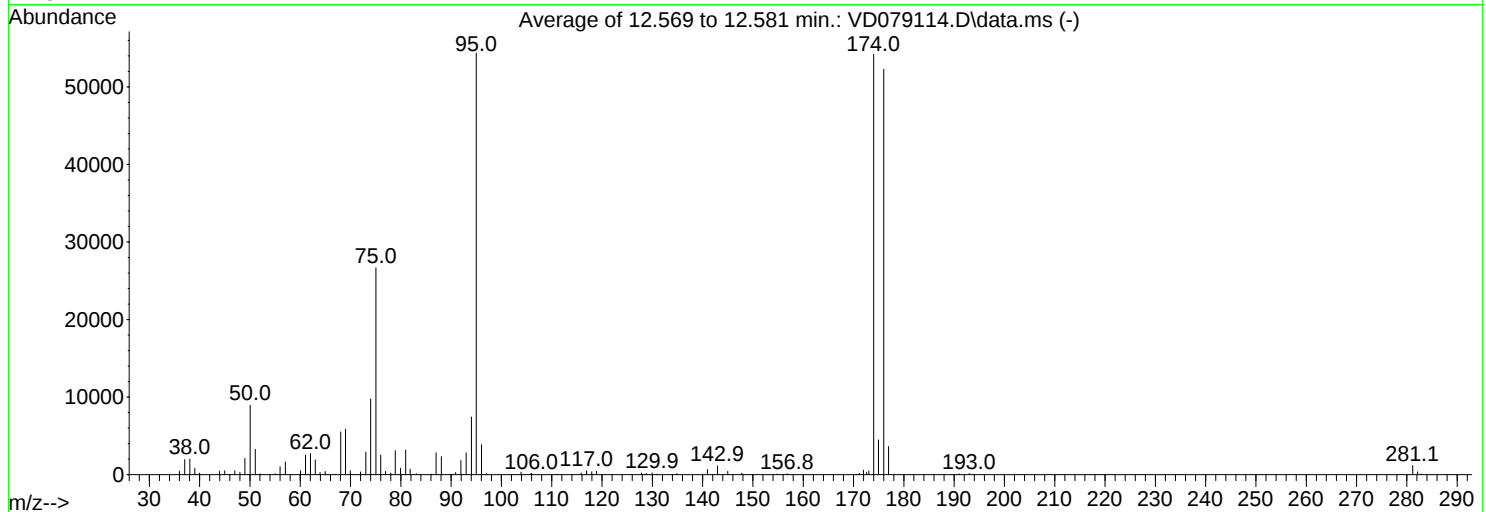


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD060324\
Data File : VD079114.D
Acq On : 03 Jun 2024 08:34
Operator : RP/MD
Sample : BFB804
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB804

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM052924SMA.M
Title : SFAM01.0
Last Update : Sat Jun 01 00:34:30 2024

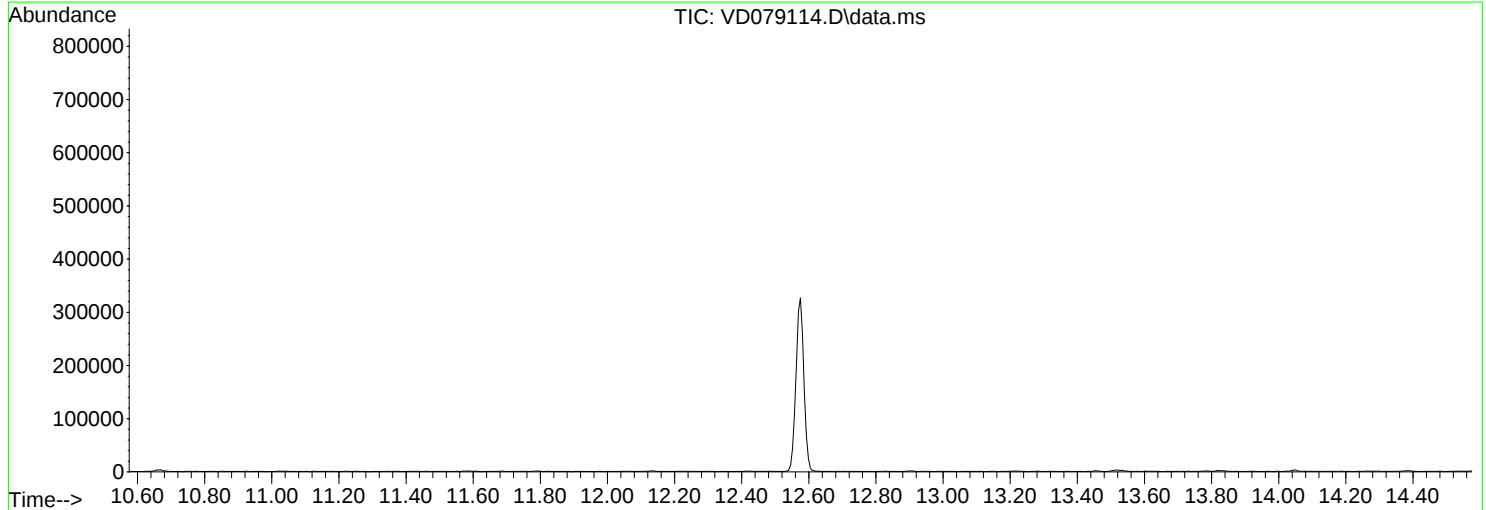

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	16.5	8948	PASS
75	95	30	80	49.0	26677	PASS
95	95	100	100	100.0	54392	PASS
96	95	5	9	7.1	3855	PASS
173	174	0.00	2	0.9	479	PASS
174	95	50	120	99.7	54205	PASS
175	174	5	9	8.3	4475	PASS
176	174	95	105	96.5	52291	PASS
177	176	5	10	6.9	3631	PASS

m/z	Abundance
40.00	643.0
44.10	317.0

Instrument :
MSVOA_D
ClientSampleId :
BFB804

m/z	Abundance
36.10	514.0
37.10	1835.0
38.10	2060.0
39.00	759.0
40.00	721.0
43.90	774.0
45.00	426.0
45.90	157.0
47.00	448.0
48.00	453.0
49.00	1850.0
50.10	10176.0
51.00	3202.0
52.00	151.0
56.00	1467.0
57.00	1712.0
60.00	639.0
61.10	2590.0
62.00	3015.0
63.00	2136.0
64.00	290.0
65.00	419.0
67.10	207.0
68.10	5575.0
69.00	5919.0
69.90	516.0
72.00	332.0
73.00	3704.0
74.00	9978.0
75.00	28632.0
76.00	2540.0
77.00	379.0
78.90	3188.0
80.00	740.0
81.00	3527.0
81.80	638.0
86.10	190.0
87.00	3001.0
88.10	2319.0
90.80	411.0
91.90	2099.0
93.00	2915.0
94.10	7707.0
95.00	54400.0
96.10	3902.0
97.00	189.0
104.00	346.0
105.80	285.0
115.90	209.0
116.90	803.0
117.90	293.0
118.90	610.0
127.80	201.0
128.70	192.0
129.90	258.0
130.90	207.0
134.90	235.0
140.90	539.0
143.00	1242.0
145.10	513.0
147.80	280.0
154.80	229.0
170.60	172.0
172.00	466.0
173.10	875.0
174.00	53424.0
174.90	4672.0
176.00	51752.0
177.00	3964.0
193.00	194.0
281.20	1020.0
282.10	343.0

Instrument :
MSVOA_D
ClientSampleId :
BFB804

m/z	Abundance
36.00	511.0
37.00	2215.0
38.00	2284.0
39.10	847.0
40.00	916.0
44.00	904.0
45.00	740.0
47.00	653.0
48.00	248.0
49.00	2228.0
50.10	9870.0
51.10	3138.0
52.10	158.0
55.00	168.0
55.90	891.0
57.10	1976.0
60.00	516.0
61.00	2873.0
62.10	2980.0
63.00	2172.0
63.90	224.0
65.00	315.0
68.00	6372.0
69.00	5718.0
69.90	319.0
72.00	340.0
73.10	3004.0
74.00	10762.0
75.10	28768.0
76.00	2765.0
76.90	585.0
78.10	311.0
78.90	3510.0
79.90	1065.0
80.90	3587.0
81.90	860.0
83.10	166.0
87.00	2756.0
88.00	2608.0
90.90	177.0
92.00	1773.0
93.00	3282.0
94.00	8258.0
95.00	62416.0
96.10	3803.0
97.00	193.0
103.90	390.0
106.00	278.0
111.10	161.0
115.80	184.0
116.90	278.0
118.00	313.0
118.80	375.0
127.80	239.0
128.90	179.0
130.00	264.0
140.90	792.0
142.80	1246.0
144.90	449.0
147.80	277.0
156.90	204.0
171.10	323.0
171.90	671.0
172.70	539.0
174.00	60104.0
175.00	4895.0
176.00	58536.0
177.00	3716.0
191.00	178.0
193.00	217.0
281.10	1366.0
282.10	448.0
282.90	232.0

Instrument :
MSVOA_D
ClientSampleId :
BFB804

m/z	Abundance
35.90	358.0
37.00	1753.0
38.10	1658.0
39.10	867.0
40.00	932.0
44.00	664.0
45.00	341.0
47.10	365.0
48.10	224.0
49.00	2190.0
50.00	6799.0
51.10	3430.0
55.00	225.0
56.10	735.0
57.10	1185.0
60.10	388.0
61.00	2068.0
62.00	2130.0
63.10	1371.0
64.00	374.0
64.90	515.0
68.00	4587.0
69.00	5960.0
70.00	642.0
72.00	399.0
73.00	2044.0
74.00	8544.0
75.00	22632.0
76.00	2273.0
77.00	282.0
77.90	306.0
78.90	2564.0
80.00	689.0
80.90	2385.0
81.90	622.0
83.10	185.0
87.00	2728.0
88.00	2073.0
91.00	213.0
92.00	1564.0
93.00	2263.0
94.00	6330.0
95.00	46360.0
96.00	3861.0
103.80	257.0
106.00	207.0
115.80	221.0
117.00	423.0
117.90	508.0
119.00	297.0
127.90	206.0
128.80	221.0
130.00	175.0
134.90	181.0
141.00	665.0
143.00	930.0
145.00	310.0
156.70	190.0
171.20	176.0
171.90	592.0
172.50	371.0
173.00	561.0
174.00	49088.0
175.00	3857.0
176.00	46584.0
176.90	3212.0
191.00	162.0
193.20	169.0
281.20	1157.0
282.20	301.0

Instrument :
MSVOA_D
ClientSampleId :
BFB804