

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD060424\
 Data File : VD079139.D
 Acq On : 04 Jun 2024 12:14
 Operator : RP/MD
 Sample : P2642-27
 Misc : 5.37G/10ml/MSVOA_D/SOIL/B
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 A4BH1

Quant Time: Jun 05 03:21:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM052924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 05 03:20:33 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.775	114	256020	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	201764	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152	54536	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.269	65	148998	18.912	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.640%
7) Chloroethane-d5	2.799	69	154142	20.234	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	80.920%
11) 1,1-Dichloroethene-d2	3.911	65	24166	17.278	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	69.120%
21) 2-Butanone-d5	6.981	46	24357	40.420	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	80.840%
24) Chloroform-d	7.569	84	143087	19.989	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	79.960%
26) 1,2-Dichloroethane-d4	8.228	65	65542	19.848	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	79.400%
32) Benzene-d6	8.199	84	278147	24.868	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	99.480%
36) 1,2-Dichloropropane-d6	9.210	67	83454	25.902	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	103.600%
41) Toluene-d8	10.269	98	222140	21.211	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	84.840%
43) trans-1,3-Dichloroprop...	10.528	79	30850	22.780	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.120%
47) 2-Hexanone-d5	10.875	63	18878	45.323	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.640%
56) 1,1,2,2-Tetrachloroeth...	12.651	84	59958	21.010	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	84.040%
66) 1,2-Dichlorobenzene-d4	13.816	152	46665	24.794	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	99.160%
Target Compounds					Qvalue	
13) Acetone	4.022	43	10060	11.531	ug/L	77


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD060424\
Data File : VD079139.D
Acq On : 04 Jun 2024 12:14
Operator : RP/MD
Sample : P2642-27
Misc : 5.37G/10ml/MSVOA_D/SOIL/B
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
A4BH1

Quant Time: Jun 05 03:21:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM052924SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 05 03:20:33 2024
Response via : Initial Calibration

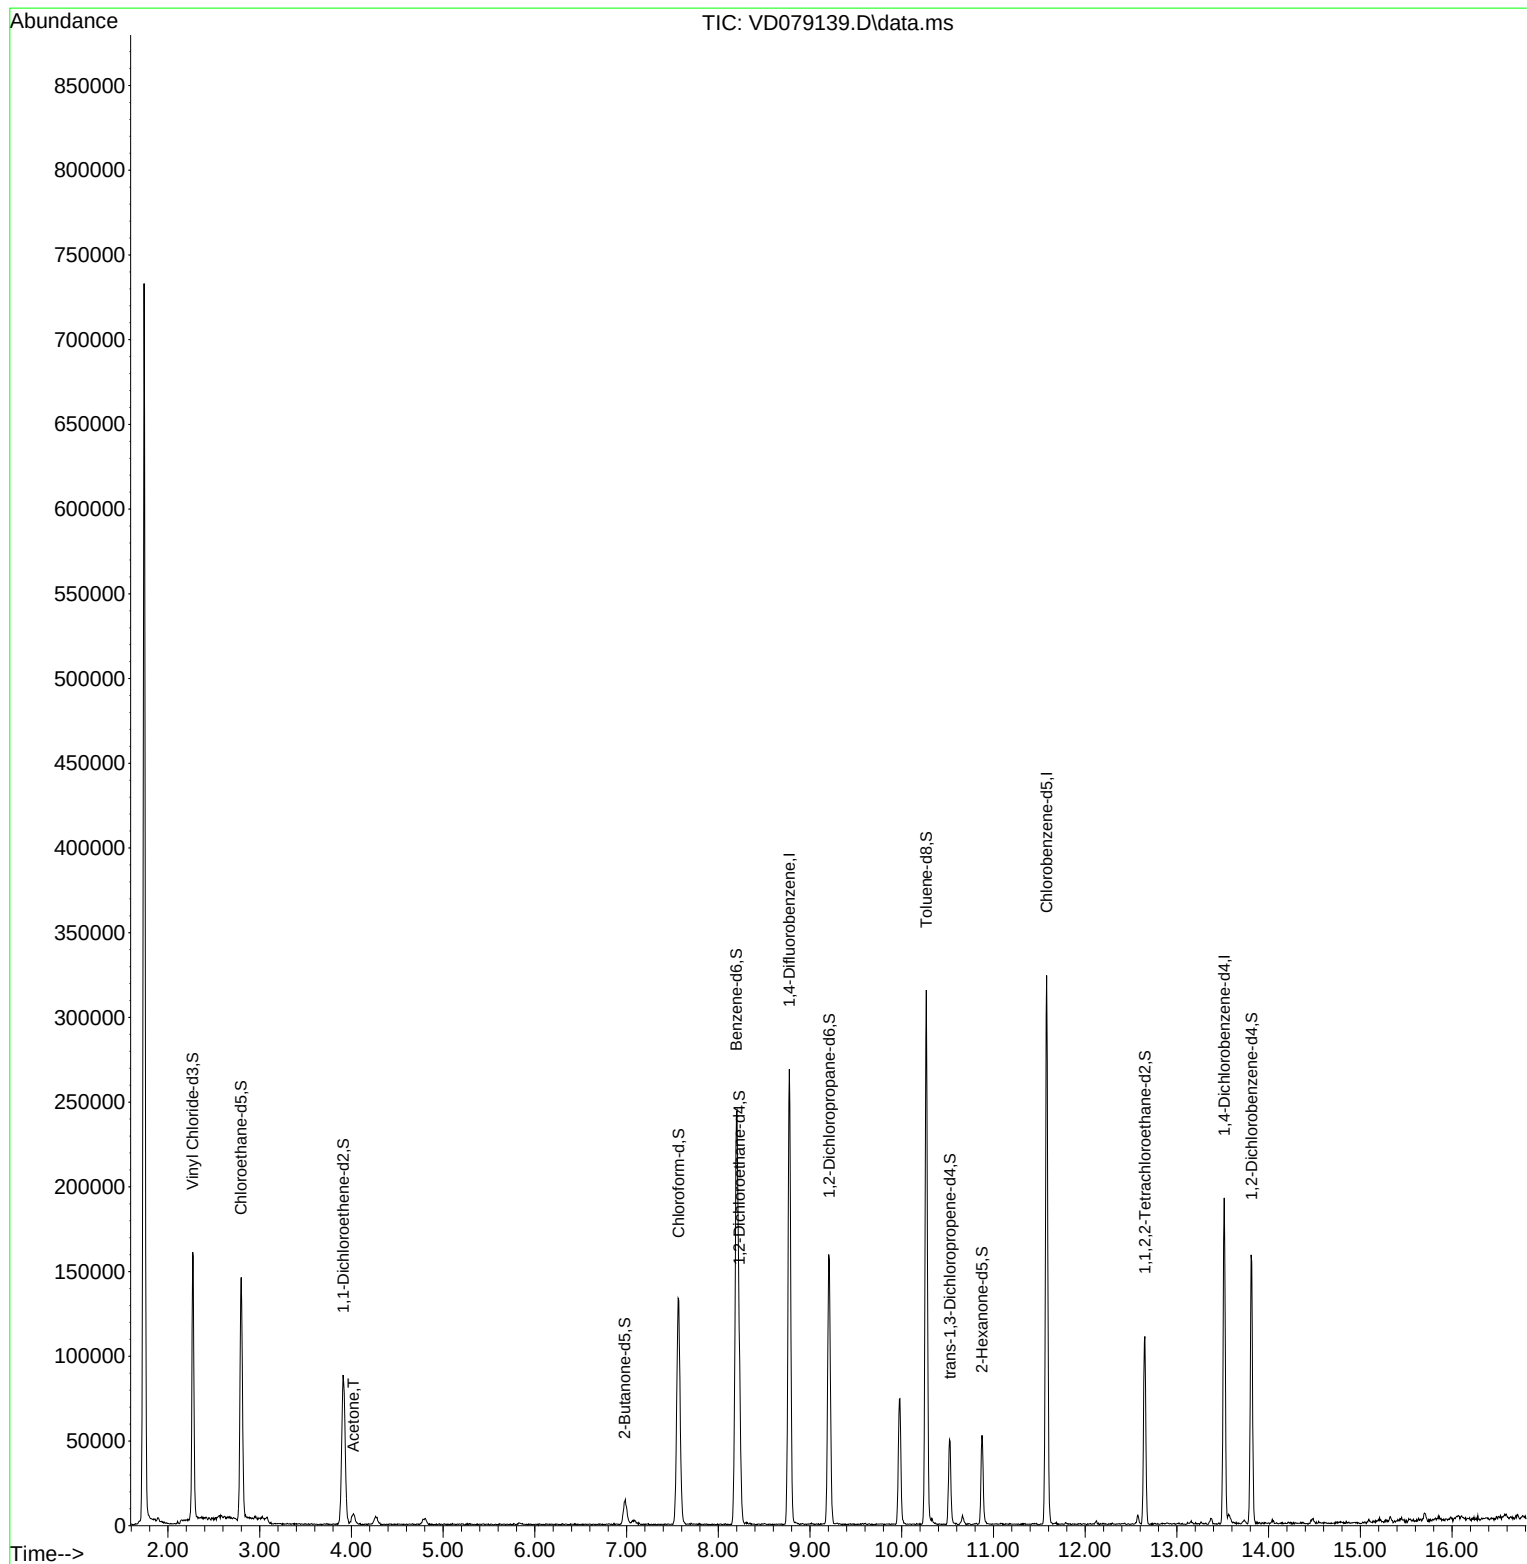

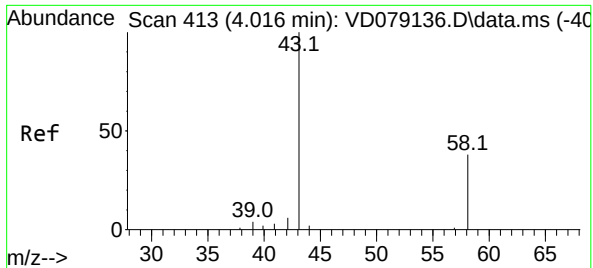

#13
 Acetone
 Concen: 11.531 ug/L
 RT: 4.022 min Scan# 41
 Delta R.T. 0.006 min
 Lab File: VD079139.D
 Acq: 04 Jun 2024 12:14

Instrument :
 MSVOA_D
 ClientSampleId :
 A4BH1

Tgt Ion: 43 Resp: 10060
 Ion Ratio Lower Upper
 43 100
 58 24.9 0.0 78.2

