
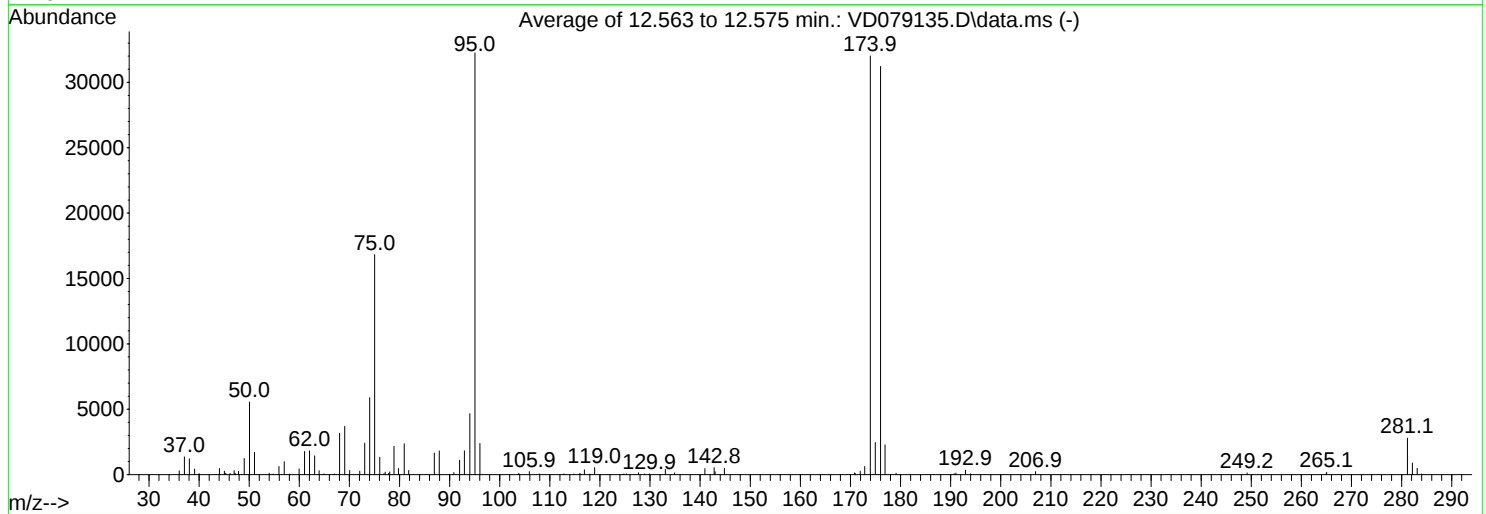


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD060424\
Data File : VD079135.D
Acq On : 04 Jun 2024 09:12
Operator : RP/MD
Sample : BFB805
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB805

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM052924SMA.M
Title : SFAM01.0
Last Update : Wed Jun 05 03:20:33 2024

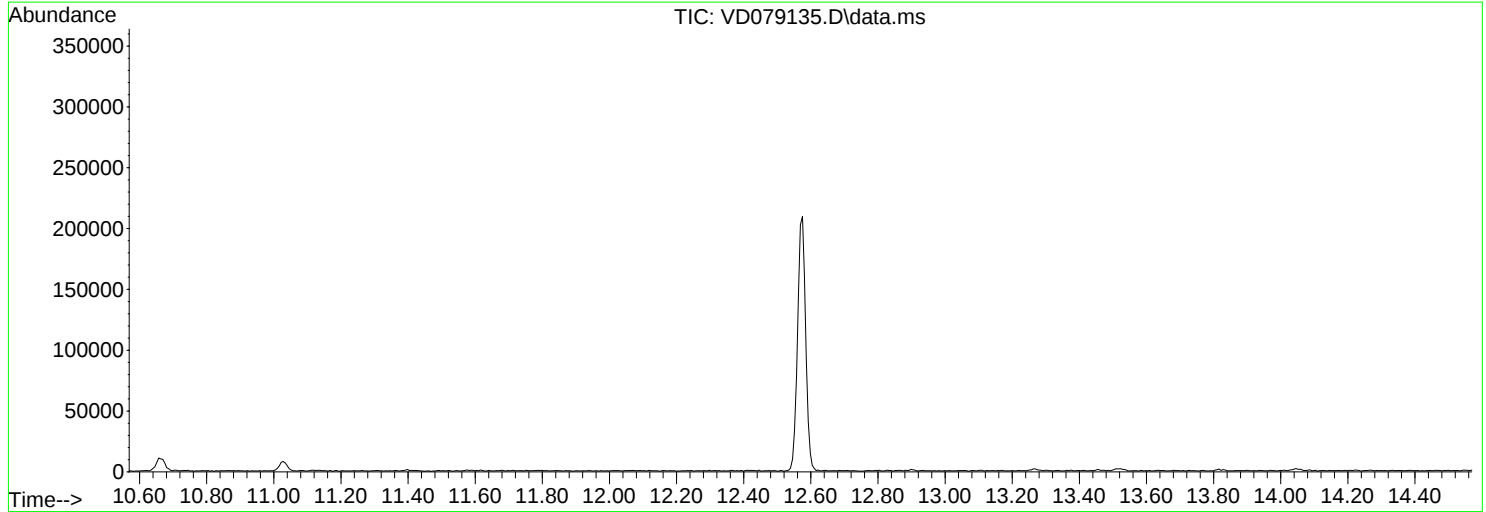

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1860

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.2	5552	PASS
75	95	30	80	52.2	16820	PASS
95	95	100	100	100.0	32251	PASS
96	95	5	9	7.4	2384	PASS
173	174	0.00	2	1.9	622	PASS
174	95	50	120	99.3	32021	PASS
175	174	5	9	7.7	2461	PASS
176	174	95	105	97.5	31205	PASS
177	176	5	10	7.3	2274	PASS

Scan 1860 (12.528 min): VD079135.D\data.ms
BFB805

m/z	Abundance
40.00	644.0
43.90	365.0

Instrument :
MSVOA_D
ClientSampleId :
BFB805

m/z	Abundance
36.00	213.0
37.00	1222.0
38.00	1047.0
39.10	327.0
40.00	855.0
43.90	501.0
45.30	345.0
47.00	643.0
47.90	171.0
49.00	902.0
50.00	4887.0
51.10	1336.0
54.00	165.0
56.00	526.0
57.10	569.0
59.90	300.0
61.10	1415.0
62.10	1391.0
63.10	1338.0
64.00	212.0
67.00	166.0
68.10	2572.0
69.00	3034.0
70.00	159.0
72.10	229.0
73.10	1863.0
74.00	5129.0
75.10	13947.0
76.10	956.0
76.90	185.0
77.80	273.0
78.80	1843.0
79.80	345.0
80.90	2313.0
81.80	200.0
86.90	1381.0
87.90	1243.0
90.80	186.0
92.00	891.0
92.90	1407.0
94.10	4062.0
95.10	24888.0
96.00	1858.0
105.80	211.0
115.90	205.0
117.00	308.0
119.00	295.0
133.00	304.0
140.90	379.0
142.80	631.0
144.90	446.0
170.80	222.0
171.90	292.0
172.80	542.0
173.90	24912.0
174.90	2130.0
176.00	23168.0
176.90	1465.0
191.00	157.0
192.90	177.0
207.00	238.0
249.20	253.0
264.90	165.0
281.10	1535.0
282.10	483.0
283.10	263.0

Instrument :
MSVOA_D
ClientSampleId :
BFB805

m/z	Abundance
36.00	373.0
37.10	1588.0
38.00	1296.0
39.10	416.0
40.10	553.0
44.10	653.0
45.00	315.0
47.20	324.0
47.90	202.0
49.00	1194.0
50.10	5793.0
51.00	2124.0
54.00	180.0
54.80	163.0
55.90	657.0
57.00	1181.0
59.90	401.0
61.00	2073.0
62.00	2277.0
63.00	1347.0
64.00	358.0
64.90	170.0
68.10	3605.0
69.00	3962.0
70.10	386.0
72.10	294.0
73.00	2286.0
74.10	6613.0
75.00	19144.0
76.00	1568.0
77.20	223.0
78.00	268.0
78.90	2252.0
79.70	571.0
81.00	2315.0
81.80	351.0
87.00	1512.0
88.00	2255.0
92.00	1116.0
93.00	2161.0
94.00	4734.0
95.10	36456.0
96.10	2811.0
105.90	221.0
107.90	169.0
114.80	165.0
116.80	447.0
118.90	796.0
127.70	253.0
128.90	165.0
133.00	372.0
135.00	189.0
141.00	636.0
143.00	668.0
144.90	295.0
171.00	226.0
171.90	223.0
172.90	659.0
174.00	34352.0
175.00	2698.0
176.00	33872.0
176.90	2589.0
179.10	158.0
190.70	203.0
193.00	439.0
265.10	274.0
281.20	2782.0
282.20	1090.0
283.20	558.0

Instrument :
MSVOA_D
ClientSampleId :
BFB805

m/z	Abundance
36.10	308.0
37.00	1257.0
38.10	1292.0
39.10	530.0
40.00	792.0
44.00	726.0
45.10	486.0
46.20	289.0
47.00	265.0
47.80	354.0
49.00	1603.0
50.00	5977.0
51.00	1642.0
55.90	695.0
56.90	1227.0
58.10	157.0
60.00	618.0
61.10	1851.0
62.00	1820.0
63.00	1613.0
63.90	353.0
68.00	3321.0
69.10	4083.0
70.00	417.0
72.00	303.0
73.00	3092.0
74.00	5918.0
75.10	17368.0
76.00	1494.0
77.10	369.0
78.10	354.0
79.00	2387.0
79.90	481.0
81.00	2458.0
81.90	398.0
87.00	2074.0
88.00	1932.0
90.90	306.0
92.00	1342.0
92.90	1896.0
94.10	5172.0
95.00	35408.0
96.00	2482.0
103.80	309.0
106.00	286.0
112.80	185.0
116.10	177.0
116.90	362.0
118.00	155.0
119.00	528.0
124.80	171.0
125.30	186.0
127.70	184.0
129.90	180.0
133.10	546.0
134.80	201.0
140.90	390.0
142.80	986.0
144.80	682.0
170.80	198.0
172.00	289.0
172.90	664.0
174.00	36800.0
175.00	2555.0
176.00	36576.0
176.90	2768.0
179.10	161.0
191.10	197.0
192.90	397.0
194.00	174.0
206.90	458.0
249.10	154.0
265.00	284.0
281.10	4037.0
282.10	1092.0
283.00	640.0
284.00	161.0

Instrument :
MSVOA_D
ClientSampleId :
BFB805