
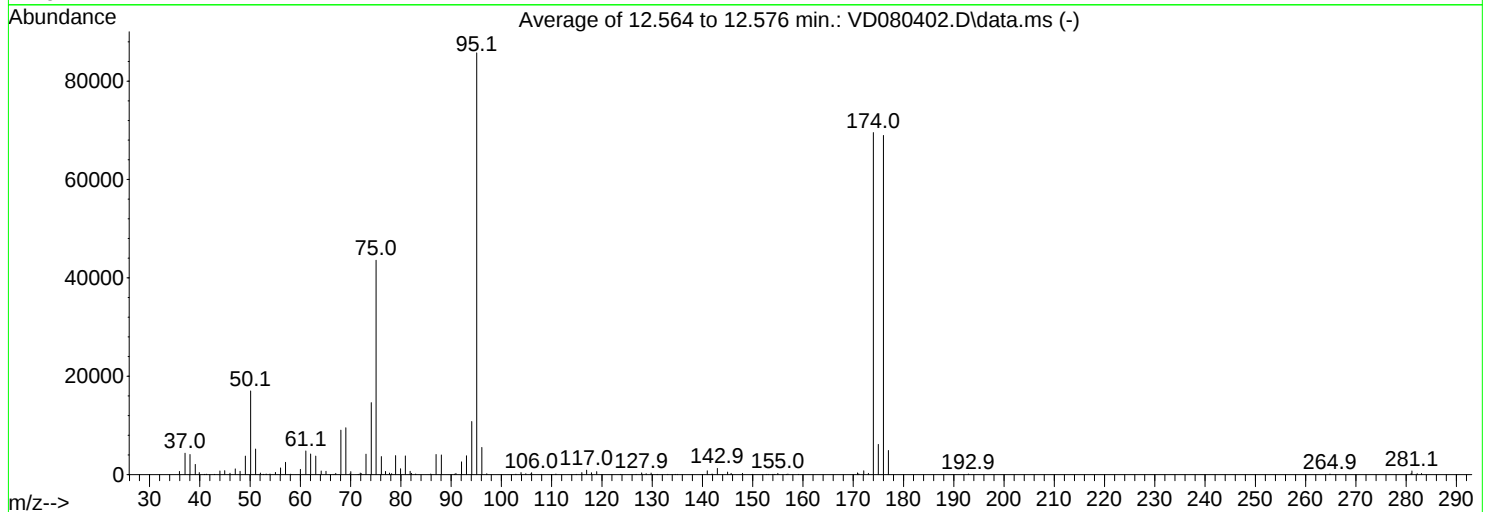


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD060425\
Data File : VD080402.D
Acq On : 04 Jun 2025 08:06
Operator : RP/MD
Sample : BFB
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D060425S.M
Title : SW846 8260
Last Update : Thu Jun 05 02:27:23 2025

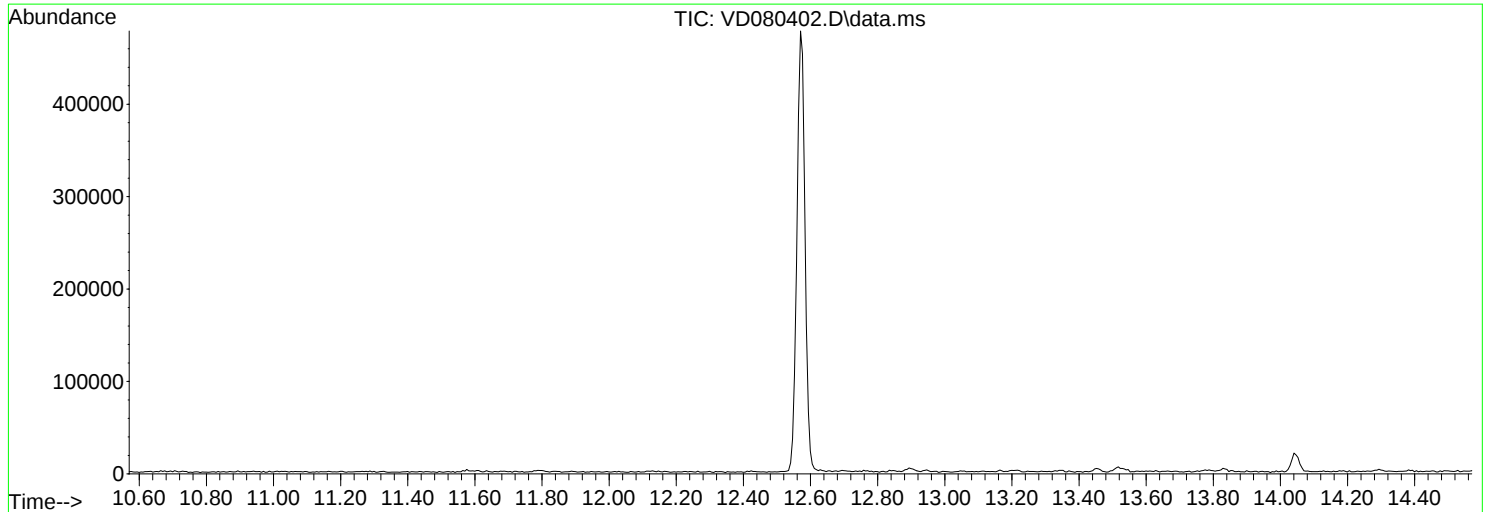

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.8	17016	PASS
75	95	30	60	50.8	43600	PASS
95	95	100	100	100.0	85749	PASS
96	95	5	9	6.4	5522	PASS
173	174	0.00	2	0.4	278	PASS
174	95	50	100	81.1	69552	PASS
175	174	5	9	8.8	6140	PASS
176	174	95	101	99.2	68973	PASS
177	176	5	9	7.1	4918	PASS