


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061022\
Data File : VD073520.D
Acq On : 10 Jun 2022 09:12
Operator : VA/SY
Sample : BFB
Misc : 5.00G/5.00ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D060922S.M
Title : SW846 8260
Last Update : Thu Jun 09 12:33:32 2022

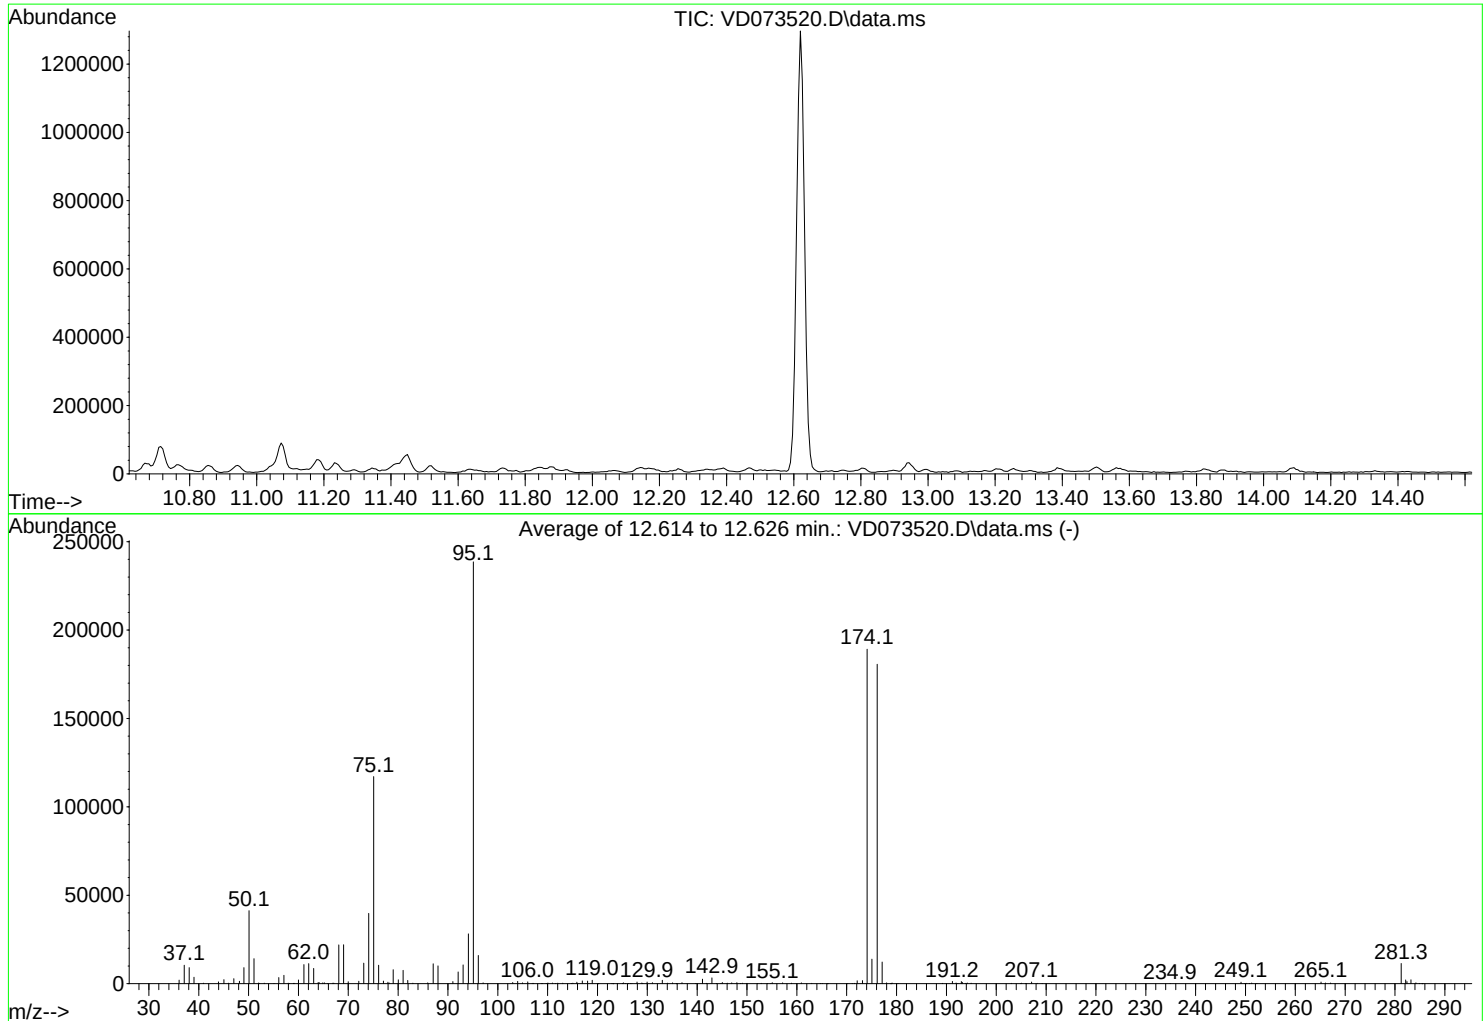

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1806

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.3	41301	PASS
75	95	30	60	49.1	117080	PASS
95	95	100	100	100.0	238568	PASS
96	95	5	9	6.7	15924	PASS
173	174	0.00	2	0.9	1739	PASS
174	95	50	100	79.3	189163	PASS
175	174	5	9	7.3	13820	PASS
176	174	95	101	95.5	180629	PASS
177	176	5	9	6.8	12237	PASS