
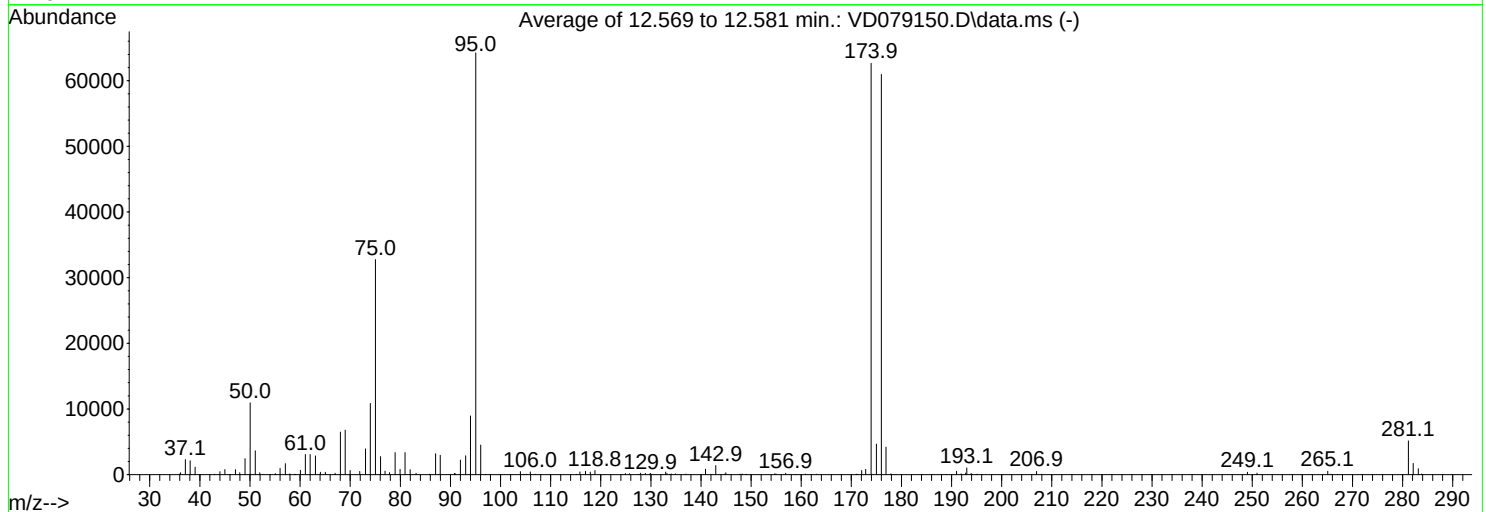


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061024\
Data File : VD079150.D
Acq On : 10 Jun 2024 09:24
Operator : RP/MD
Sample : BFB806
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB806

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM052924SMA.M
Title : SFAM01.0
Last Update : Wed Jun 12 01:05:41 2024

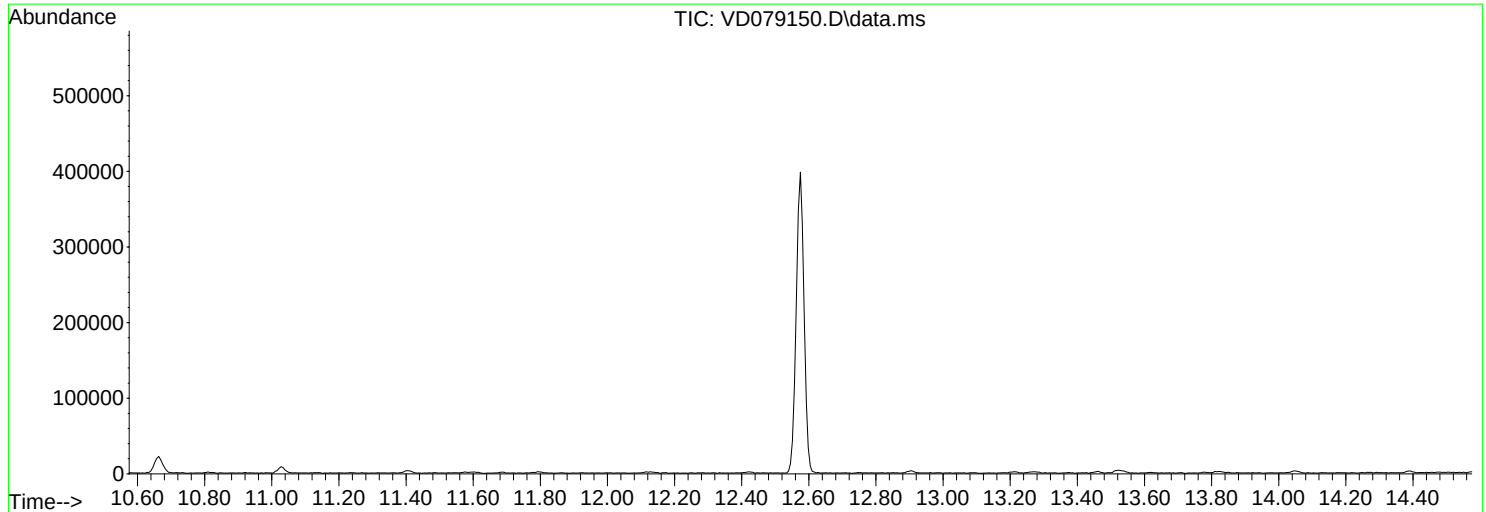

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.0	10934	PASS
75	95	30	80	51.0	32760	PASS
95	95	100	100	100.0	64237	PASS
96	95	5	9	7.0	4501	PASS
173	174	0.00	2	1.3	817	PASS
174	95	50	120	97.5	62653	PASS
175	174	5	9	7.4	4652	PASS
176	174	95	105	97.3	60939	PASS
177	176	5	10	6.9	4190	PASS

m/z	Abundance
39.90	902.0
44.00	279.0

Instrument :
MSVOA_D
ClientSampleId :
BFB806

m/z	Abundance
36.10	408.0
37.10	2564.0
38.00	2345.0
39.00	967.0
40.00	931.0
44.00	993.0
45.00	923.0
47.10	510.0
48.00	374.0
49.00	2597.0
50.00	11083.0
51.00	3154.0
52.00	398.0
56.00	834.0
57.00	1722.0
57.90	164.0
60.00	719.0
61.00	3193.0
62.00	2982.0
63.10	3042.0
64.00	566.0
65.10	326.0
67.00	207.0
68.00	6546.0
69.00	6663.0
70.00	707.0
71.90	663.0
73.00	4238.0
74.00	10327.0
75.00	32176.0
76.00	2841.0
76.90	503.0
77.90	285.0
78.90	3618.0
80.00	844.0
80.90	2938.0
81.90	894.0
83.10	187.0
87.00	3275.0
87.90	3583.0
90.80	228.0
92.00	2499.0
93.00	2856.0
94.00	8705.0
95.10	64096.0
96.10	4251.0
104.00	516.0
105.10	197.0
105.90	482.0
115.90	284.0
116.90	437.0
118.10	320.0
118.90	574.0
127.90	249.0
128.90	317.0
129.80	265.0
133.00	725.0
134.10	312.0
134.90	168.0
140.90	719.0
142.90	1586.0
144.80	307.0
148.20	275.0
155.00	162.0
156.90	216.0
158.90	182.0
171.00	200.0
172.00	731.0
172.90	905.0
173.90	59384.0
175.00	4750.0
176.00	56192.0
176.90	3756.0
178.90	162.0
188.90	164.0
191.10	381.0
192.80	770.0
193.20	557.0
193.90	219.0
207.00	307.0
249.10	329.0
250.90	160.0
265.00	422.0
281.10	3727.0
282.10	1510.0
283.20	801.0

Instrument :
MSVOA_D
ClientSampleId :
BFB806

m/z	Abundance
36.20	497.0
37.10	2125.0
38.10	2266.0
39.00	1362.0
40.00	865.0
42.90	191.0
44.10	612.0
45.00	957.0
47.10	1056.0
47.90	513.0
49.00	2825.0
50.10	11542.0
51.10	4566.0
51.90	182.0
54.10	171.0
55.10	304.0
55.90	1035.0
57.00	1944.0
58.00	195.0
58.90	157.0
60.00	725.0
61.10	3211.0
62.00	3446.0
63.00	2961.0
64.10	516.0
65.00	468.0
67.00	298.0
68.10	7083.0
69.00	7740.0
70.00	674.0
71.90	555.0
73.10	3849.0
74.00	12101.0
75.00	37576.0
76.10	3139.0
77.00	484.0
77.80	256.0
79.00	3258.0
79.90	712.0
80.90	3709.0
81.90	703.0
83.20	281.0
87.00	3687.0
88.00	2917.0
91.00	375.0
92.00	1988.0
93.10	3091.0
94.00	10183.0
95.00	71376.0
96.00	5040.0
103.90	527.0
106.00	329.0
111.90	155.0
115.80	459.0
116.90	570.0
117.90	557.0
118.90	650.0
125.00	215.0
125.80	247.0
127.90	454.0
128.90	294.0
130.00	379.0
132.80	431.0
133.80	247.0
134.90	203.0
137.00	160.0
140.90	1089.0
143.00	1692.0
145.00	499.0
146.00	174.0
147.80	258.0
149.00	194.0
154.70	343.0
157.00	278.0
160.90	312.0
172.10	529.0
172.80	904.0
174.00	68584.0
175.00	5162.0
176.00	69424.0
176.90	4998.0
177.90	179.0
191.00	487.0
191.90	169.0
193.00	1278.0
193.90	305.0
194.90	172.0
206.90	560.0
249.10	379.0
251.00	424.0
265.00	538.0
265.70	219.0

Instrument :
MSVOA_D
ClientSampleId :
BFB806

281.10

282.10

283.20

5699.0

1801.0

691.0

Instrument :

MSVOA_D

ClientSampleId :

BFB806

m/z	Abundance
35.90	327.0
37.10	2170.0
38.00	1763.0
39.10	1105.0
40.00	933.0
44.00	596.0
45.10	456.0
46.00	170.0
47.10	696.0
49.00	1931.0
50.10	10177.0
51.00	3178.0
52.00	282.0
55.00	181.0
56.10	992.0
57.10	1412.0
59.10	150.0
60.10	513.0
61.00	2824.0
62.00	2769.0
63.00	2543.0
65.00	333.0
67.10	156.0
68.00	5828.0
69.00	5909.0
70.00	506.0
71.90	259.0
73.00	3717.0
74.00	10112.0
75.10	28528.0
76.00	2304.0
77.00	616.0
77.80	392.0
78.90	3193.0
79.90	866.0
81.00	3459.0
82.00	667.0
83.10	162.0
85.80	192.0
87.10	2658.0
88.00	2376.0
90.80	358.0
92.00	2158.0
93.00	2678.0
94.00	7949.0
95.10	57240.0
96.00	4212.0
97.00	188.0
104.00	362.0
104.70	160.0
105.90	410.0
106.90	195.0
115.10	156.0
115.80	468.0
117.00	555.0
117.80	318.0
118.80	654.0
124.80	286.0
125.70	200.0
127.50	153.0
129.90	198.0
133.20	546.0
137.00	155.0
140.90	709.0
142.90	862.0
144.90	355.0
154.90	180.0
156.80	212.0
163.10	212.0
171.20	161.0
172.00	644.0
172.80	642.0
174.00	59992.0
175.00	4045.0
176.00	57200.0
176.90	3815.0
177.90	204.0
190.90	680.0
191.90	187.0
193.00	1248.0
194.10	197.0
195.10	233.0
207.00	609.0
208.00	237.0
249.00	411.0
251.00	155.0
265.10	589.0
267.00	168.0
281.20	5993.0
282.10	1828.0
283.10	1195.0
283.80	301.0

Instrument :
MSVOA_D
ClientSampleId :
BFB806