

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061124\
 Data File : VD079173.D
 Acq On : 11 Jun 2024 20:12
 Operator : RP/MD
 Sample : P2775-16
 Misc : 4.41G/10ml/MSVOA_D/SOIL/A
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 A4CA1

Quant Time: Jun 12 01:08:42 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM052924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Jun 12 01:05:41 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.775	114	142470	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117	110599	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152	26610	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.275	65	82679	18.858	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.440%
7) Chloroethane-d5	2.805	69	81960	19.334	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	77.320%
11) 1,1-Dichloroethene-d2	3.916	65	14554	18.700	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	74.800%
21) 2-Butanone-d5	6.987	46	9453	28.190	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	56.380%
24) Chloroform-d	7.569	84	87805	22.042	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.160%
26) 1,2-Dichloroethane-d4	8.234	65	38363	20.876	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	83.520%
32) Benzene-d6	8.198	84	154951	25.273	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	101.080%
36) 1,2-Dichloropropane-d6	9.210	67	49081	27.790	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	111.160%
41) Toluene-d8	10.269	98	116842	20.353	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	81.400%
43) trans-1,3-Dichloroprop...	10.528	79	13137	17.697	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	70.800%
47) 2-Hexanone-d5	10.881	63	5393	23.620	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	47.240%
56) 1,1,2,2-Tetrachloroeth...	12.651	84	28591	18.277	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	73.120%
66) 1,2-Dichlorobenzene-d4	13.816	152	19379	21.102	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	84.400%
Target Compounds						
16) Methylene chloride	4.816	84	17027	6.707	ug/L	Qvalue 84


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061124\
Data File : VD079173.D
Acq On : 11 Jun 2024 20:12
Operator : RP/MD
Sample : P2775-16
Misc : 4.41G/10ml/MSVOA_D/SOIL/A
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
A4CA1


Quant Time: Jun 12 01:08:42 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM052924SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Jun 12 01:05:41 2024
Response via : Initial Calibration

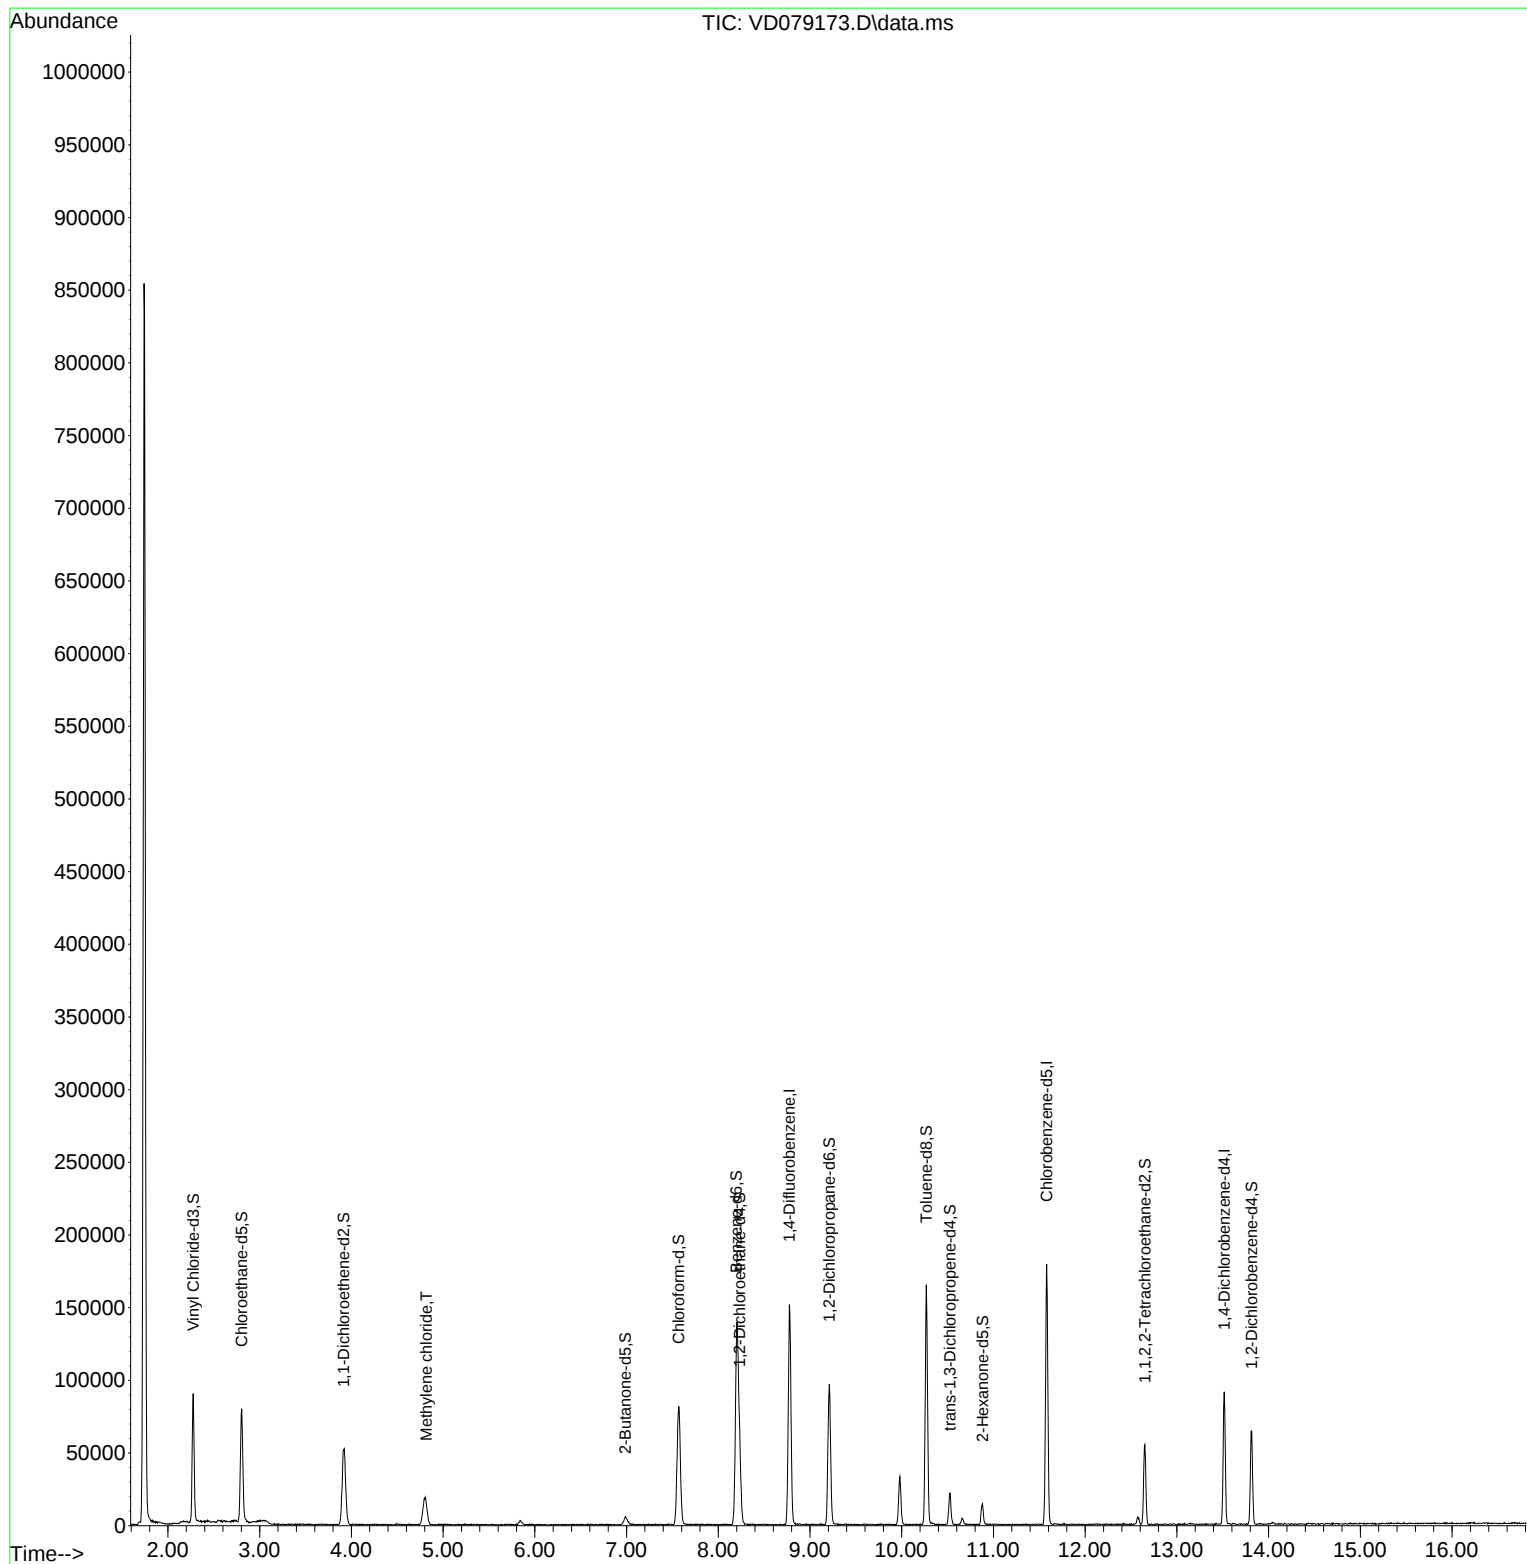

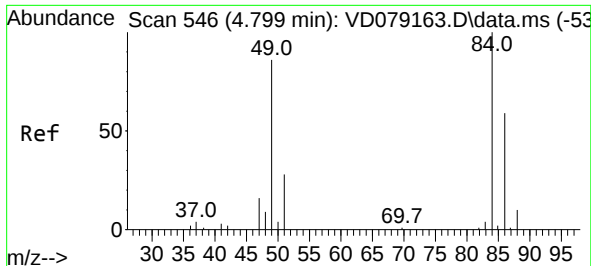

#16
Methylene chloride
Concen: 6.707 ug/L
RT: 4.816 min Scan# 54
Delta R.T. 0.017 min
Lab File: VD079173.D
Acq: 11 Jun 2024 20:12

Instrument :
MSVOA_D
ClientSampleId :
A4CA1

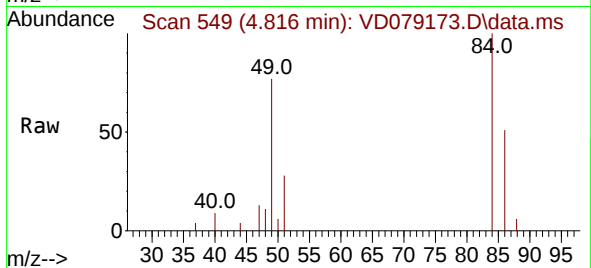

Tgt Ion: 84	Resp: 17027
Ion Ratio	Lower Upper
84 100	
86 51.3	40.9 76.0
49 76.7	67.5 125.3

