
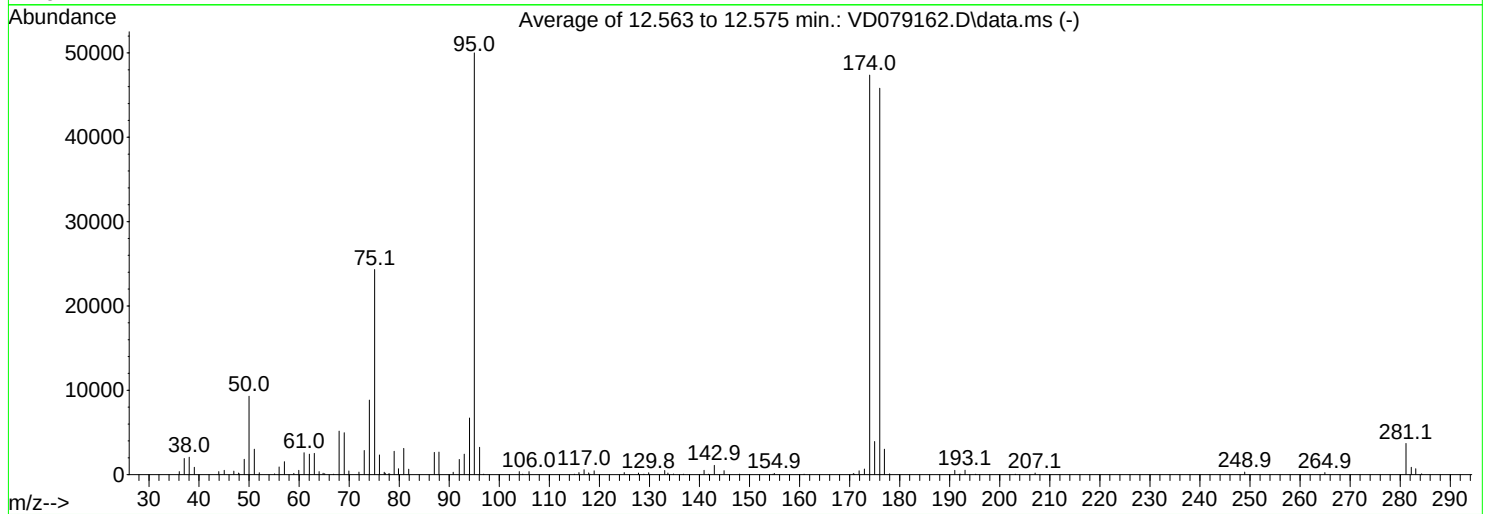


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061124\
Data File : VD079162.D
Acq On : 11 Jun 2024 14:39
Operator : RP/MD
Sample : BFB807
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB807

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM052924SMA.M
Title : SFAM01.0
Last Update : Wed Jun 12 01:05:41 2024

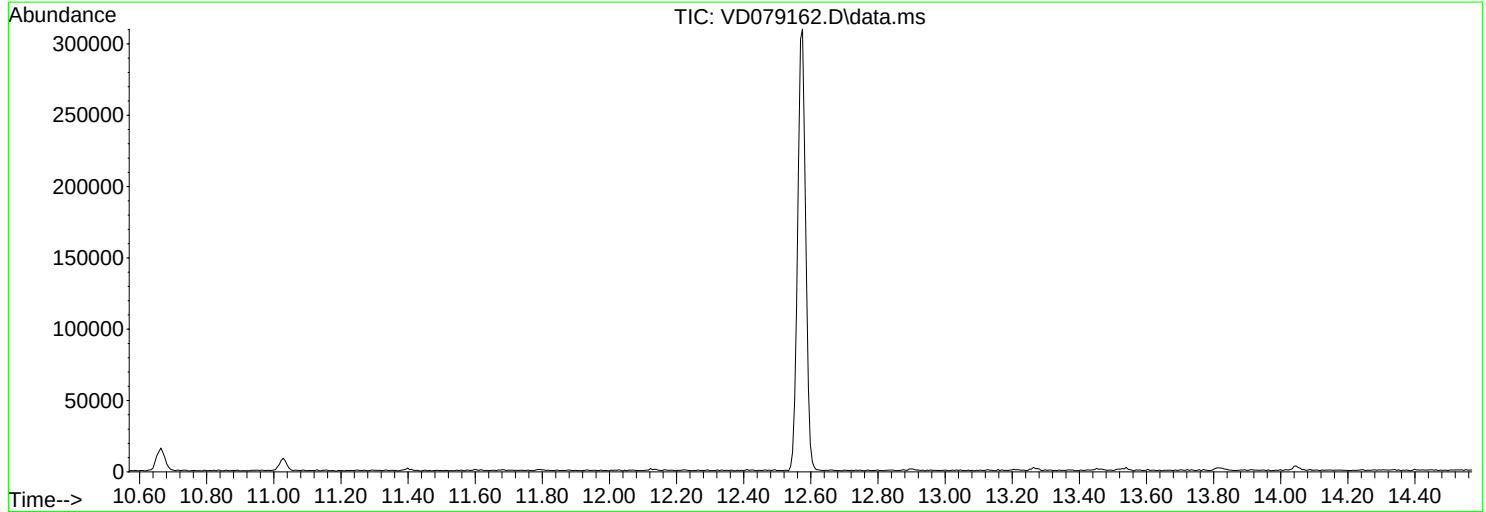

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1860

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.6	9288	PASS
75	95	30	80	48.6	24315	PASS
95	95	100	100	100.0	50008	PASS
96	95	5	9	6.5	3244	PASS
173	174	0.00	2	1.4	665	PASS
174	95	50	120	94.7	47376	PASS
175	174	5	9	8.3	3936	PASS
176	174	95	105	96.7	45811	PASS
177	176	5	10	6.6	3012	PASS

m/z	Abundance
40.00	676.0
43.90	416.0

Instrument :
MSVOA_D
ClientSampleId :
BFB807

m/z	Abundance
36.20	388.0
37.00	1677.0
38.00	1882.0
39.10	789.0
40.00	579.0
44.10	914.0
45.10	465.0
47.00	395.0
48.00	259.0
49.00	1427.0
50.00	7753.0
51.00	2041.0
52.00	237.0
56.00	650.0
57.10	1196.0
60.00	433.0
61.00	2258.0
62.10	1899.0
63.00	1688.0
64.00	265.0
64.80	354.0
68.00	3766.0
69.00	4028.0
70.00	470.0
71.90	240.0
73.00	1953.0
74.10	7089.0
75.10	18656.0
76.10	1943.0
77.00	311.0
79.00	2593.0
79.90	813.0
80.90	2121.0
81.90	288.0
87.00	2231.0
88.00	2238.0
90.90	172.0
92.00	1337.0
93.00	2140.0
94.00	4695.0
95.00	40032.0
96.00	2824.0
104.10	329.0
106.00	309.0
115.90	239.0
117.00	444.0
119.00	358.0
125.00	212.0
127.90	278.0
129.80	195.0
133.10	448.0
141.00	451.0
141.80	168.0
142.90	1058.0
144.90	314.0
154.70	194.0
170.70	194.0
172.00	350.0
173.00	591.0
174.00	36952.0
175.00	3359.0
176.00	33360.0
177.00	2441.0
191.00	284.0
193.00	366.0
249.00	263.0
264.90	217.0
281.20	1948.0
282.20	508.0
283.20	242.0

Instrument :
MSVOA_D
ClientSampleId :
BFB807

m/z	Abundance
36.00	357.0
37.10	1946.0
38.00	2178.0
39.00	953.0
39.90	446.0
44.00	720.0
45.00	372.0
47.00	505.0
47.80	322.0
49.00	1822.0
50.00	9413.0
51.10	3320.0
52.00	253.0
56.00	1127.0
57.10	1878.0
58.90	201.0
59.90	567.0
61.00	2599.0
62.10	2629.0
63.10	3232.0
64.10	445.0
65.10	348.0
66.90	153.0
68.00	5617.0
69.00	5249.0
69.90	330.0
72.00	318.0
73.00	3727.0
74.00	9214.0
75.10	27368.0
76.10	2508.0
77.20	500.0
77.90	270.0
79.00	2970.0
79.80	515.0
80.90	3387.0
81.90	786.0
87.00	2872.0
87.90	2958.0
90.70	234.0
92.00	2323.0
93.00	2773.0
94.10	8191.0
95.00	55680.0
96.00	3506.0
103.90	471.0
106.00	270.0
115.90	200.0
116.90	493.0
117.80	166.0
118.10	181.0
119.00	574.0
124.90	281.0
128.90	180.0
129.90	204.0
133.00	365.0
140.90	576.0
143.00	1237.0
144.90	453.0
148.00	176.0
155.00	230.0
160.90	163.0
170.80	188.0
171.80	374.0
172.90	545.0
174.00	52248.0
175.00	4134.0
176.00	50856.0
176.90	3467.0
178.00	275.0
190.90	424.0
192.20	184.0
193.10	634.0
207.00	369.0
248.90	433.0
265.00	216.0
281.10	4128.0
282.20	821.0
283.10	748.0

Instrument :
MSVOA_D
ClientSampleId :
BFB807

m/z	Abundance
36.00	335.0
37.00	2103.0
38.10	2141.0
39.10	874.0
40.00	504.0
44.00	699.0
45.10	685.0
46.90	368.0
48.10	218.0
49.10	2233.0
50.00	10697.0
51.00	3688.0
52.10	204.0
55.10	279.0
56.00	937.0
57.00	1553.0
59.00	248.0
59.90	546.0
61.00	2929.0
62.00	2750.0
63.00	2640.0
63.90	392.0
64.80	177.0
68.00	6083.0
69.00	5632.0
70.00	531.0
72.00	341.0
73.00	2894.0
74.00	10231.0
75.10	26920.0
76.00	2562.0
77.00	554.0
78.10	259.0
79.00	2756.0
79.90	776.0
80.90	3817.0
81.90	848.0
87.00	2809.0
88.00	2853.0
90.80	458.0
92.00	1725.0
93.00	2359.0
94.10	7277.0
95.00	54312.0
96.10	3403.0
96.90	161.0
104.00	302.0
104.70	160.0
105.90	489.0
115.00	165.0
115.90	285.0
116.90	819.0
117.90	444.0
118.80	445.0
125.00	226.0
127.70	312.0
129.90	266.0
133.10	653.0
133.70	584.0
134.80	203.0
136.80	201.0
140.80	521.0
142.90	1038.0
144.90	648.0
154.90	237.0
171.00	172.0
171.90	648.0
172.90	859.0
174.00	52928.0
175.00	4314.0
176.00	53216.0
177.00	3127.0
190.90	432.0
191.10	426.0
191.90	161.0
193.10	621.0
195.20	153.0
203.10	168.0
207.10	211.0
248.90	239.0
265.00	292.0
281.20	5021.0
282.20	1319.0
283.10	1110.0
284.30	270.0

Instrument :
MSVOA_D
ClientSampleId :
BFB807