
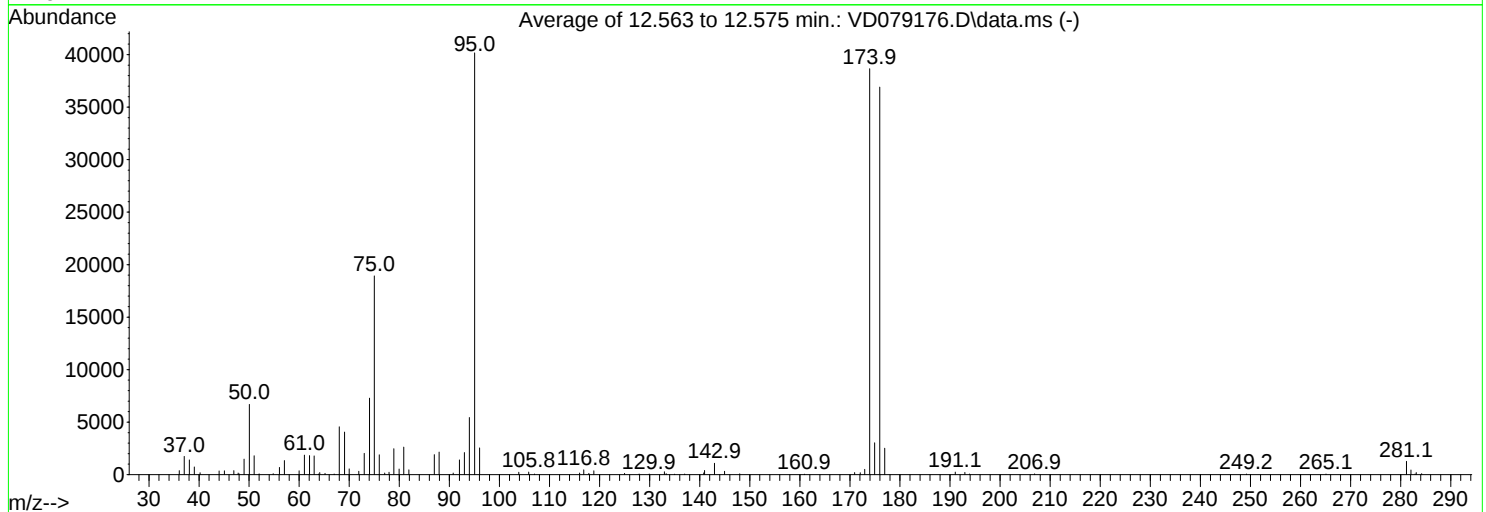


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061324\
Data File : VD079176.D
Acq On : 13 Jun 2024 08:31
Operator : RP/MD
Sample : BFB808
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB808

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM052924SMA.M
Title : SFAM01.0
Last Update : Fri Jun 14 04:47:47 2024

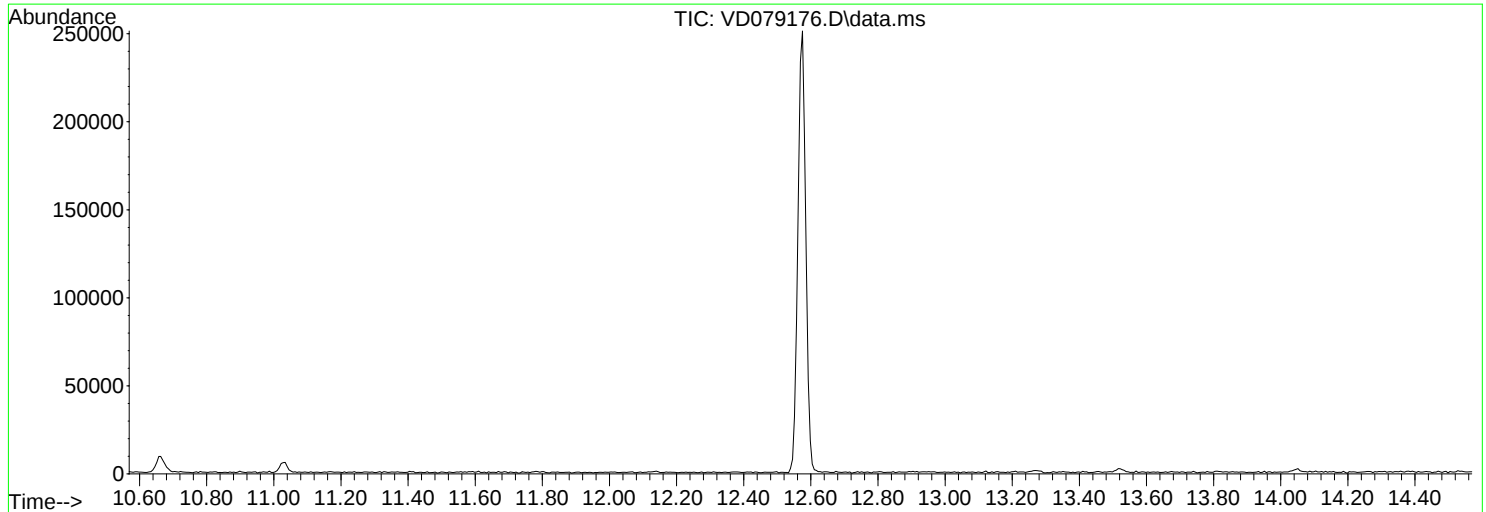

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	6694	PASS
75	95	30	80	47.1	18930	PASS
95	95	100	100	100.0	40171	PASS
96	95	5	9	6.4	2552	PASS
173	174	0.00	2	1.3	507	PASS
174	95	50	120	96.2	38661	PASS
175	174	5	9	7.8	3033	PASS
176	174	95	105	95.5	36912	PASS
177	176	5	10	6.8	2521	PASS

Scan 1860 (12.528 min): VD079176.D\data.ms
BFB808

m/z	Abundance
39.90	609.0
44.00	190.0

Instrument :
MSVOA_D
ClientSampleId :
BFB808

m/z	Abundance
36.10	472.0
37.10	1274.0
38.00	1240.0
39.20	483.0
40.20	532.0
44.00	596.0
45.10	173.0
47.00	269.0
49.00	1326.0
50.00	4992.0
51.00	1207.0
54.80	270.0
56.00	560.0
57.10	1157.0
60.00	364.0
61.00	1317.0
62.00	1290.0
63.00	1262.0
63.90	169.0
65.20	189.0
68.00	3387.0
69.10	3360.0
70.20	167.0
71.90	180.0
73.10	1414.0
74.10	5405.0
75.00	14245.0
75.90	1570.0
78.90	1904.0
80.00	389.0
80.90	1683.0
81.90	301.0
87.00	1310.0
88.00	1980.0
90.80	256.0
92.00	947.0
93.10	1632.0
94.00	4130.0
95.00	30240.0
96.00	1942.0
103.90	188.0
105.80	290.0
116.90	389.0
117.80	201.0
119.00	235.0
133.00	199.0
140.80	486.0
143.00	1081.0
145.00	307.0
173.00	237.0
173.90	28736.0
174.90	2255.0
176.00	28648.0
176.90	1935.0
206.90	209.0
281.10	651.0
282.10	657.0
282.90	178.0

Instrument :
MSVOA_D
ClientSampleId :
BFB808

m/z	Abundance
36.00	296.0
37.00	2115.0
38.00	1393.0
39.00	767.0
39.90	725.0
44.00	596.0
45.00	463.0
47.00	221.0
47.80	469.0
49.00	1450.0
50.10	7051.0
51.00	1864.0
56.10	675.0
57.00	1282.0
60.00	306.0
61.00	2072.0
62.10	2018.0
63.00	1737.0
64.10	246.0
65.10	181.0
67.00	169.0
68.00	4850.0
69.00	3844.0
70.00	579.0
71.90	399.0
72.90	2302.0
74.00	7982.0
75.00	20944.0
76.00	1903.0
77.10	195.0
78.10	244.0
78.90	2953.0
80.00	464.0
80.90	2832.0
81.90	555.0
87.00	2182.0
87.90	2202.0
90.70	185.0
92.00	1546.0
93.00	2522.0
94.00	5428.0
95.10	45184.0
96.00	2598.0
103.80	159.0
105.80	237.0
107.00	172.0
116.90	571.0
118.80	368.0
125.00	189.0
129.90	189.0
132.90	261.0
133.30	293.0
141.00	634.0
143.00	966.0
144.90	244.0
148.00	222.0
170.90	281.0
172.10	225.0
172.80	469.0
174.00	42024.0
175.00	3487.0
176.00	39656.0
177.00	2476.0
191.00	317.0
192.90	263.0
193.90	206.0
281.20	1569.0
282.00	273.0
283.10	290.0

Instrument :
MSVOA_D
ClientSampleId :
BFB808

m/z	Abundance
36.00	358.0
37.00	1809.0
38.10	1583.0
39.00	949.0
40.00	590.0
44.10	452.0
45.00	446.0
46.90	638.0
48.00	252.0
49.00	1651.0
50.10	8039.0
51.00	2339.0
52.00	244.0
56.10	810.0
57.00	1563.0
60.00	424.0
61.10	2174.0
62.00	2141.0
63.00	2372.0
64.10	361.0
68.00	5430.0
69.00	4957.0
70.00	885.0
71.90	366.0
73.00	2382.0
74.00	8457.0
75.00	21600.0
76.10	2199.0
77.10	267.0
77.90	441.0
78.90	2543.0
79.90	739.0
80.90	3326.0
81.90	526.0
87.00	2201.0
88.00	2284.0
92.00	1694.0
92.90	2164.0
94.00	6772.0
95.00	45088.0
96.10	3117.0
103.90	345.0
105.90	217.0
116.00	459.0
116.80	434.0
117.90	178.0
118.80	516.0
125.00	188.0
127.90	176.0
132.90	388.0
135.00	153.0
137.00	187.0
140.90	568.0
142.90	1183.0
145.00	395.0
160.90	151.0
171.00	323.0
172.00	315.0
173.00	814.0
173.90	45224.0
175.00	3357.0
175.90	42432.0
177.00	3153.0
191.10	413.0
193.00	394.0
249.20	178.0
265.10	183.0
281.20	1572.0
282.10	417.0
283.10	330.0
284.20	277.0

Instrument :
MSVOA_D
ClientSampleId :
BFB808