
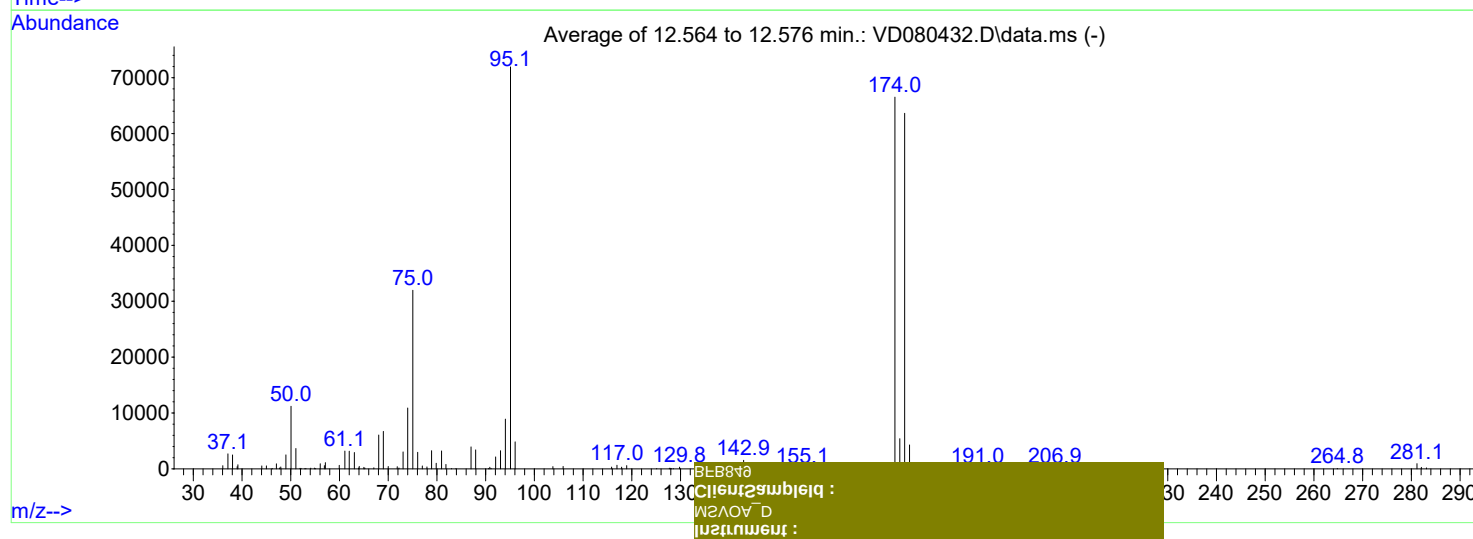


Data Path : D:\MassHunter\GCMS\1\data\VD061325\
Data File : VD080432.D
Acq On : 13 Jun 2025 08:31
Operator : RP/MD
Sample : BFB849
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM061325SMA.M
Title : SFAM01.0
Last Update : Mon Jun 16 11:17:50 2025

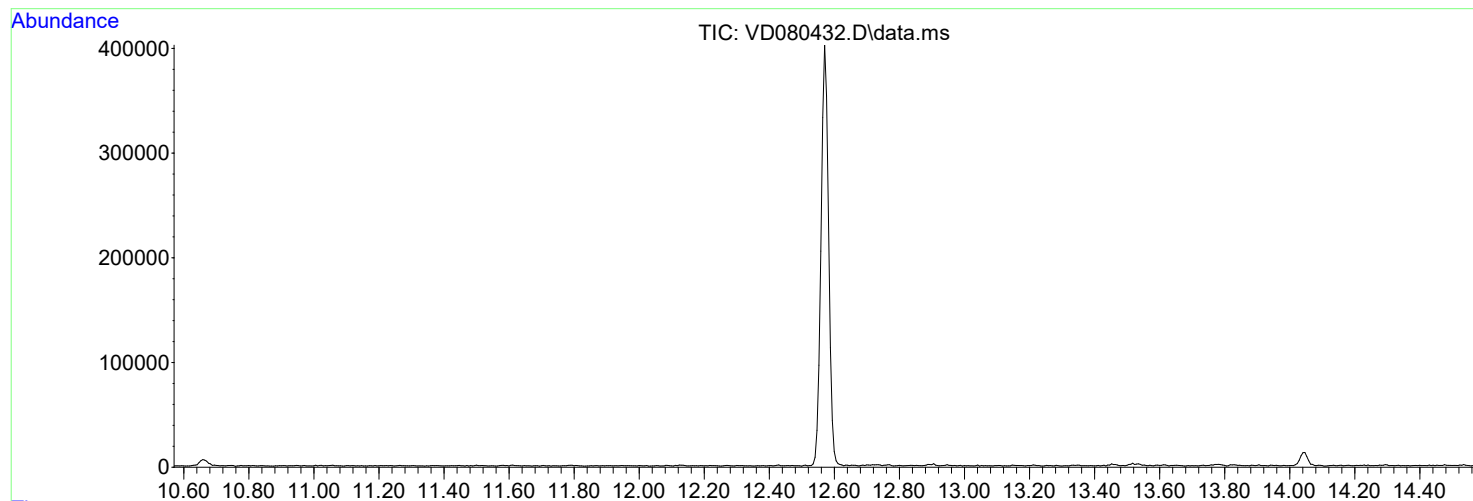

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1827

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.6	11204	PASS
75	95	30	80	44.4	31960	PASS
95	95	100	100	100.0	71936	PASS
96	95	5	9	6.7	4839	PASS
173	174	0.00	2	0.8	549	PASS
174	95	50	120	92.5	66525	PASS
175	174	5	9	8.1	5405	PASS
176	174	95	105	95.7	63635	PASS
177	176	5	10	6.7	4284	PASS

m/z	Abundance
40.00	906.0
43.80	429.0

BFB849
ClientSampleId :
MS/MS.D
Instrument :

m/z	Abundance
36.00	519.0
37.10	2658.0
38.10	1927.0
39.00	1212.0
39.90	812.0
43.90	1030.0
45.00	382.0
47.10	809.0
47.90	423.0
49.00	2334.0
50.00	9922.0
51.00	3267.0
52.90	171.0
54.80	206.0
56.00	919.0
56.90	1750.0
59.90	605.0
61.10	2868.0
62.00	3082.0
63.10	2537.0
63.90	474.0
65.00	486.0
67.10	193.0
68.10	5447.0
69.00	6857.0
70.00	453.0
72.00	296.0
73.10	2811.0
74.00	10212.0
75.10	29536.0
76.10	2709.0
77.00	488.0
77.90	410.0
78.90	3236.0
79.80	1057.0
80.90	2804.0
81.80	688.0
87.00	4055.0
88.00	3059.0
90.90	512.0
92.10	1755.0
93.00	3005.0
94.00	8513.0
95.10	66200.0
96.10	4432.0
103.80	481.0
105.90	479.0
115.90	392.0
116.90	639.0
118.00	345.0
118.90	626.0
127.70	208.0
129.80	323.0
135.00	175.0
141.00	512.0
142.90	1793.0
143.90	190.0
144.90	467.0
145.90	200.0
147.90	379.0
154.90	282.0
160.80	175.0
170.60	282.0
171.80	634.0
173.00	1647.0
174.00	59280.0
175.00	4876.0
176.00	57968.0
177.00	3550.0
178.10	335.0
281.20	570.0

БЕБ849
ClientSampleId :
MS/MS.D
Instrument :

m/z	Abundance
36.10	525.0
37.10	3145.0
38.10	3107.0
39.20	1419.0
40.00	907.0
44.10	817.0
45.10	699.0
46.20	181.0
47.00	976.0
48.00	614.0
49.00	2892.0
50.10	12770.0
51.10	4156.0
51.90	288.0
53.10	240.0
54.20	225.0
54.90	226.0
56.10	1220.0
57.10	1840.0
59.90	686.0
61.10	3456.0
62.00	3082.0
63.10	3214.0
64.10	463.0
65.00	349.0
66.90	206.0
68.10	7148.0
69.00	7134.0
70.10	530.0
71.80	511.0
72.20	486.0
73.10	3443.0
74.00	12170.0
75.00	36056.0
76.00	3194.0
76.90	797.0
78.00	375.0
78.90	3713.0
79.90	1129.0
81.00	3894.0
81.90	880.0
87.00	3981.0
88.00	3352.0
90.80	373.0
92.10	2140.0
93.00	3637.0
94.10	9696.0
95.10	79672.0
96.10	5137.0
103.80	419.0
105.90	497.0
115.90	280.0
117.00	787.0
117.80	294.0
119.00	682.0
127.90	327.0
129.90	393.0
134.80	207.0
136.90	178.0
140.90	957.0
143.00	1399.0
143.90	206.0
144.90	800.0
145.90	189.0
155.10	328.0
159.00	174.0
171.10	427.0
171.80	569.0
174.00	75232.0
175.00	6051.0
176.00	67784.0
177.00	5545.0
191.00	213.0
281.10	1273.0
282.10	428.0
283.10	300.0

БЕБ849
ClientSampleId :
MS/MS.D
Instrument :

m/z	Abundance
36.00	671.0
37.10	2280.0
38.00	2457.0
39.10	790.0
39.90	962.0
44.00	770.0
44.90	528.0
47.10	933.0
47.70	497.0
49.00	2294.0
50.10	10920.0
51.00	3531.0
52.10	295.0
54.00	174.0
55.10	187.0
56.00	614.0
57.10	1507.0
60.00	608.0
61.10	3242.0
62.00	3316.0
63.00	3039.0
64.00	872.0
65.20	477.0
67.10	204.0
68.00	5592.0
69.00	6142.0
69.90	307.0
71.80	374.0
73.00	2859.0
74.00	10313.0
75.00	30288.0
76.00	3003.0
77.10	297.0
78.00	275.0
78.90	2814.0
79.90	826.0
80.90	2941.0
81.90	822.0
83.00	171.0
83.90	154.0
87.00	3759.0
87.90	3791.0
90.60	194.0
91.10	300.0
92.00	2534.0
93.10	3118.0
94.10	8511.0
95.10	69936.0
96.00	4948.0
103.80	334.0
105.90	334.0
115.80	304.0
116.90	540.0
117.90	302.0
119.00	455.0
125.10	175.0
127.70	177.0
128.10	192.0
128.50	168.0
129.70	207.0
133.20	185.0
141.00	715.0
143.00	1417.0
145.00	472.0
155.10	152.0
157.00	173.0
171.90	795.0
174.00	65064.0
175.00	5288.0
176.00	65152.0
177.00	3756.0
178.00	189.0
191.00	291.0
192.80	254.0
206.90	182.0
264.80	223.0
281.10	970.0
282.00	401.0
283.10	250.0

БЕБ849
ClientSampleId :
MS/MS.D
Instrument :