
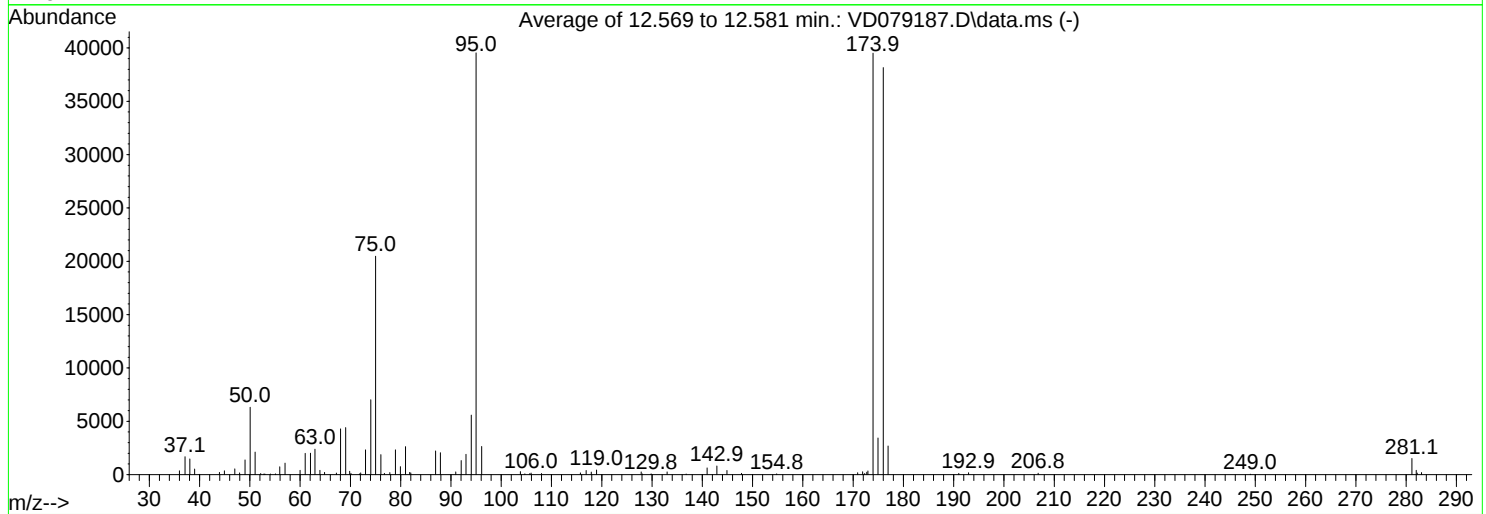


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061424\
Data File : VD079187.D
Acq On : 14 Jun 2024 08:21
Operator : RP/MD
Sample : BFB809
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB809

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM052924SMA.M
Title : SFAM01.0
Last Update : Sat Jun 15 02:21:23 2024

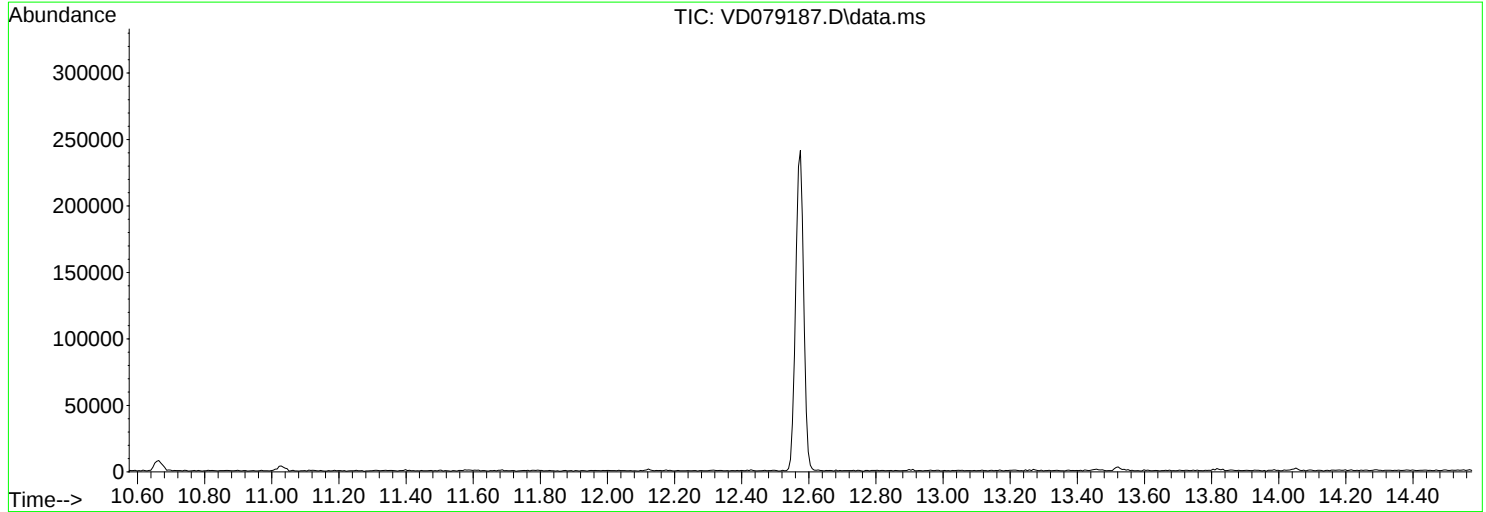

AutoFind: Scans 1867, 1868, 1869; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.0	6323	PASS
75	95	30	80	51.8	20469	PASS
95	95	100	100	100.0	39541	PASS
96	95	5	9	6.7	2644	PASS
173	174	0.00	2	0.9	353	PASS
174	95	50	120	99.9	39509	PASS
175	174	5	9	8.7	3432	PASS
176	174	95	105	96.6	38152	PASS
177	176	5	10	7.0	2687	PASS

m/z	Abundance
39.90	513.0
44.00	377.0

Instrument :
MSVOA_D
ClientSampleId :
BFB809

m/z	Abundance
36.00	420.0
37.10	2099.0
38.10	1627.0
39.00	717.0
40.00	488.0
43.90	393.0
45.00	350.0
47.10	524.0
48.00	302.0
49.10	1634.0
50.00	6978.0
51.10	2448.0
52.10	154.0
52.80	173.0
56.00	819.0
57.00	1022.0
60.00	253.0
61.00	2215.0
62.10	1804.0
63.00	2441.0
64.00	403.0
64.90	176.0
68.00	4927.0
69.00	5210.0
69.90	569.0
71.80	236.0
73.00	2843.0
74.00	7126.0
75.00	22000.0
76.10	1756.0
76.70	159.0
77.90	259.0
79.00	2288.0
79.90	1016.0
81.00	2679.0
81.80	330.0
86.90	2370.0
87.90	2076.0
90.90	229.0
92.00	1459.0
93.00	2127.0
94.00	5680.0
95.00	41312.0
96.10	2614.0
103.90	204.0
104.70	240.0
105.70	316.0
108.00	161.0
115.70	306.0
116.90	411.0
117.80	164.0
118.90	436.0
127.90	321.0
132.90	237.0
141.00	666.0
142.90	690.0
144.80	282.0
171.00	266.0
171.90	241.0
172.70	685.0
173.90	41488.0
174.90	3210.0
176.00	37928.0
176.90	2812.0
281.10	1079.0
282.00	439.0
283.20	169.0

Instrument :
MSVOA_D
ClientSampleId :
BFB809

m/z	Abundance
36.00	380.0
37.10	1748.0
38.10	1526.0
39.00	510.0
40.00	566.0
44.00	758.0
44.90	486.0
46.90	427.0
49.10	1678.0
50.10	6630.0
51.10	2085.0
52.20	174.0
55.10	203.0
55.90	850.0
57.00	1116.0
60.00	505.0
61.00	2060.0
62.00	2162.0
63.00	2761.0
63.90	578.0
64.80	201.0
67.20	260.0
68.10	4506.0
69.10	4612.0
69.80	383.0
72.10	216.0
73.00	2395.0
74.10	7588.0
75.00	22944.0
76.00	1906.0
77.80	339.0
78.90	2840.0
80.00	784.0
80.90	3026.0
82.00	512.0
87.00	2213.0
87.90	2063.0
91.00	222.0
92.10	1305.0
93.00	2323.0
94.10	5787.0
95.00	41976.0
96.10	2650.0
103.70	471.0
106.00	220.0
108.00	162.0
115.80	208.0
116.90	531.0
117.90	284.0
118.90	461.0
127.90	214.0
129.80	250.0
133.00	323.0
136.80	196.0
141.00	636.0
142.90	1032.0
144.90	582.0
147.80	355.0
154.80	248.0
170.80	265.0
171.90	588.0
173.00	525.0
174.00	42608.0
174.90	4191.0
176.00	42088.0
177.00	3270.0
191.00	179.0
192.90	297.0
206.80	232.0
281.20	1811.0
282.00	425.0
282.20	436.0
283.00	432.0

Instrument :
MSVOA_D
ClientSampleId :
BFB809

m/z	Abundance
36.00	281.0
37.00	1195.0
38.00	1240.0
39.10	357.0
40.00	597.0
43.90	596.0
44.90	234.0
47.00	651.0
47.90	186.0
48.90	834.0
50.00	5360.0
51.00	1834.0
53.00	174.0
54.10	194.0
56.00	552.0
57.00	1100.0
60.00	444.0
61.00	1691.0
62.00	2048.0
62.90	1972.0
64.00	232.0
64.90	266.0
67.20	180.0
68.00	3424.0
69.00	3429.0
70.10	362.0
72.00	262.0
73.00	1736.0
74.00	6353.0
75.00	16464.0
76.10	1981.0
76.80	221.0
78.90	1864.0
80.00	455.0
81.00	2193.0
81.80	314.0
87.00	2088.0
87.90	2029.0
91.00	300.0
92.00	1217.0
93.00	1276.0
94.00	5268.0
95.00	35336.0
96.10	2667.0
103.90	166.0
105.90	249.0
117.00	229.0
118.00	272.0
119.00	404.0
127.70	215.0
128.10	199.0
133.10	202.0
140.90	569.0
142.90	700.0
145.00	313.0
172.30	314.0
172.90	535.0
173.90	34432.0
175.00	2895.0
176.00	34440.0
176.90	1978.0
191.00	176.0
193.00	228.0
206.80	193.0
249.00	158.0
281.10	1670.0
282.00	361.0

Instrument :
MSVOA_D
ClientSampleId :
BFB809