

Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD061518\
 Data File : VD058161.D
 Acq On : 15 Jun 2018 19:28
 Operator : VA/AP
 Sample : J3471-01RE
 Misc : 4.25g/5ml/MSVOA D/SOIL
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 #1RE

Quant Time: Jun 16 00:08:27 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060618S.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 07 08:57:33 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	5.64	168	629557	50.00	ug/l	-0.01
34) 1,4-Difluorobenzene	6.69	114	803986	50.00	ug/l	-0.01
63) Chlorobenzene-d5	10.69	117	581262	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	12.90	152	221379	50.00	ug/l	-0.01
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	6.01	65	406151	64.53	ug/l	-0.01
Spiked Amount 50.000			Recovery	=	129.06%	
35) Dibromofluoromethane	5.54	113	431949	69.44	ug/l	-0.02
Spiked Amount 50.000			Recovery	=	138.88%	
50) Toluene-d8	8.70	98	926854	62.67	ug/l	-0.01
Spiked Amount 50.000			Recovery	=	125.34%	
62) 4-Bromofluorobenzene	11.93	95	307698	47.69	ug/l	0.00
Spiked Amount 50.000			Recovery	=	95.38%	


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA D\DATA\VD061518\
Data File : VD058161.D
Acq On : 15 Jun 2018 19:28
Operator : VA/AP
Sample : J3471-01RE
Misc : 4.25g/5ml/MSVOA D/SOIL
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
#1RE

Quant Time: Jun 16 00:08:27 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_D\METHOD\82D060618S.M
Quant Title : SW846 8260
QLast Update : Thu Jun 07 08:57:33 2018
Response via : Initial Calibration

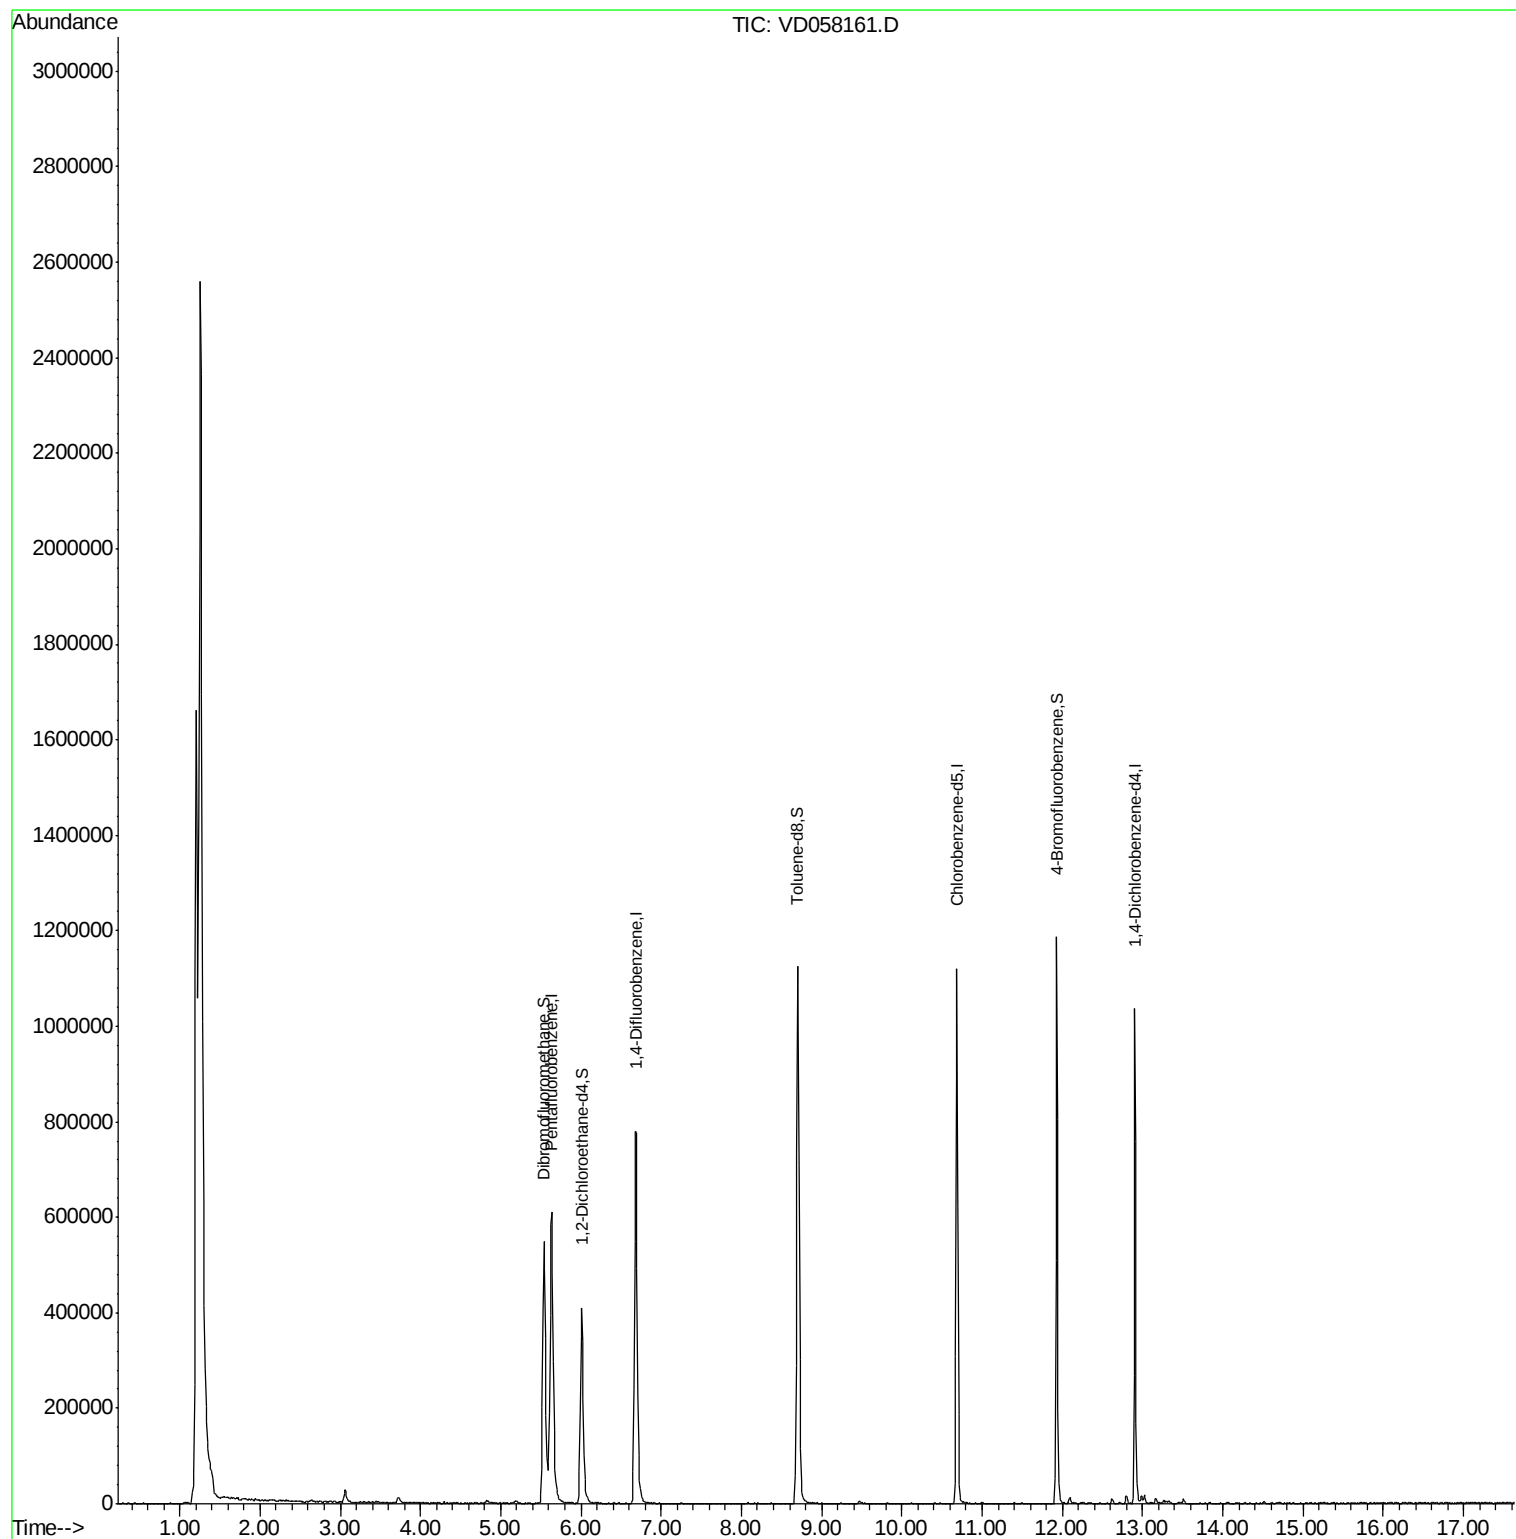

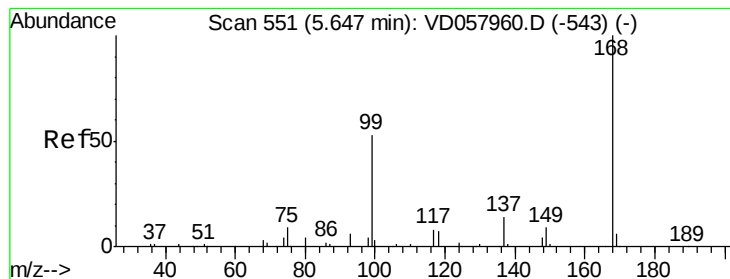

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 5.64 min Scan# 550

Delta R.T. -0.01 min

Lab File: VD058161.D

Acq: 15 Jun 2018 19:28

Instrument :

MSVOA_D

ClientSampleId :


#1RE

Tot Ion:168 Resp: 629557

Ion Ratio Lower Upper




168 100

99 51.6 46.8 70.2

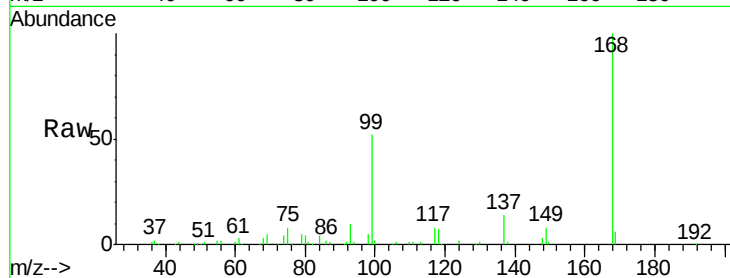

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.95 (98.65 to 99.65): VDC

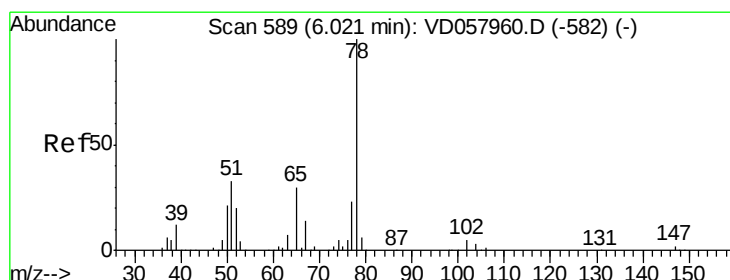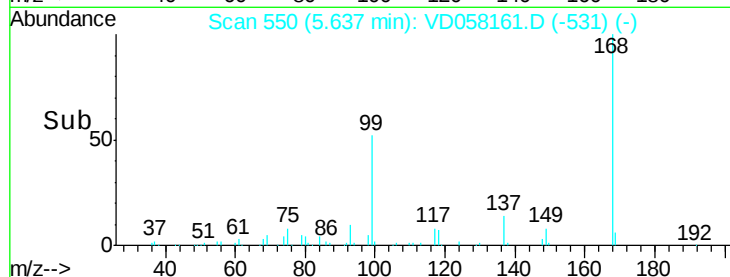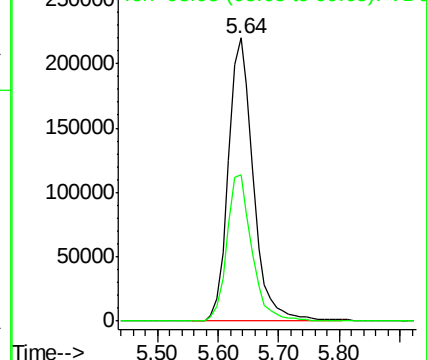

#33

1,2-Dichloroethane-d4

Concen: N.D. ug/l

RT: 6.01 min Scan# 588

Delta R.T. -0.01 min

Lab File: VD058161.D


Acq: 15 Jun 2018 19:28

Tgt Ion: 65 Resp: 406151

Ion Ratio Lower Upper



65 100


67 47.8 0.0 94.0

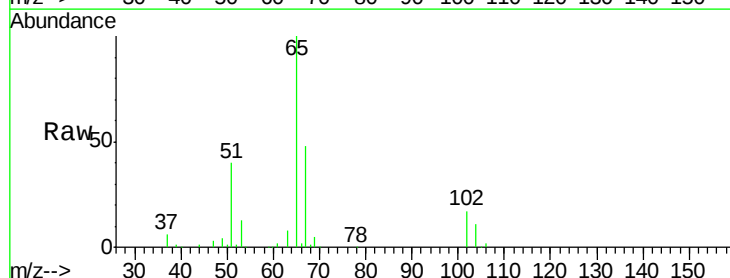

Abundance Ion 64.95 (64.65 to 65.65): VDC

Ion 66.90 (66.60 to 67.60): VDC

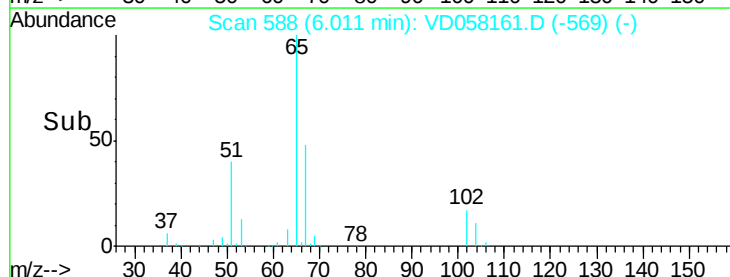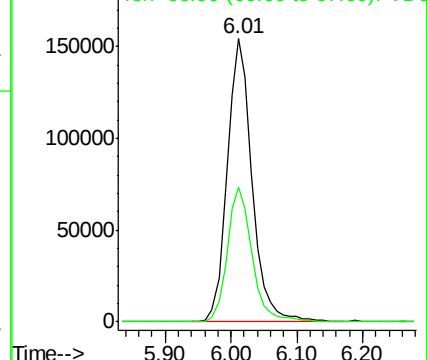

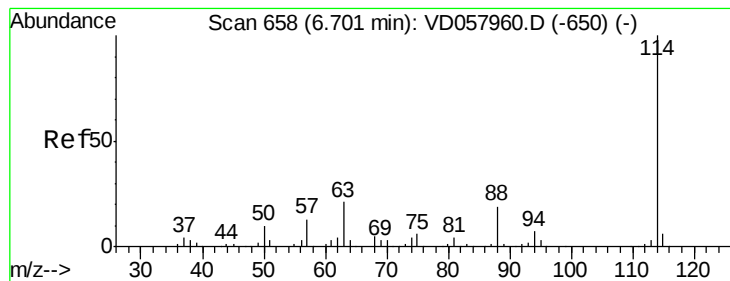

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 6.69 min Scan# 657

Delta R.T. -0.01 min

Lab File: VD058161.D

Acq: 15 Jun 2018 19:28

Instrument :

MSVOA_D

ClientSampleId :

#1RE


Tot Ion:114 Resp: 803986

Ion Ratio Lower Upper

114 100

63 21.4 0.0 42.8




88 19.2 0.0 37.8

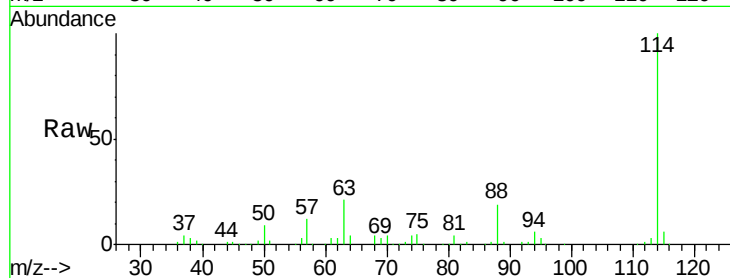

Abundance Ion 114.00 (113.70 to 114.70): V

Ion 62.95 (62.65 to 63.65): V

Ion 87.90 (87.60 to 88.60): V

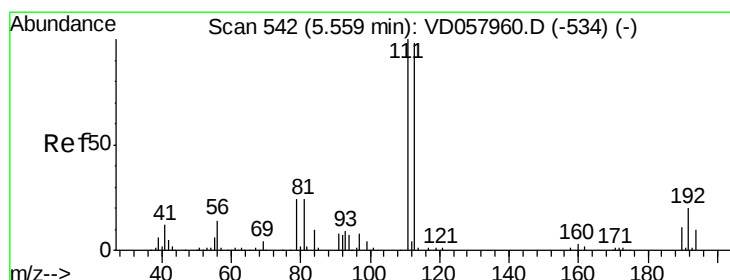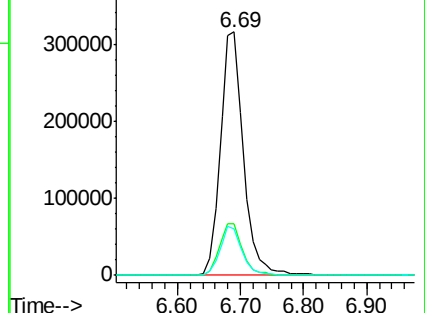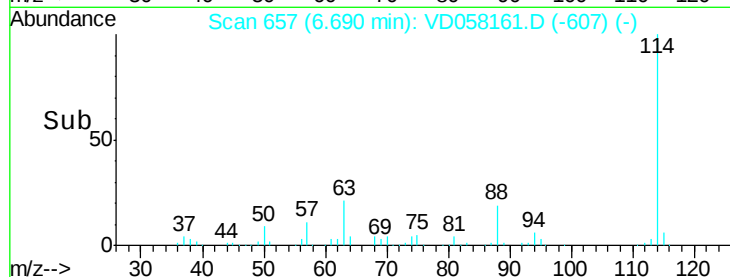

#35

Dibromofluoromethane

Concen: 50.000 ug/l

RT: 5.54 min Scan# 540

Delta R.T. -0.02 min

Lab File: VD058161.D

Acq: 15 Jun 2018 19:28


Tgt Ion:113 Resp: 431949

Ion Ratio Lower Upper

113 100

111 105.1 81.5 122.3



192 20.9 16.4 24.6

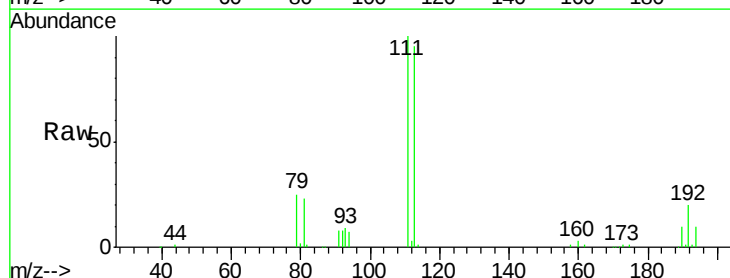


Abundance Ion 112.90 (112.60 to 113.60): V

Ion 110.90 (110.60 to 111.60): V

Ion 191.80 (191.50 to 192.50): V

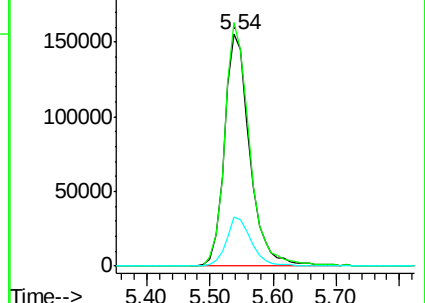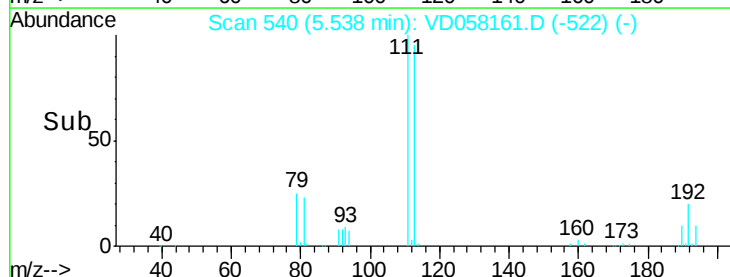


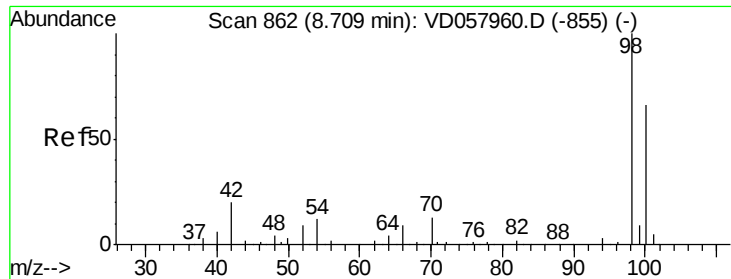




#50
Toluene-d8
Concen: N.D. ug/l
RT: 8.70 min Scan# 861
Delta R.T. -0.01 min
Lab File: VD058161.D
Acq: 15 Jun 2018 19:28

Instrument :
MSVOA_D
ClientSampleId :
#1RE

Tot Ion: 98 Resp: 926854
Ion Ratio Lower Upper
98 100
100 65.3 53.4 80.0

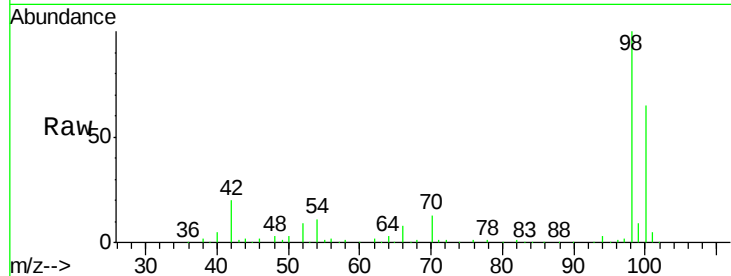


Abundance Ion 98.05 (97.75 to 98.75): VDC
Ion 100.05 (99.75 to 100.75): VDC

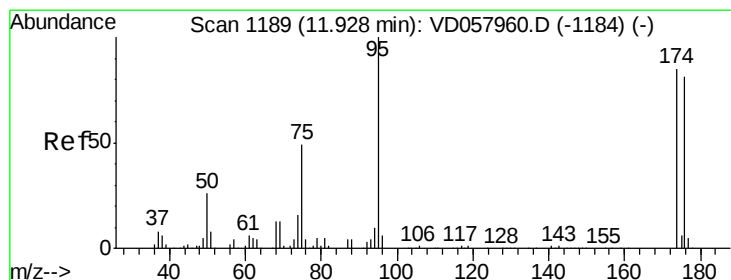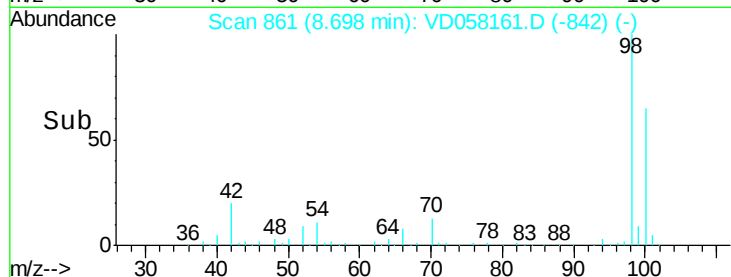
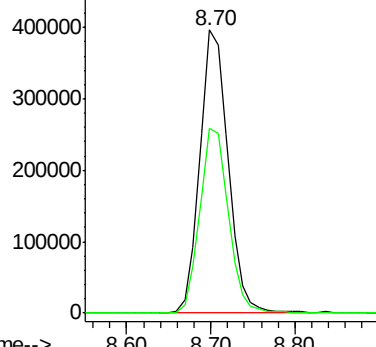



#62
4-Bromofluorobenzene
Concen: N.D. ug/l
RT: 11.93 min Scan# 1189
Delta R.T. -0.00 min
Lab File: VD058161.D
Acq: 15 Jun 2018 19:28

Tgt Ion: 95 Resp: 307698
Ion Ratio Lower Upper
95 100
174 91.1 0.0 169.4
176 90.5 0.0 162.6

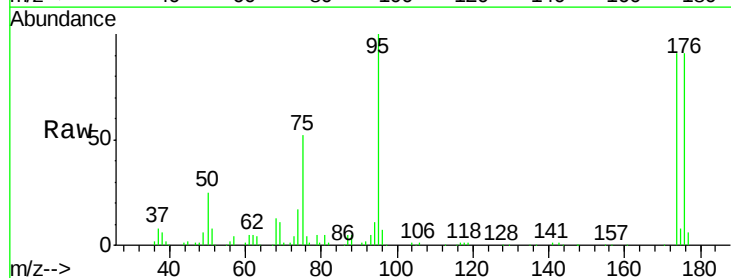

Abundance Ion 95.00 (94.70 to 95.70): VDC
Ion 173.90 (173.60 to 174.60): VDC
Ion 175.90 (175.60 to 176.60): VDC

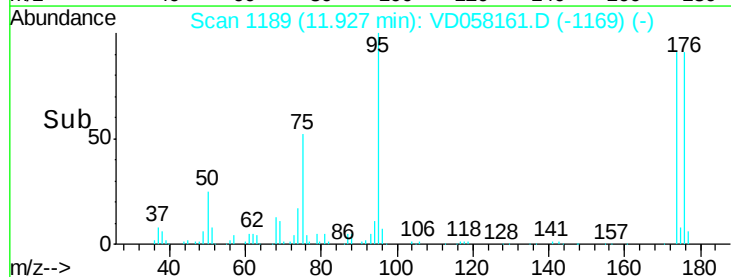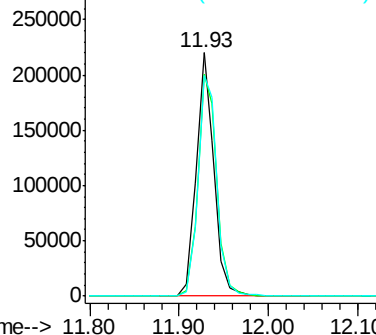


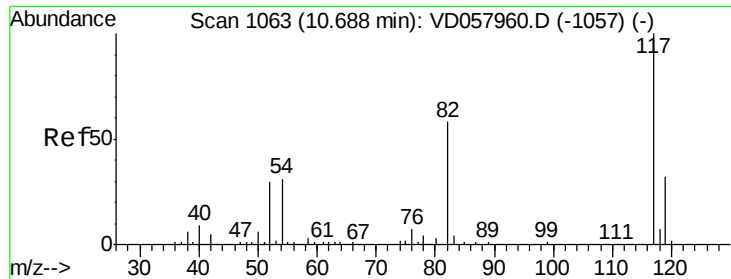




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 10.69 min Scan# 1063
Delta R.T. -0.00 min
Lab File: VD058161.D
Acq: 15 Jun 2018 19:28

Instrument :
MSVOA_D
ClientSampleId :
#1RE

Tot Ion:117 Resp: 581262
Ion Ratio Lower Upper
117 100
82 58.5 46.8 70.2
119 32.9 25.8 38.6

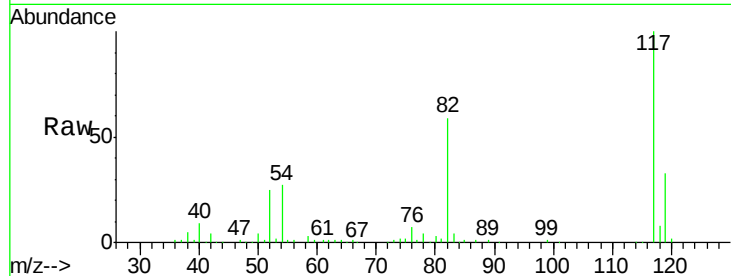


Abundance Ion 116.95 (116.65 to 117.65): V
Ion 82.05 (81.75 to 82.75): V
Ion 118.95 (118.65 to 119.65): V

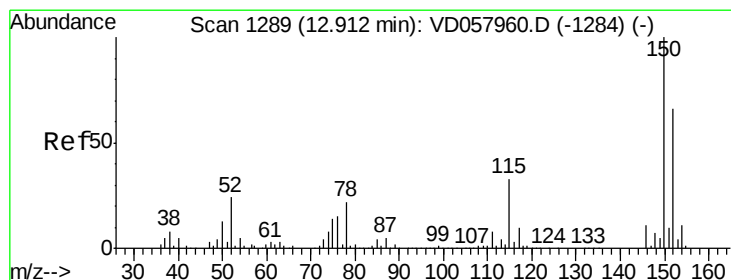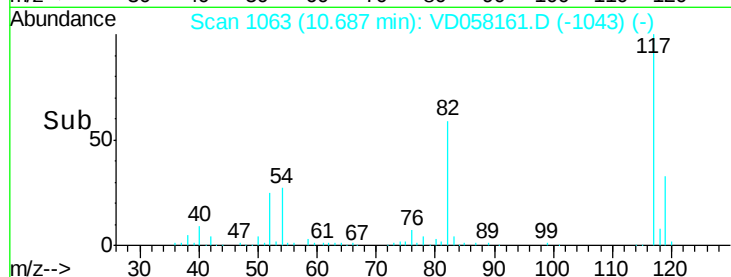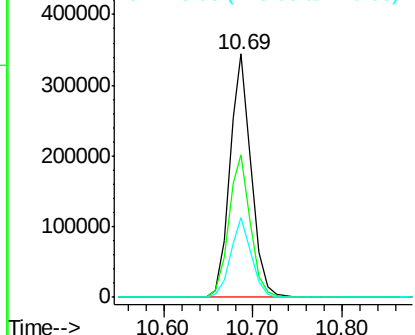

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 12.90 min Scan# 1288
Delta R.T. -0.01 min
Lab File: VD058161.D
Acq: 15 Jun 2018 19:28

Tgt Ion:152 Resp: 221379
Ion Ratio Lower Upper
152 100
115 55.7 25.6 76.6
150 153.7 0.0 306.8

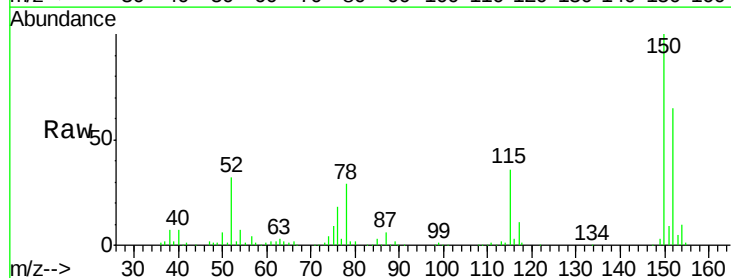

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 115.00 (114.70 to 115.70): V
Ion 149.90 (149.60 to 150.60): V

