


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061518\
 Data File : VD058152.D
 Acq On : 15 Jun 2018 13:22
 Operator : VA/AP
 Sample : BFB
 Misc : 5.00g/5ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060618S.M
 Title : SW846 8260
 Last Update : Thu Jun 07 08:57:33 2018

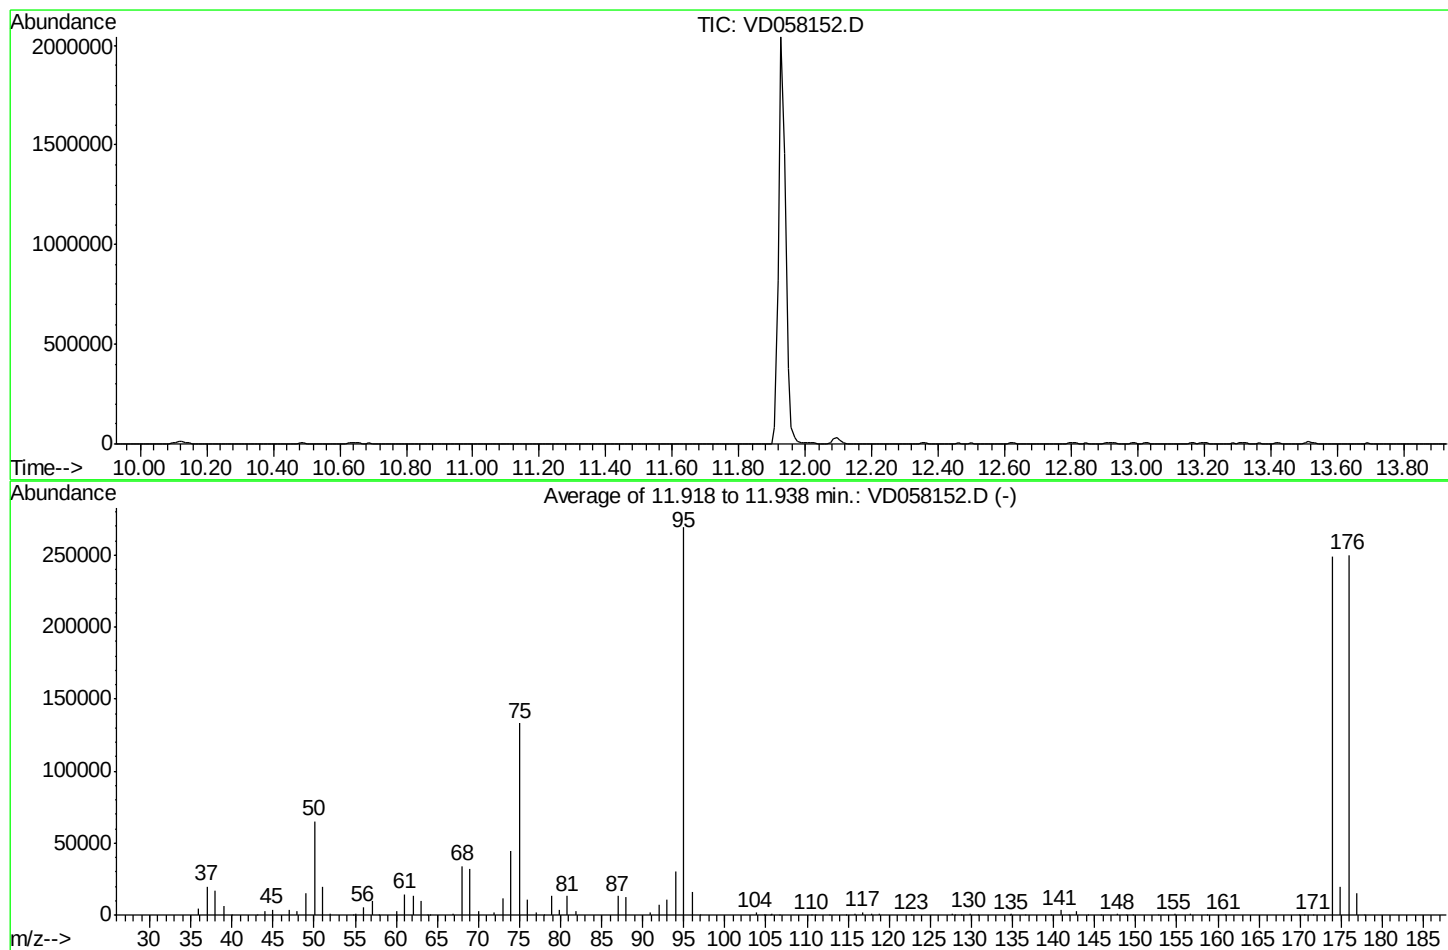

AutoFind: Scans 1188, 1189, 1190; Background Corrected with Scan 1183

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	24.2	65053	PASS
75	95	30	60	49.4	132941	PASS
95	95	100	100	100.0	269205	PASS
96	95	5	9	6.0	16278	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	92.5	248954	PASS
175	174	5	9	7.7	19213	PASS
176	174	95	101	100.4	250037	PASS
177	176	5	9	6.1	15129	PASS