

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061622\
 Data File : VD073611.D
 Acq On : 16 Jun 2022 12:10
 Operator : VA/SY
 Sample : N3329-03
 Misc : 5.01G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 PALMYRA-RT-73-COMP-2

Quant Time: Jun 16 15:11:16 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D060922S.M
 Quant Title : SW846 8260
 QLast Update : Thu Jun 09 12:33:32 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.973	168	305683	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.861	114	517809	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.638	117	472240	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.561	152	209841	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.326	65	162150	49.430	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	=	98.860%
35) Dibromofluoromethane	7.908	113	166845	50.108	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	=	100.220%
50) Toluene-d8	10.332	98	608171	48.309	ug/l	0.00
Spiked Amount	50.000	Range	49 - 140	Recovery	=	96.620%
62) 4-Bromofluorobenzene	12.620	95	194126	42.476	ug/l	0.00
Spiked Amount	50.000	Range	25 - 144	Recovery	=	84.960%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061622\
Data File : VD073611.D
Acq On : 16 Jun 2022 12:10
Operator : VA/SY
Sample : N3329-03
Misc : 5.01G/5.00ml/MSVOA_D/SOIL
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
PALMYRA-RT-73-COMP-2

Quant Time: Jun 16 15:11:16 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D060922S.M
Quant Title : SW846 8260
QLast Update : Thu Jun 09 12:33:32 2022
Response via : Initial Calibration




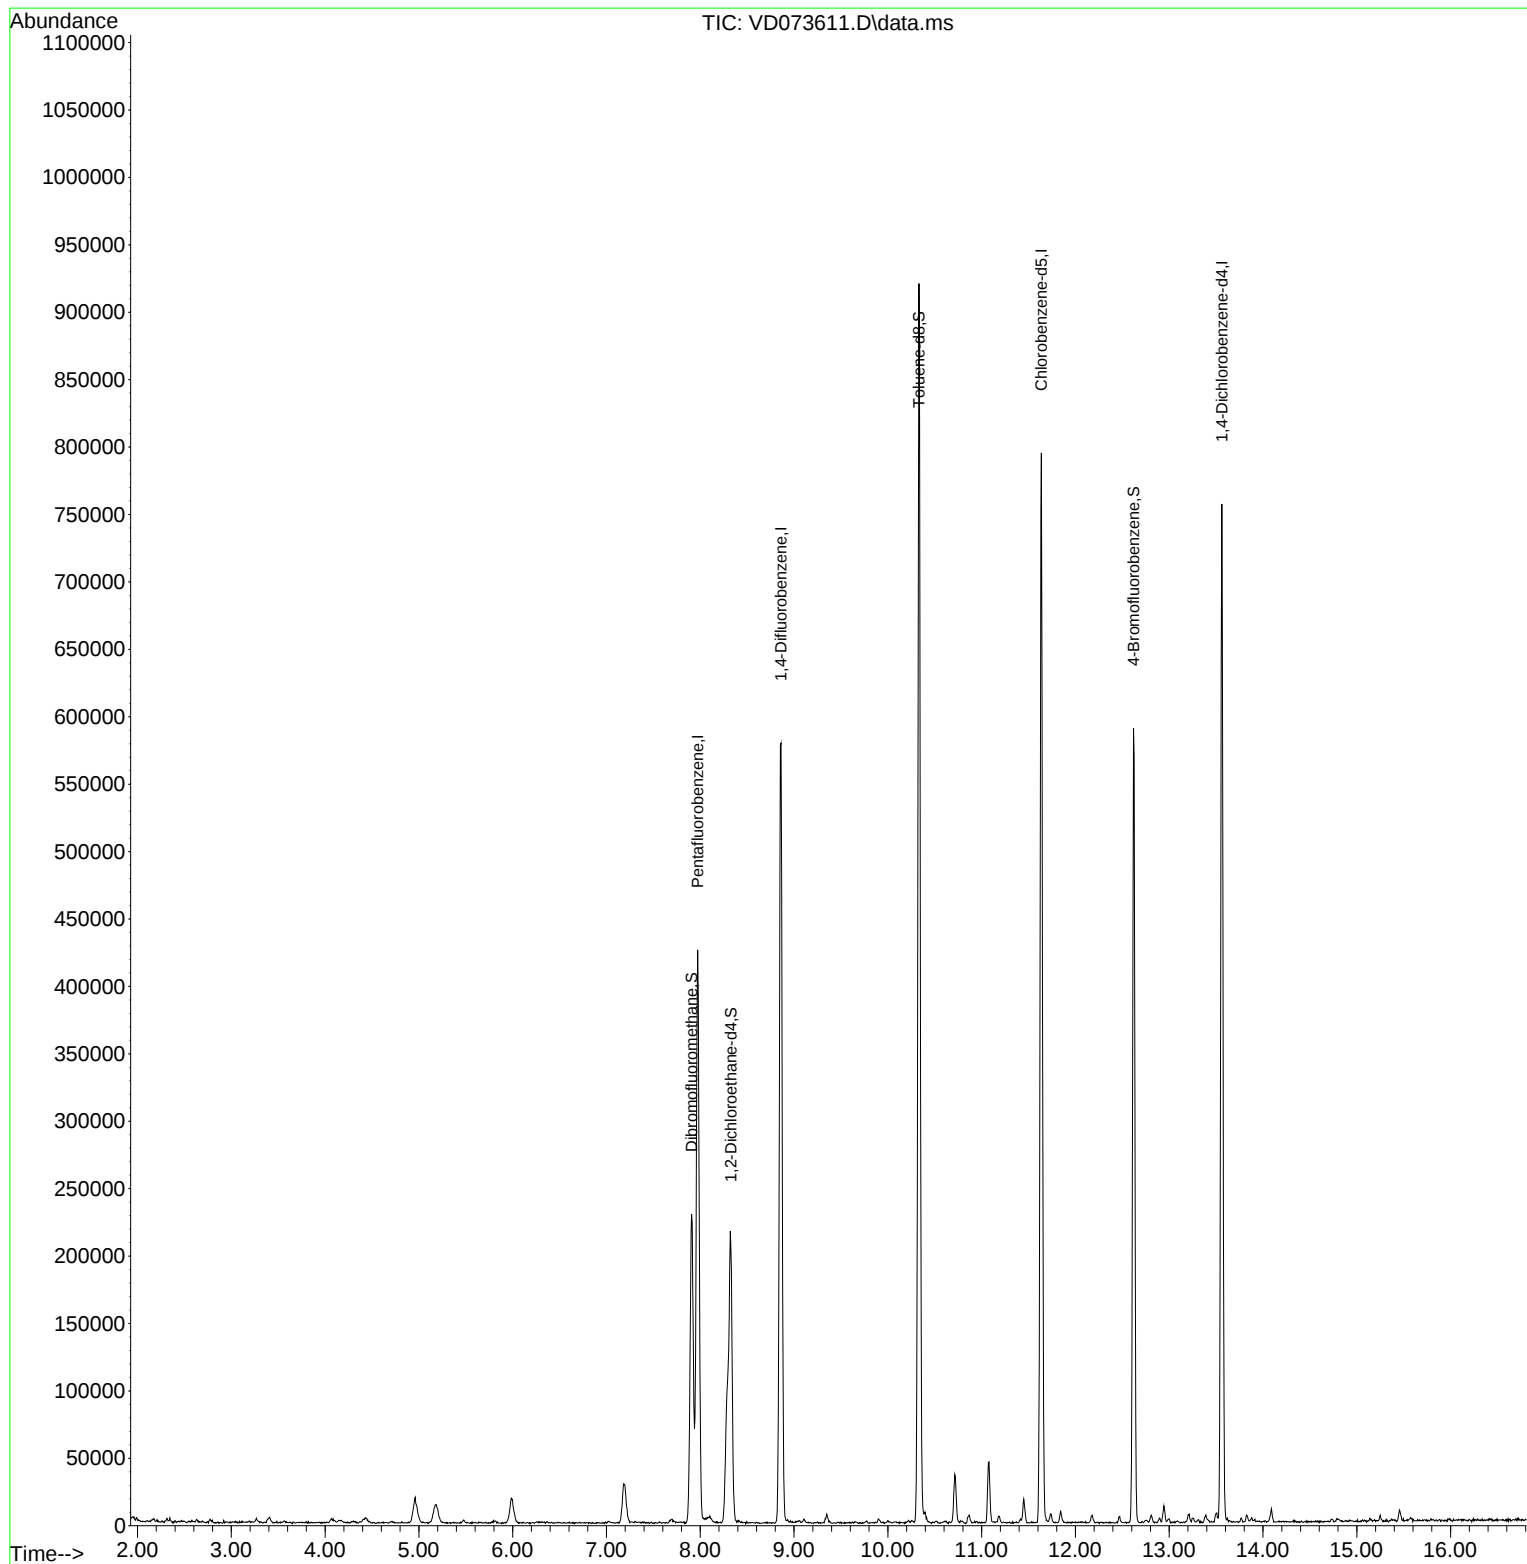


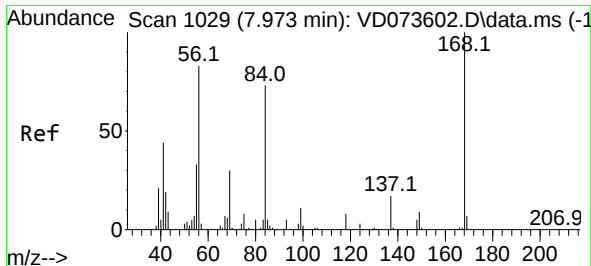

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 7.973 min Scan# 1029
Delta R.T. 0.000 min
Lab File: VD073611.D
Acq: 16 Jun 2022 12:10




Instrument :
MSVOA_D
ClientSampleId :
PALMYRA-RT-73-COMP-2


Tgt Ion:168 Resp: 305683
Ion Ratio Lower Upper
168 100
99 55.2 49.8 74.6

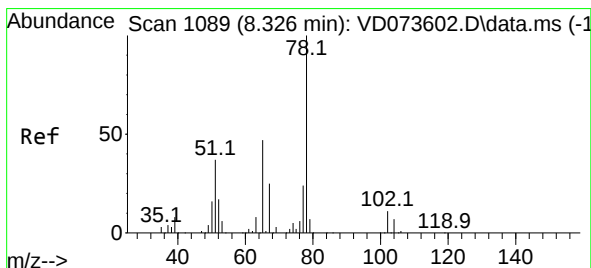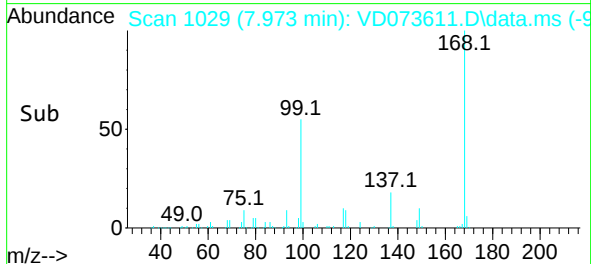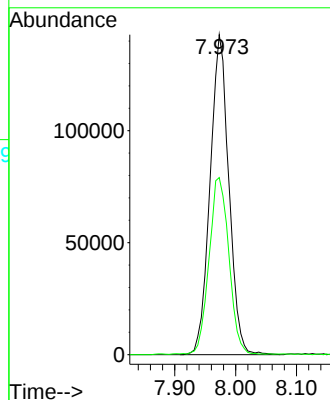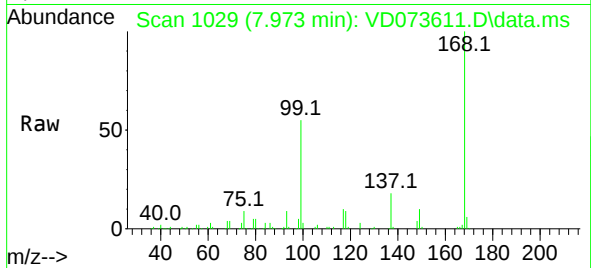

#33
1,2-Dichloroethane-d4
Concen: 49.430 ug/l
RT: 8.326 min Scan# 1089
Delta R.T. 0.006 min
Lab File: VD073611.D
Acq: 16 Jun 2022 12:10

Tgt Ion: 65 Resp: 162150
Ion Ratio Lower Upper
65 100
67 53.0 0.0 101.4

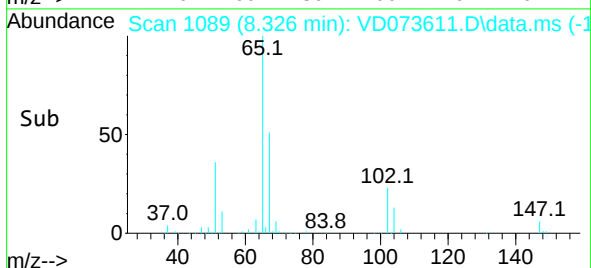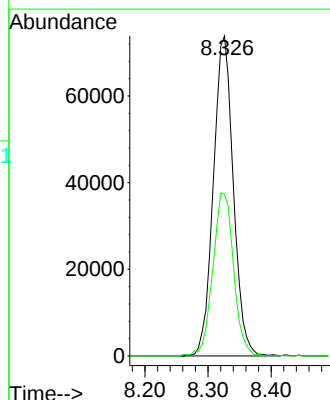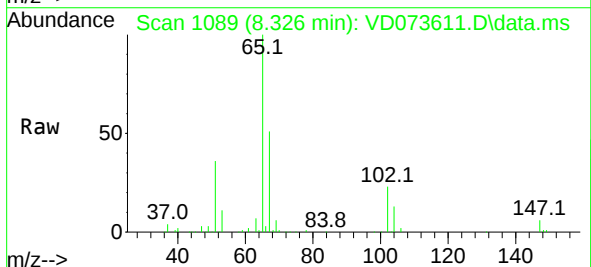

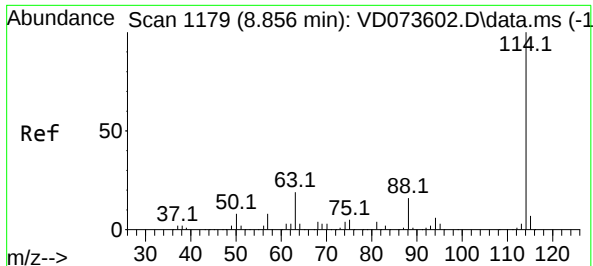

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.861 min Scan# 1179

Delta R.T. 0.006 min

Lab File: VD073611.D

Acq: 16 Jun 2022 12:10

Instrument :

MSVOA_D

ClientSampleId :

PALMYRA-RT-73-COMP-2





Tgt Ion:114 Resp: 517809

Ion Ratio Lower Upper

114 100

63 19.9 0.0 46.6

88 15.1 0.0 33.2

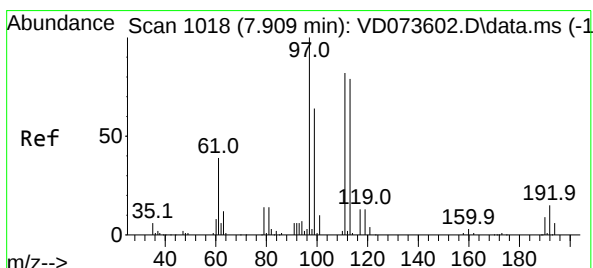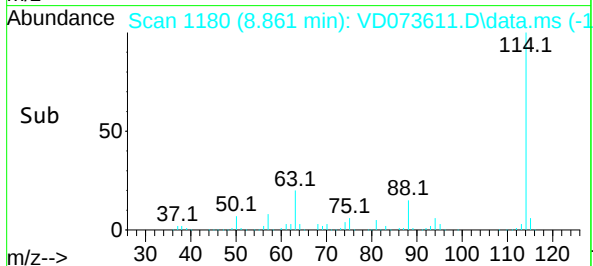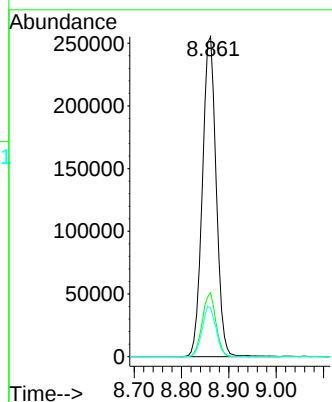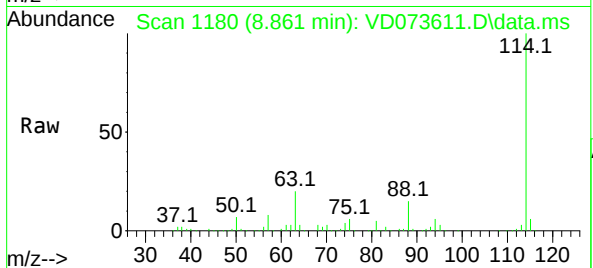

#35

Dibromofluoromethane

Concen: 50.108 ug/l

RT: 7.908 min Scan# 1018

Delta R.T. 0.000 min

Lab File: VD073611.D

Acq: 16 Jun 2022 12:10




Tgt Ion:113 Resp: 166845


Ion Ratio Lower Upper

113 100

111 103.2 83.8 125.6

192 19.5 14.6 21.8


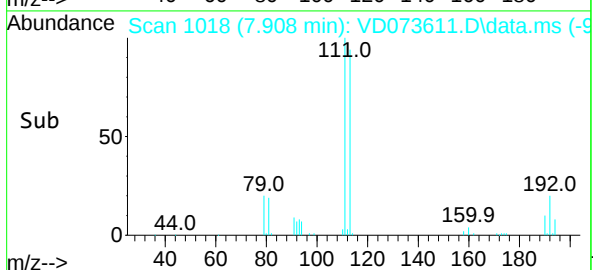
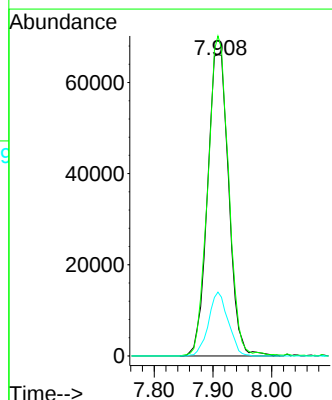
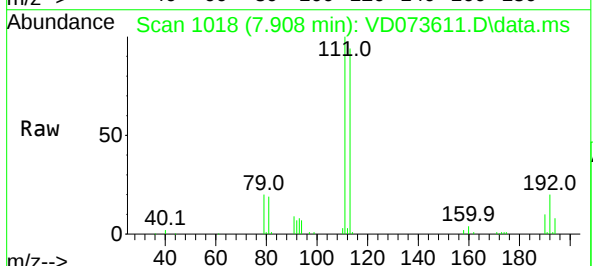


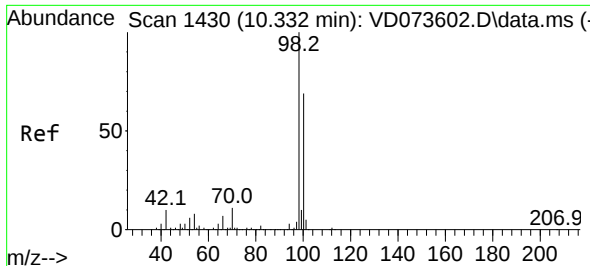

#50
Toluene-d8
Concen: 48.309 ug/l
RT: 10.332 min Scan# 1430
Delta R.T. -0.000 min
Lab File: VD073611.D
Acq: 16 Jun 2022 12:10




Instrument :
MSVOA_D
ClientSampleId :
PALMYRA-RT-73-COMP-2


Tgt Ion: 98 Resp: 608171
Ion Ratio Lower Upper
98 100
100 66.2 52.4 78.6

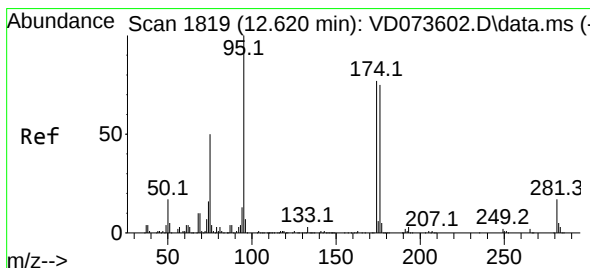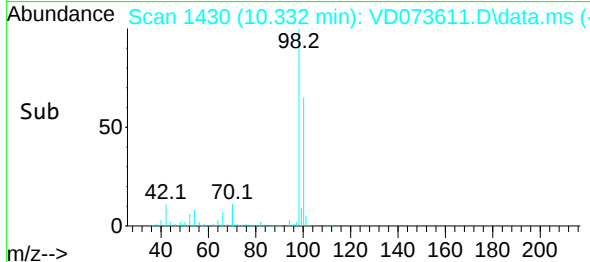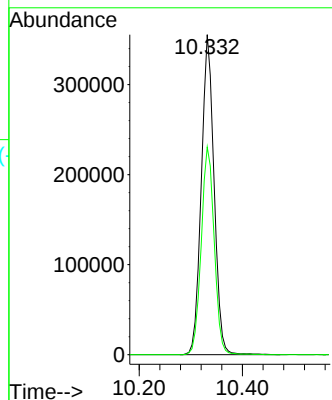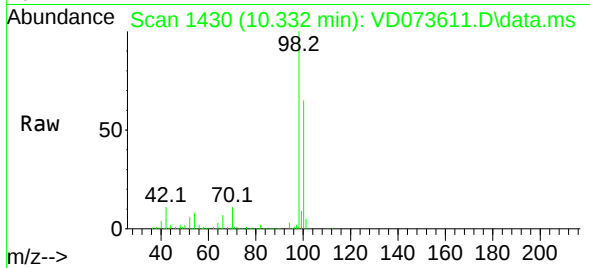

#62
4-Bromofluorobenzene
Concen: 42.476 ug/l
RT: 12.620 min Scan# 1819
Delta R.T. -0.000 min
Lab File: VD073611.D
Acq: 16 Jun 2022 12:10

Tgt Ion: 95 Resp: 194126
Ion Ratio Lower Upper
95 100
174 80.6 0.0 152.8
176 75.9 0.0 145.4


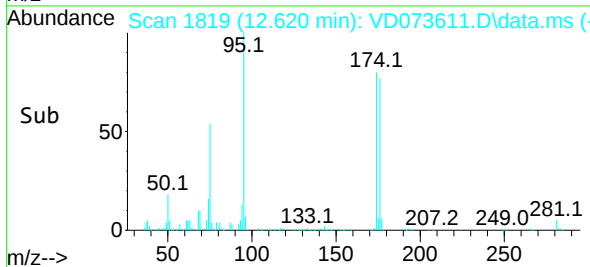
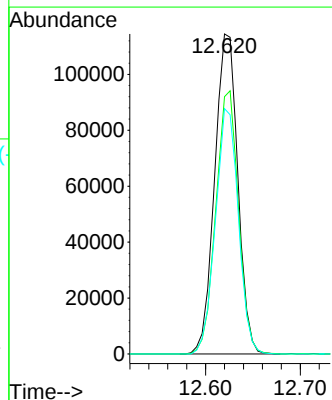
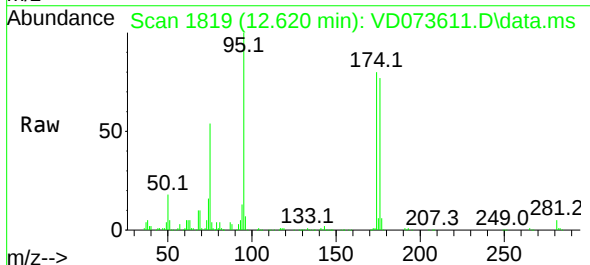


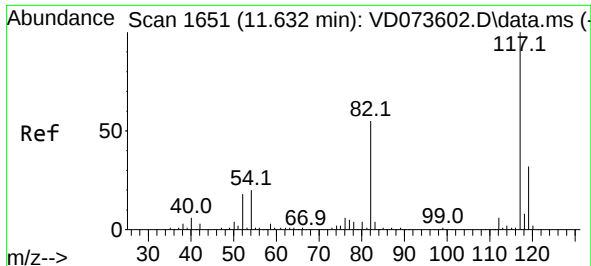

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.638 min Scan# 117
Delta R.T. 0.006 min
Lab File: VD073611.D
Acq: 16 Jun 2022 12:10

Instrument :
MSVOA_D
ClientSampleId :
PALMYRA-RT-73-COMP-2

Tgt Ion:117 Resp: 472240
Ion Ratio Lower Upper
117 100
82 54.9 45.3 67.9
119 31.5 26.6 40.0

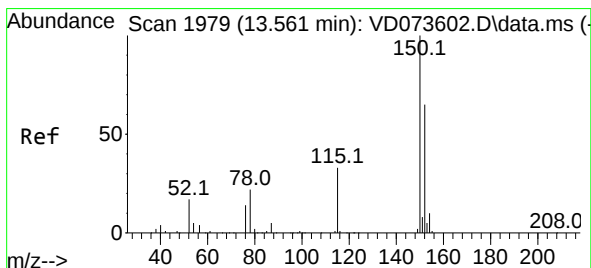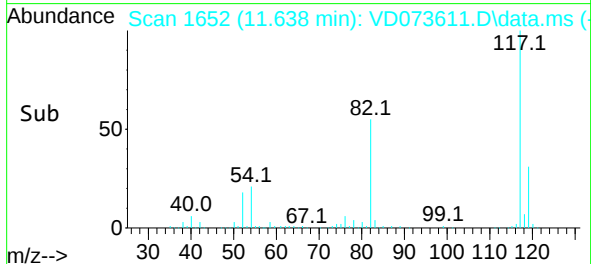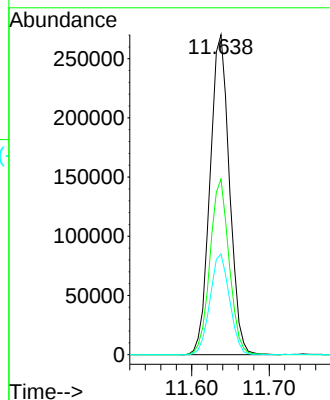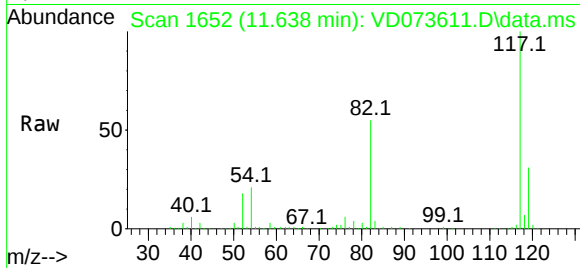

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.561 min Scan# 1979
Delta R.T. 0.000 min
Lab File: VD073611.D
Acq: 16 Jun 2022 12:10

Tgt Ion:152 Resp: 209841
Ion Ratio Lower Upper
152 100
115 60.0 31.3 93.8
150 156.0 0.0 348.6

