


Data Path : Z:\voasrv\HPCHEM1\MSVOA D\Data\VD061818\
Data File : VD058174.D
Acq On : 18 Jun 2018 9:52
Operator : VA/AP
Sample : BFB
Misc : 5.00µl/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D060618S.M
Title : SW846 8260
Last Update : Thu Jun 07 08:57:33 2018

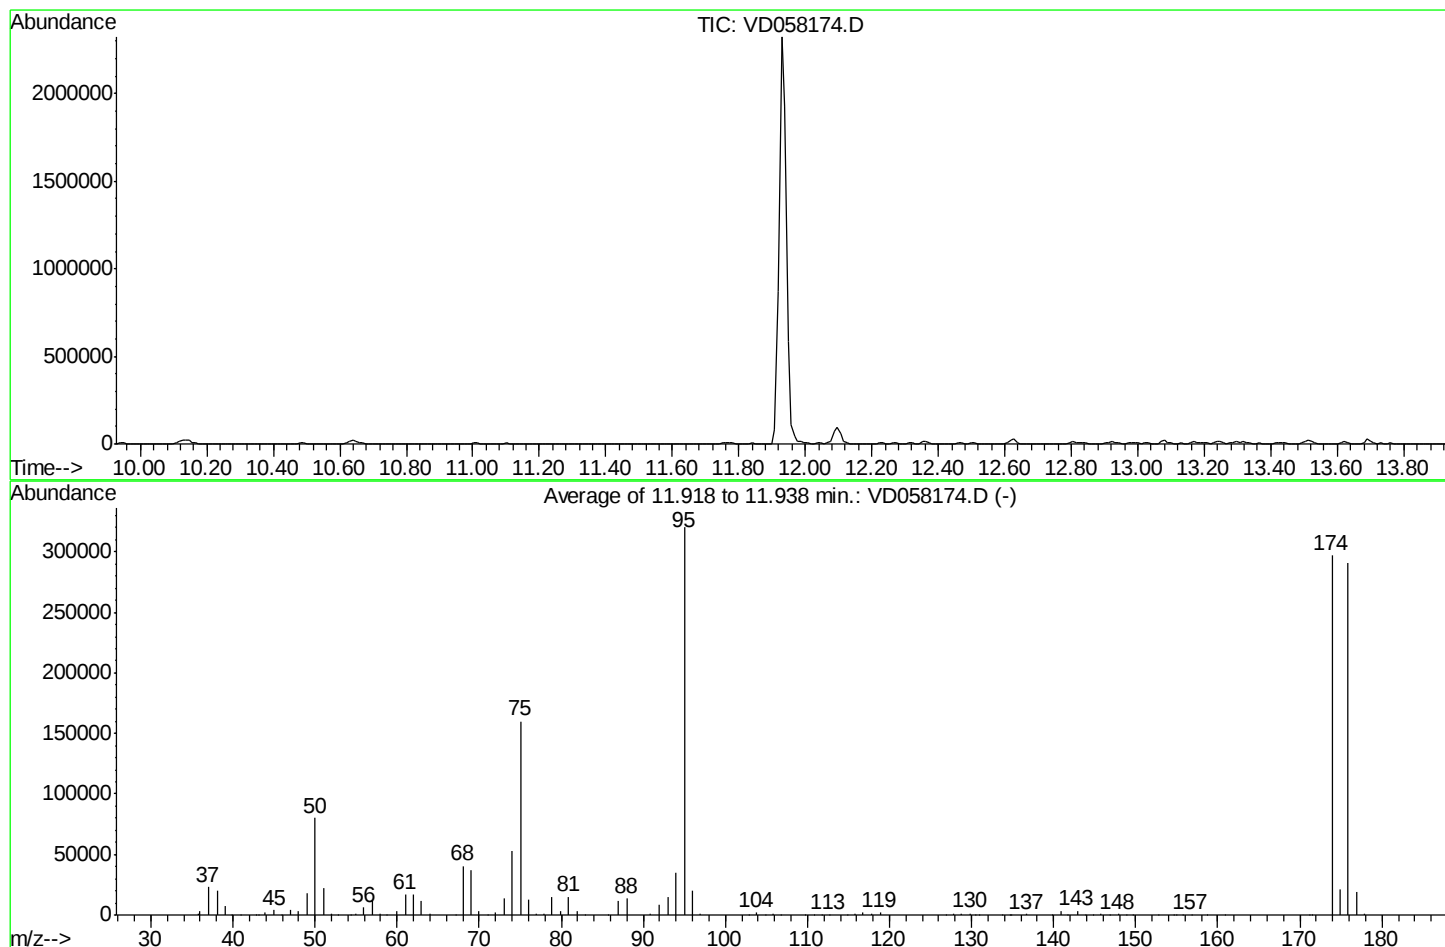

AutoFind: Scans 1188, 1189, 1190; Background Corrected with Scan 1183

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.0	80109	PASS
75	95	30	60	49.9	159864	PASS
95	95	100	100	100.0	320320	PASS
96	95	5	9	6.3	20084	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	92.8	297200	PASS
175	174	5	9	7.3	21558	PASS
176	174	95	101	97.7	290474	PASS
177	176	5	9	6.4	18559	PASS