
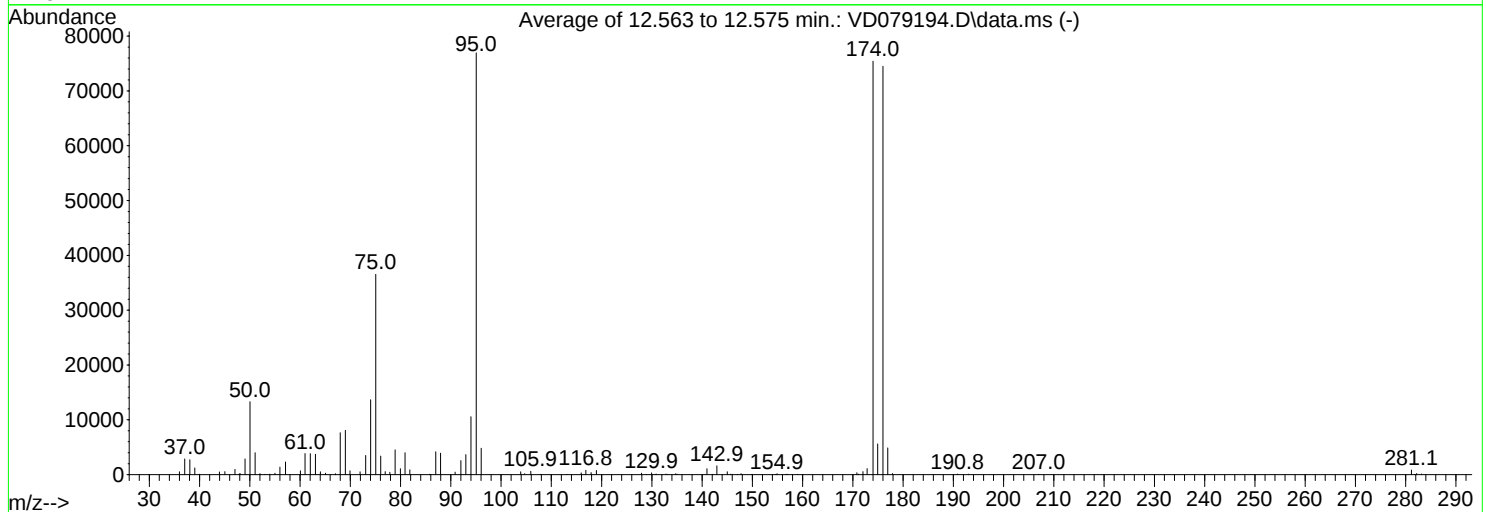


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061824\
Data File : VD079194.D
Acq On : 18 Jun 2024 08:40
Operator : RP/MD
Sample : BFB810
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB810

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM052924SMA.M
Title : SFAM01.0
Last Update : Wed Jun 19 07:16:52 2024

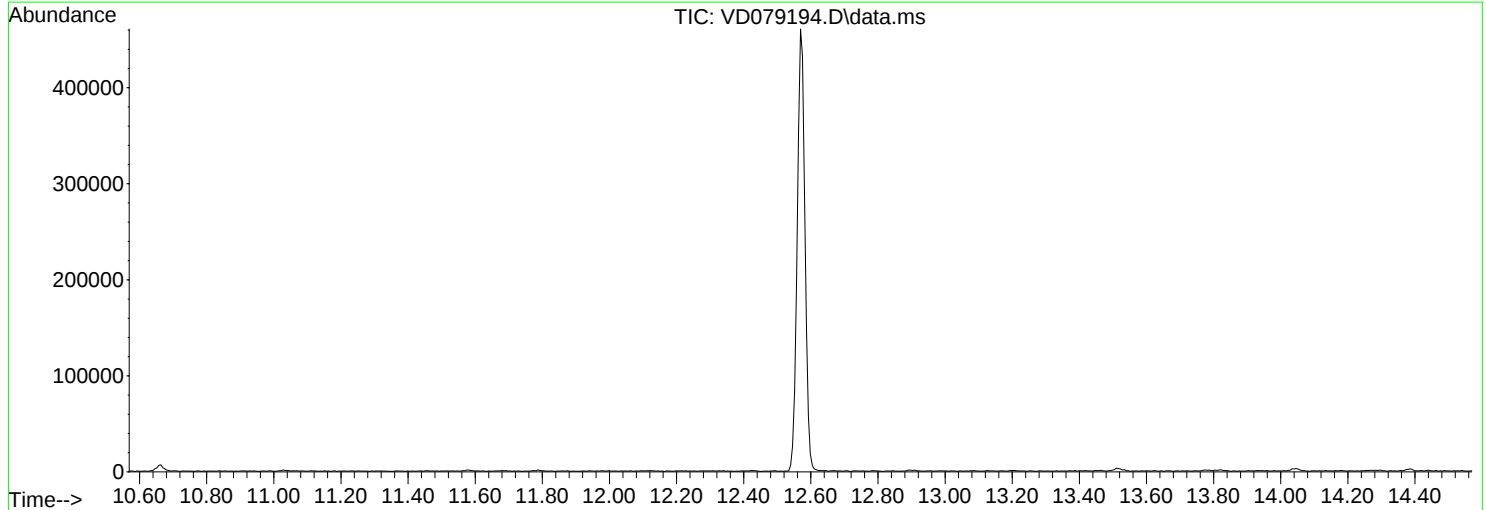

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1859

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	17.3	13296	PASS
75	95	30	80	47.5	36555	PASS
95	95	100	100	100.0	76947	PASS
96	95	5	9	6.3	4811	PASS
173	174	0.00	2	1.5	1125	PASS
174	95	50	120	98.0	75424	PASS
175	174	5	9	7.4	5592	PASS
176	174	95	105	98.8	74499	PASS
177	176	5	10	6.6	4884	PASS

m/z	Abundance
39.90	538.0
44.00	257.0

Instrument :
MSVOA_D
ClientSampleId :
BFB810

m/z	Abundance
36.10	454.0
37.10	2744.0
38.10	2298.0
39.00	1261.0
40.00	640.0
44.00	731.0
45.00	636.0
47.00	1126.0
47.90	429.0
49.10	2963.0
50.10	11380.0
51.10	3662.0
52.00	210.0
53.00	151.0
55.00	188.0
56.00	1162.0
57.10	1859.0
60.00	398.0
61.00	3640.0
62.10	3575.0
63.00	3450.0
64.10	390.0
65.10	231.0
67.00	233.0
68.00	6759.0
69.00	7383.0
70.00	655.0
71.90	407.0
73.00	3480.0
74.10	11556.0
75.10	31456.0
76.10	2729.0
77.00	677.0
77.80	223.0
78.90	4083.0
80.00	856.0
80.90	3631.0
81.90	707.0
87.10	3472.0
87.90	3226.0
90.80	289.0
92.00	1874.0
93.00	3043.0
94.00	8934.0
95.00	64064.0
96.10	3727.0
103.90	382.0
105.90	464.0
107.90	153.0
116.00	243.0
116.80	621.0
117.80	303.0
118.90	696.0
129.90	206.0
134.70	323.0
141.00	894.0
143.00	1314.0
145.10	701.0
146.00	167.0
147.80	242.0
154.70	154.0
170.90	399.0
172.00	586.0
172.90	1063.0
174.00	62144.0
175.00	4481.0
176.00	61144.0
176.90	4020.0
178.00	239.0
281.20	802.0
282.20	274.0

Instrument :
MSVOA_D
ClientSampleId :
BFB810

m/z	Abundance
36.00	534.0
37.10	3164.0
38.00	3235.0
39.10	1285.0
40.10	748.0
44.00	756.0
45.00	574.0
47.10	948.0
48.10	264.0
49.00	2906.0
50.10	15264.0
51.00	4093.0
52.00	356.0
55.00	307.0
56.00	1511.0
57.10	2608.0
60.00	1039.0
61.00	4088.0
62.00	4257.0
63.00	3807.0
64.00	714.0
65.00	368.0
68.00	8596.0
69.00	8826.0
69.90	605.0
71.90	665.0
73.10	4088.0
74.00	13799.0
75.00	41208.0
76.00	4037.0
76.90	466.0
77.90	538.0
78.90	5117.0
79.90	1162.0
80.90	4508.0
81.80	857.0
85.80	153.0
86.90	4849.0
88.00	4687.0
90.90	645.0
92.00	2939.0
93.00	4011.0
94.00	11285.0
95.10	86896.0
96.00	5753.0
103.90	569.0
104.70	206.0
105.90	773.0
116.00	215.0
116.90	777.0
117.90	565.0
118.90	906.0
128.00	306.0
128.90	221.0
130.00	335.0
130.90	176.0
132.80	164.0
133.20	187.0
134.80	227.0
141.00	1314.0
142.10	157.0
142.90	1842.0
145.00	621.0
147.00	181.0
149.90	192.0
154.90	278.0
156.70	183.0
159.00	221.0
170.70	336.0
171.10	294.0
172.00	704.0
172.80	1351.0
174.00	84224.0
174.90	6266.0
176.00	81896.0
177.00	5236.0
177.90	194.0
190.90	172.0
281.10	939.0
281.80	215.0
283.20	205.0

Instrument :
MSVOA_D
ClientSampleId :
BFB810

m/z	Abundance
35.90	557.0
37.00	2688.0
38.00	2660.0
39.10	1176.0
40.00	531.0
43.90	769.0
45.10	441.0
47.00	827.0
48.00	372.0
49.00	2716.0
50.00	13243.0
51.00	4216.0
52.20	158.0
54.00	255.0
55.00	340.0
56.00	1427.0
57.10	2465.0
60.10	659.0
61.00	3845.0
62.10	3672.0
63.10	3851.0
64.10	457.0
65.10	232.0
67.10	316.0
68.00	7629.0
69.00	8071.0
70.00	822.0
72.00	504.0
73.10	2940.0
74.00	15603.0
75.00	37000.0
76.00	3401.0
76.90	571.0
77.80	594.0
78.90	4368.0
79.90	1189.0
80.90	3830.0
81.90	1048.0
86.00	202.0
87.00	4212.0
87.90	3812.0
90.90	508.0
92.00	2875.0
93.00	3932.0
94.00	11472.0
95.10	79880.0
96.10	4953.0
103.70	299.0
104.00	318.0
104.70	297.0
105.90	622.0
113.10	189.0
115.90	486.0
116.90	1005.0
118.00	277.0
119.00	676.0
127.90	481.0
129.90	427.0
130.80	179.0
132.80	218.0
135.00	310.0
140.90	1000.0
143.00	1663.0
144.90	278.0
145.70	253.0
147.70	323.0
154.90	244.0
156.90	266.0
170.80	317.0
172.10	375.0
172.90	962.0
174.00	79904.0
175.00	6030.0
176.00	80456.0
177.00	5396.0
177.80	161.0
190.80	181.0
193.00	245.0
207.00	207.0
281.10	799.0
282.20	374.0
283.10	180.0

Instrument :
MSVOA_D
ClientSampleId :
BFB810