
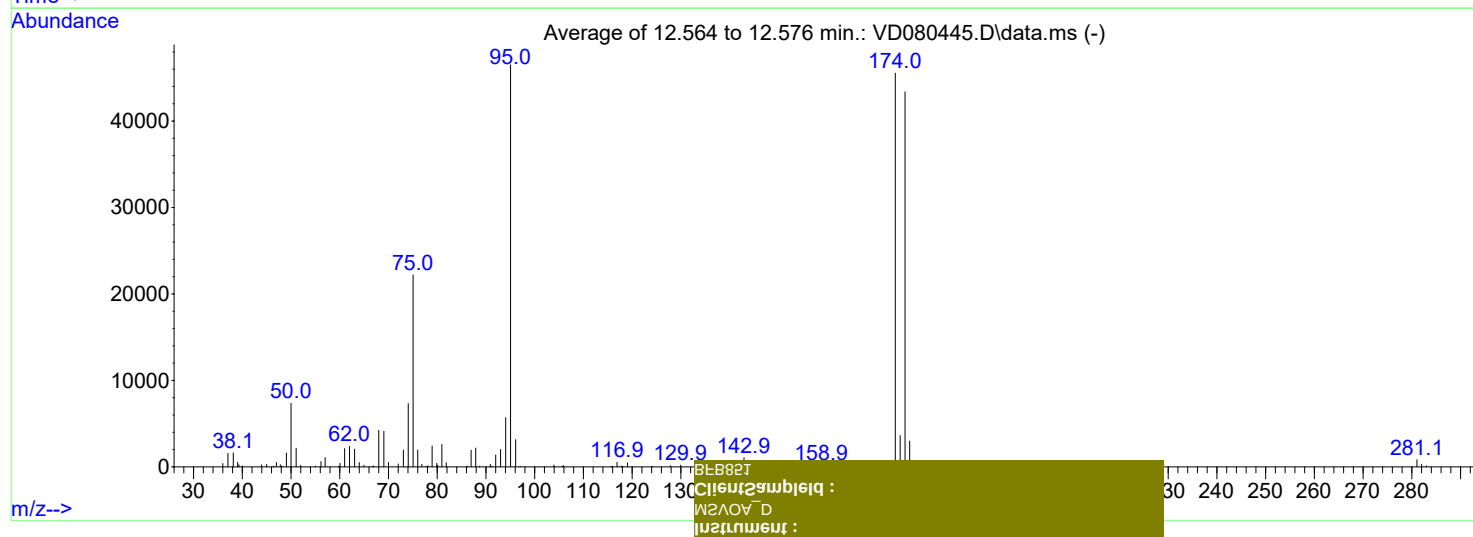


Data Path : D:\MassHunter\GCMS\1\data\VD061825\
Data File : VD080445.D
Acq On : 18 Jun 2025 08:36
Operator : RP/MD
Sample : BFB851
Misc : 5.00G/5ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM061825SMA.M
Title : SFAM01.0
Last Update : Tue Jun 17 09:27:31 2025

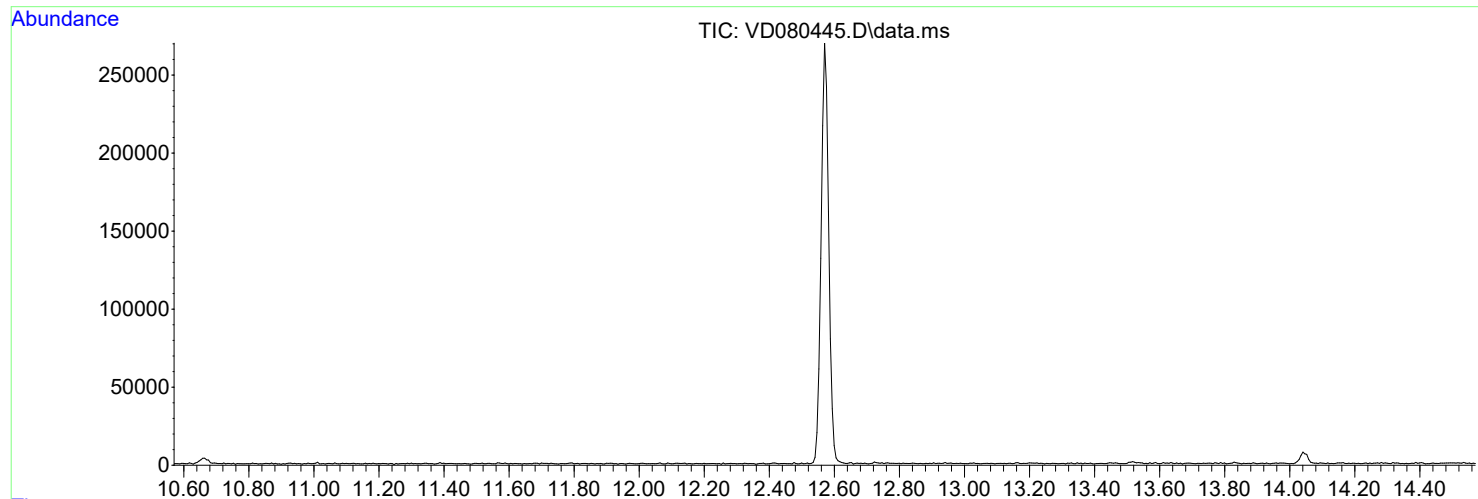

AutoFind: Scans 1835, 1836, 1837; Background Corrected with Scan 1828

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.8	7352	PASS
75	95	30	80	47.7	22197	PASS
95	95	100	100	100.0	46496	PASS
96	95	5	9	6.8	3153	PASS
173	174	0.00	2	0.6	271	PASS
174	95	50	120	97.9	45541	PASS
175	174	5	9	8.0	3624	PASS
176	174	95	105	95.3	43384	PASS
177	176	5	10	6.9	2987	PASS

m/z	Abundance
40.10	625.0
44.00	321.0

BFB82T
Client Sample :
MS/MS.D
Instrument :

m/z	Abundance
36.00	338.0
37.00	1422.0
38.10	1619.0
39.00	744.0
40.00	732.0
43.90	361.0
45.10	206.0
47.00	385.0
47.90	317.0
49.00	1450.0
50.00	6907.0
51.00	1841.0
55.00	256.0
56.10	631.0
57.00	1013.0
59.80	215.0
60.20	201.0
61.00	1653.0
62.00	2126.0
63.10	1762.0
64.00	265.0
66.80	194.0
68.00	3961.0
69.10	3643.0
70.00	558.0
72.10	213.0
73.10	1861.0
74.10	5745.0
75.10	20464.0
76.00	2008.0
76.80	297.0
78.10	237.0
78.90	2407.0
79.90	589.0
81.00	2466.0
82.00	333.0
86.90	1695.0
87.90	1902.0
91.00	338.0
92.10	1522.0
93.00	1838.0
94.00	4622.0
95.10	42376.0
96.10	3307.0
105.70	247.0
115.70	155.0
116.90	400.0
118.10	164.0
119.00	422.0
124.10	161.0
129.90	224.0
140.90	870.0
142.90	910.0
145.00	426.0
147.90	209.0
158.90	183.0
171.10	200.0
171.80	357.0
174.00	39728.0
175.00	3503.0
176.00	37968.0
177.00	3046.0
178.00	162.0
281.00	691.0
282.00	187.0
283.00	206.0

BFB82T
Client Sample :
MS/MS.D
Instrument :

m/z	Abundance
36.00	525.0
37.10	1687.0
38.20	1609.0
39.30	743.0
40.00	857.0
44.00	637.0
45.00	332.0
47.00	615.0
47.70	169.0
49.10	1873.0
50.00	7747.0
51.10	2578.0
51.90	210.0
56.20	481.0
57.00	1362.0
60.00	700.0
61.00	2624.0
62.00	2630.0
63.10	2246.0
64.10	776.0
65.00	211.0
67.00	158.0
68.00	4265.0
69.00	4603.0
70.00	702.0
72.10	299.0
73.10	1908.0
74.00	9072.0
75.00	23856.0
76.00	2195.0
76.90	259.0
77.70	189.0
79.00	2470.0
80.10	554.0
80.90	2724.0
81.80	656.0
86.20	193.0
86.90	2156.0
87.90	2418.0
88.70	246.0
90.90	241.0
92.00	1446.0
93.00	2417.0
94.10	6597.0
95.10	51848.0
96.10	3195.0
97.00	197.0
103.90	403.0
105.90	242.0
115.90	249.0
116.90	493.0
117.80	304.0
119.10	402.0
128.00	155.0
129.90	221.0
140.80	618.0
142.20	165.0
142.90	1381.0
144.90	529.0
146.10	164.0
146.90	156.0
148.00	162.0
154.80	222.0
158.90	267.0
170.70	263.0
171.10	210.0
172.00	381.0
174.00	50784.0
175.00	3636.0
176.00	49304.0
177.00	2972.0
178.00	186.0
281.00	889.0
282.10	205.0

BFB82T
Client Sample ID :
MS/MS
Instrument :

m/z	Abundance
36.00	287.0
37.10	1583.0
38.10	1641.0
39.10	846.0
40.10	644.0
44.00	661.0
44.90	342.0
46.40	211.0
47.00	527.0
47.70	261.0
48.10	289.0
49.10	1516.0
50.00	7401.0
51.10	2039.0
52.00	304.0
56.10	728.0
57.00	846.0
60.10	331.0
61.00	2077.0
62.00	2361.0
63.00	2129.0
63.90	477.0
64.90	292.0
66.90	156.0
68.00	4476.0
69.10	4080.0
70.10	257.0
71.90	506.0
73.00	2032.0
74.00	7138.0
75.10	22272.0
76.00	1644.0
76.90	344.0
78.10	204.0
78.90	2383.0
79.90	633.0
80.90	2593.0
81.90	482.0
87.00	1947.0
87.90	2208.0
90.80	257.0
91.20	170.0
91.90	1171.0
93.00	1760.0
94.00	5869.0
95.00	45264.0
96.10	2956.0
104.00	239.0
105.90	193.0
116.90	687.0
119.10	569.0
127.80	291.0
130.00	158.0
140.90	763.0
143.00	890.0
145.00	568.0
147.70	164.0
154.80	155.0
171.00	462.0
172.10	563.0
172.90	813.0
174.00	46112.0
175.00	3733.0
176.00	42880.0
176.90	2942.0
281.10	877.0
282.00	451.0
283.00	165.0

BFB82T
Client Sample ID :
MS/MS
Instrument :