




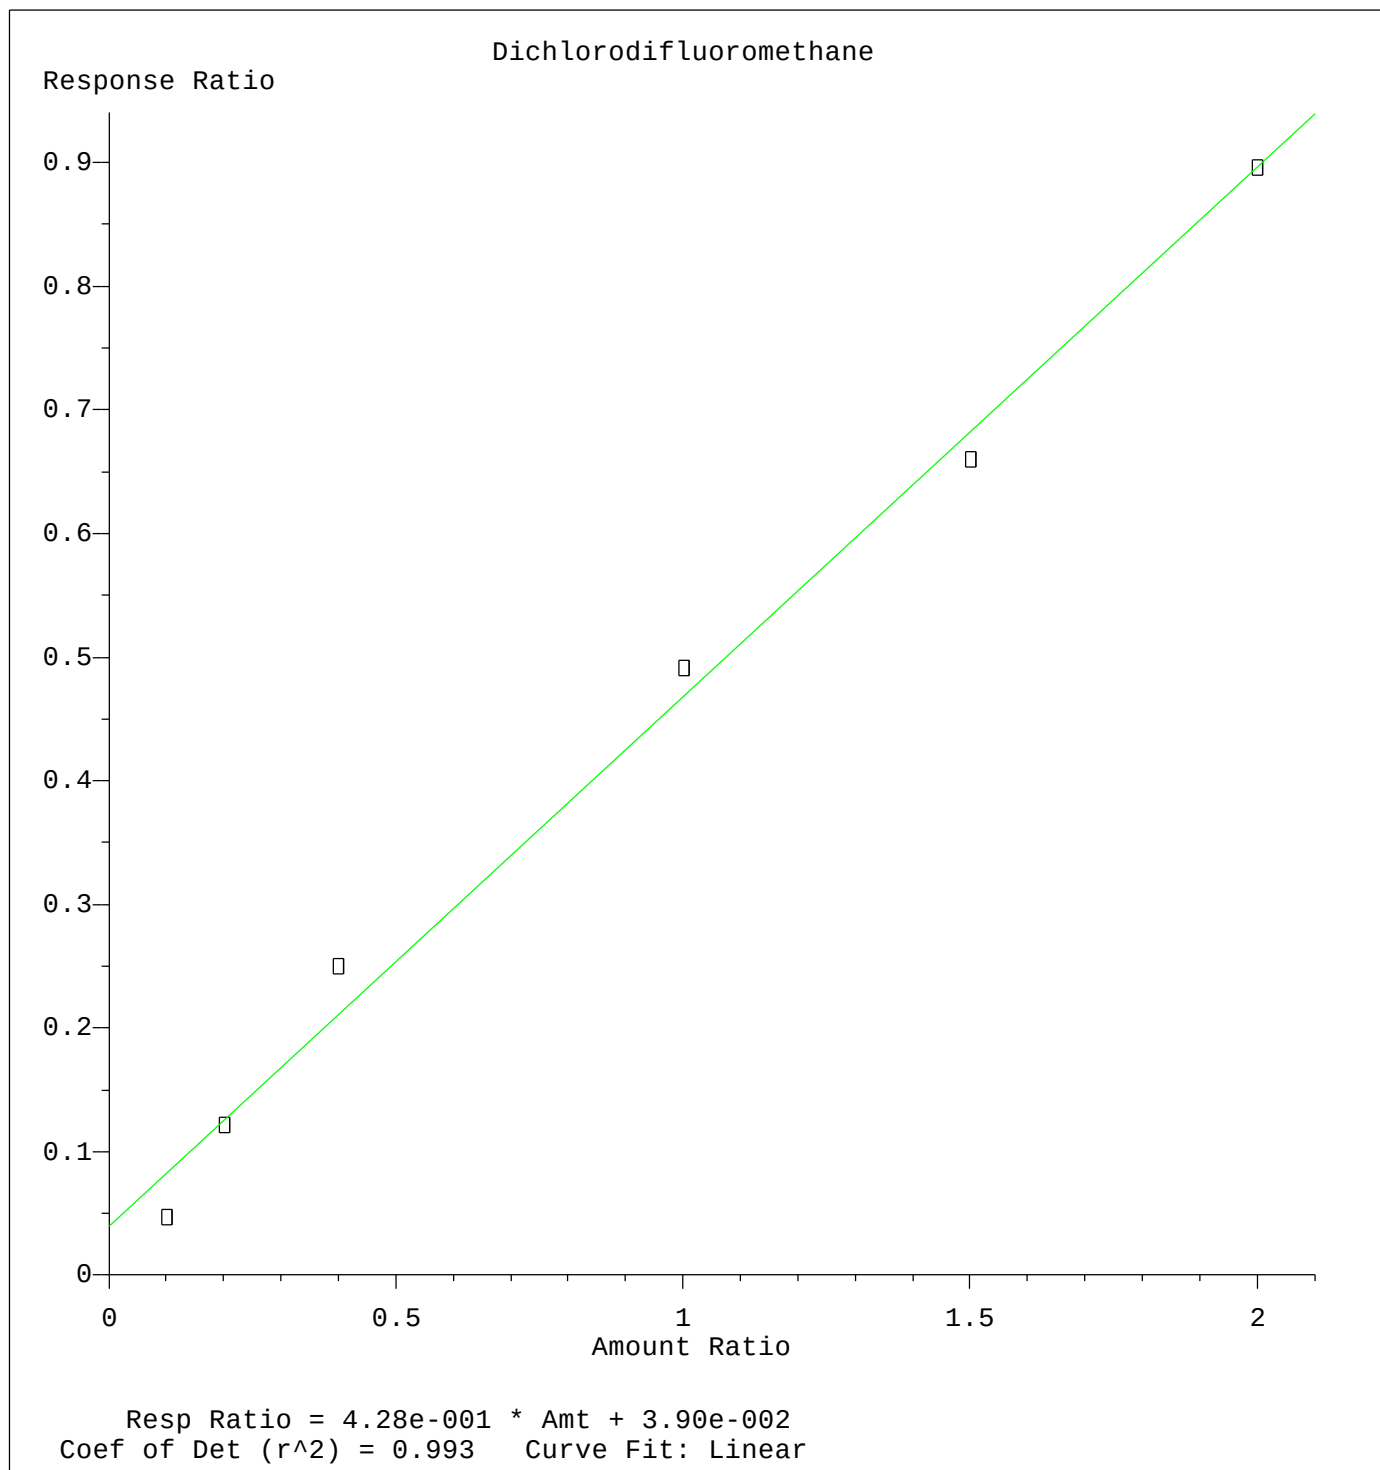


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D061918S.M
Calibration Table Last Updated: Wed Jun 20 05:52:56 2018

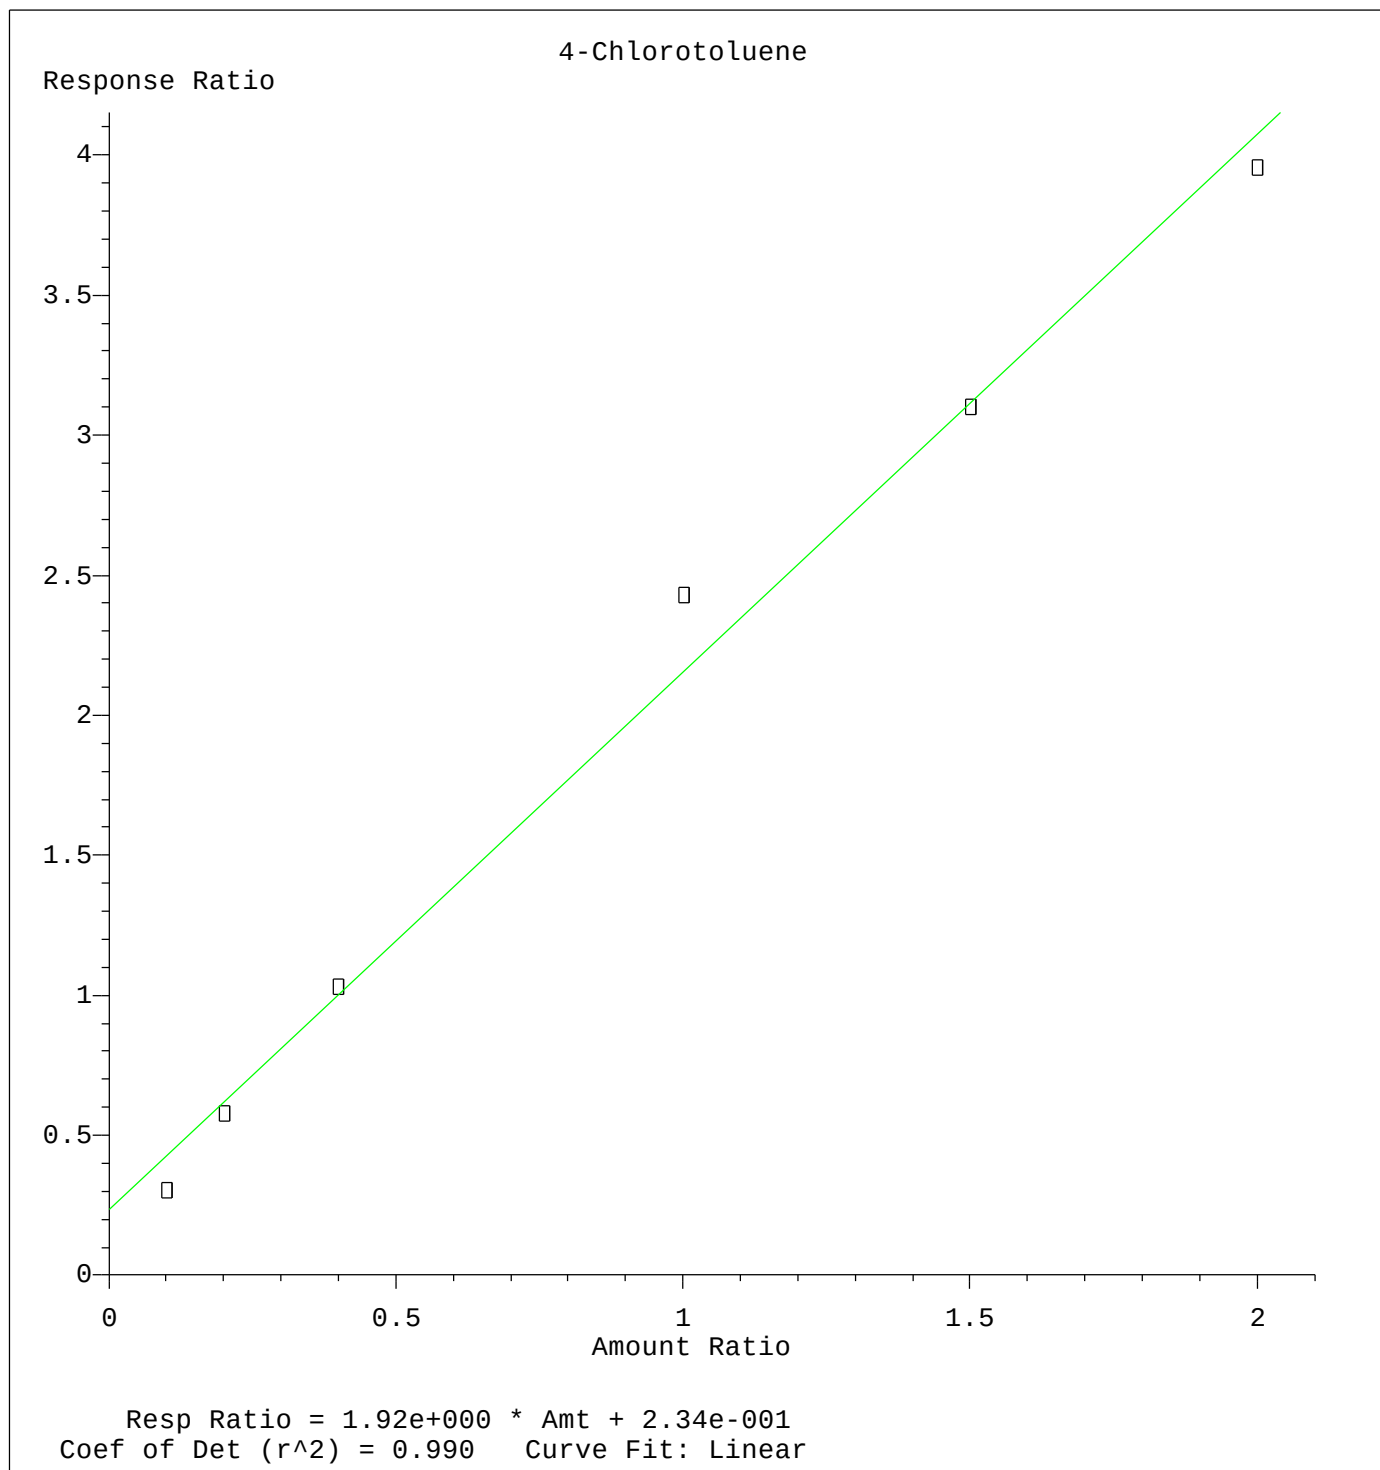


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D061918S.M
Calibration Table Last Updated: Wed Jun 20 05:52:56 2018

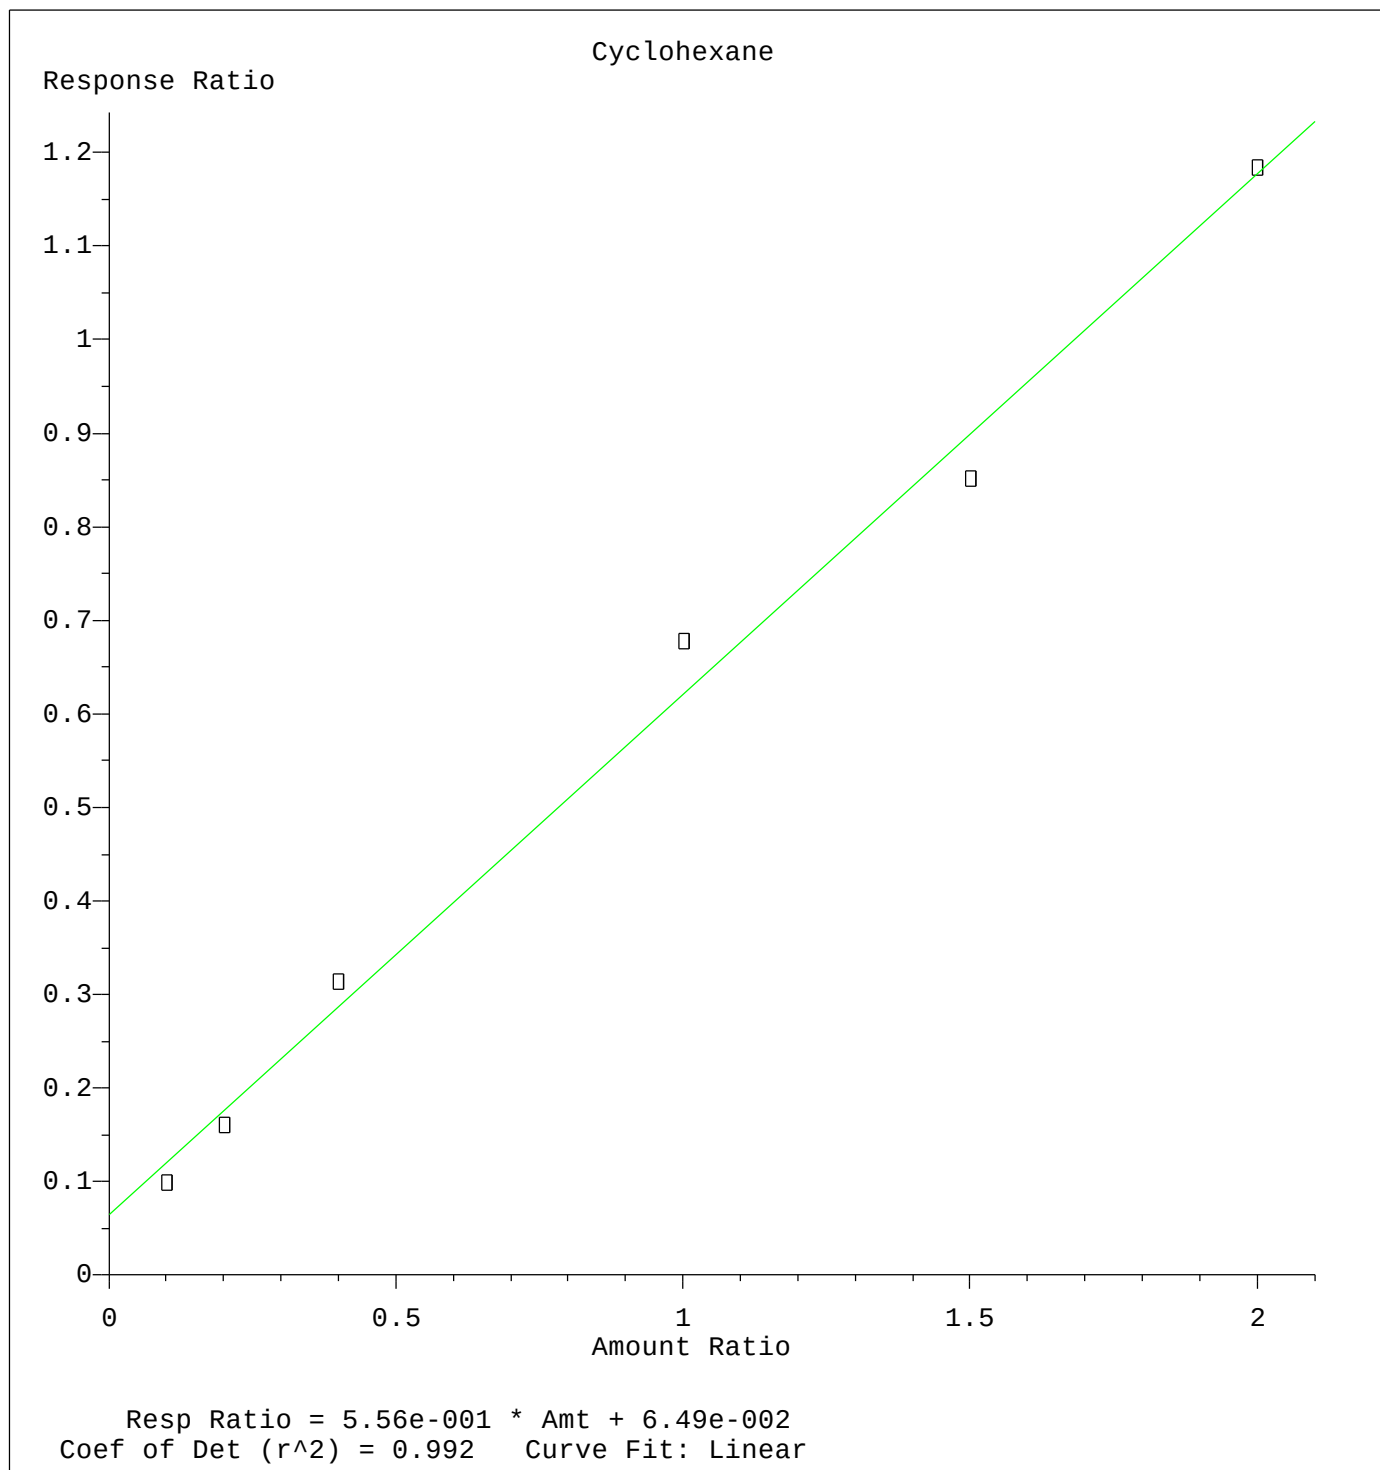


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D061918S.M
Calibration Table Last Updated: Wed Jun 20 05:52:56 2018

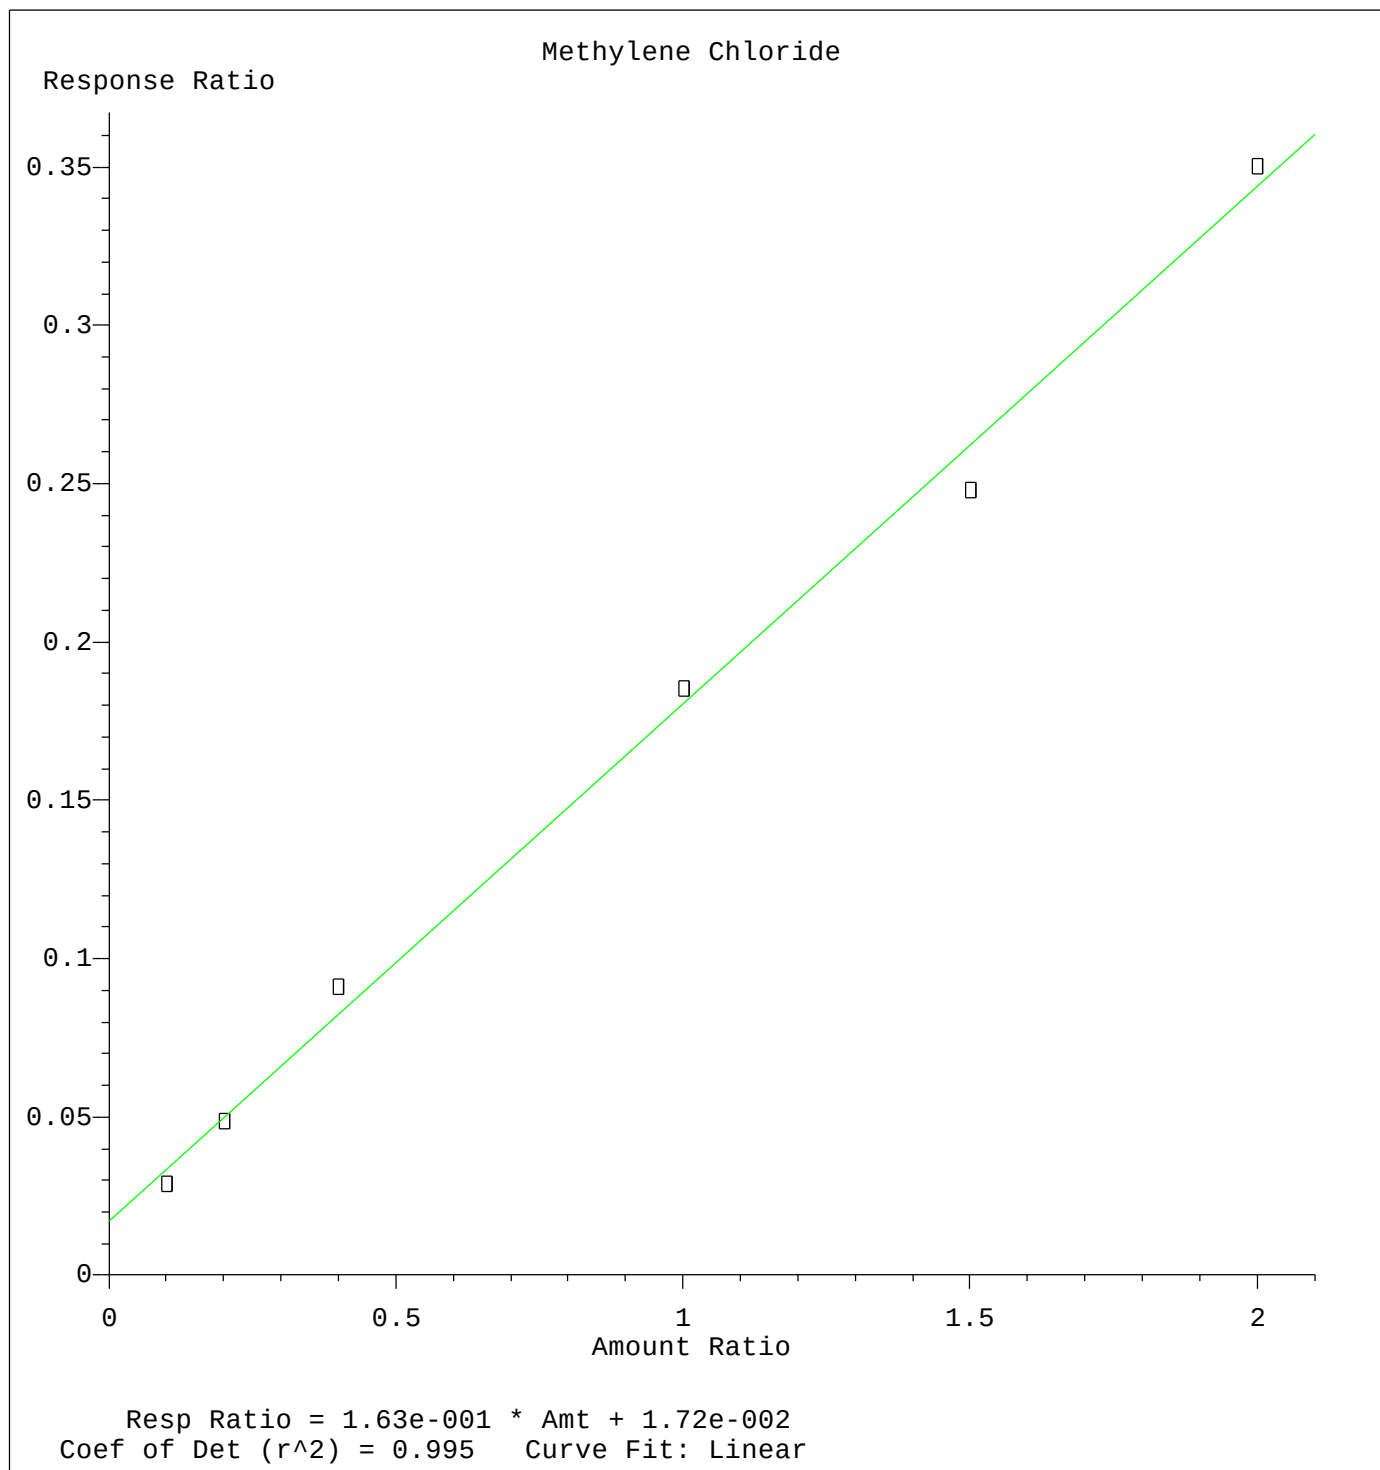


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D061918S.M
Calibration Table Last Updated: Wed Jun 20 05:52:56 2018

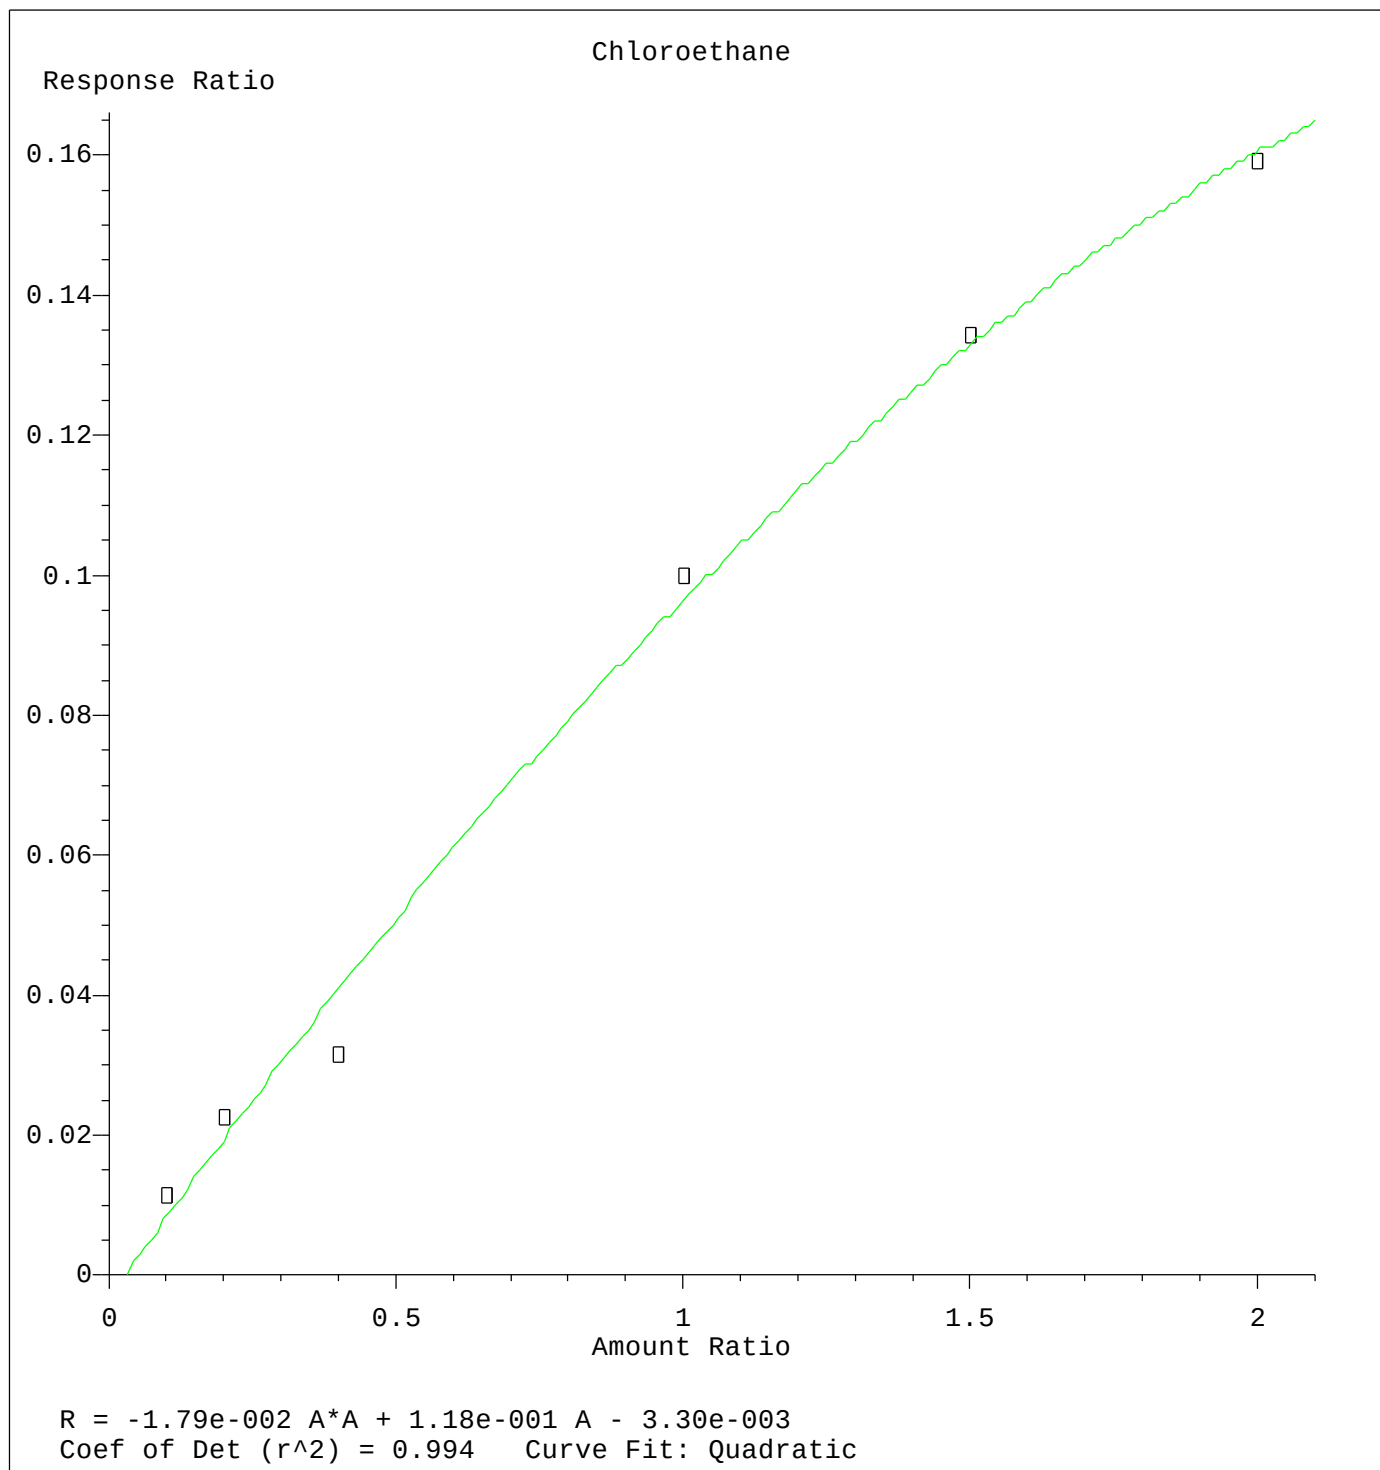

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D061918S.M
Calibration Table Last Updated: Wed Jun 20 05:52:56 2018

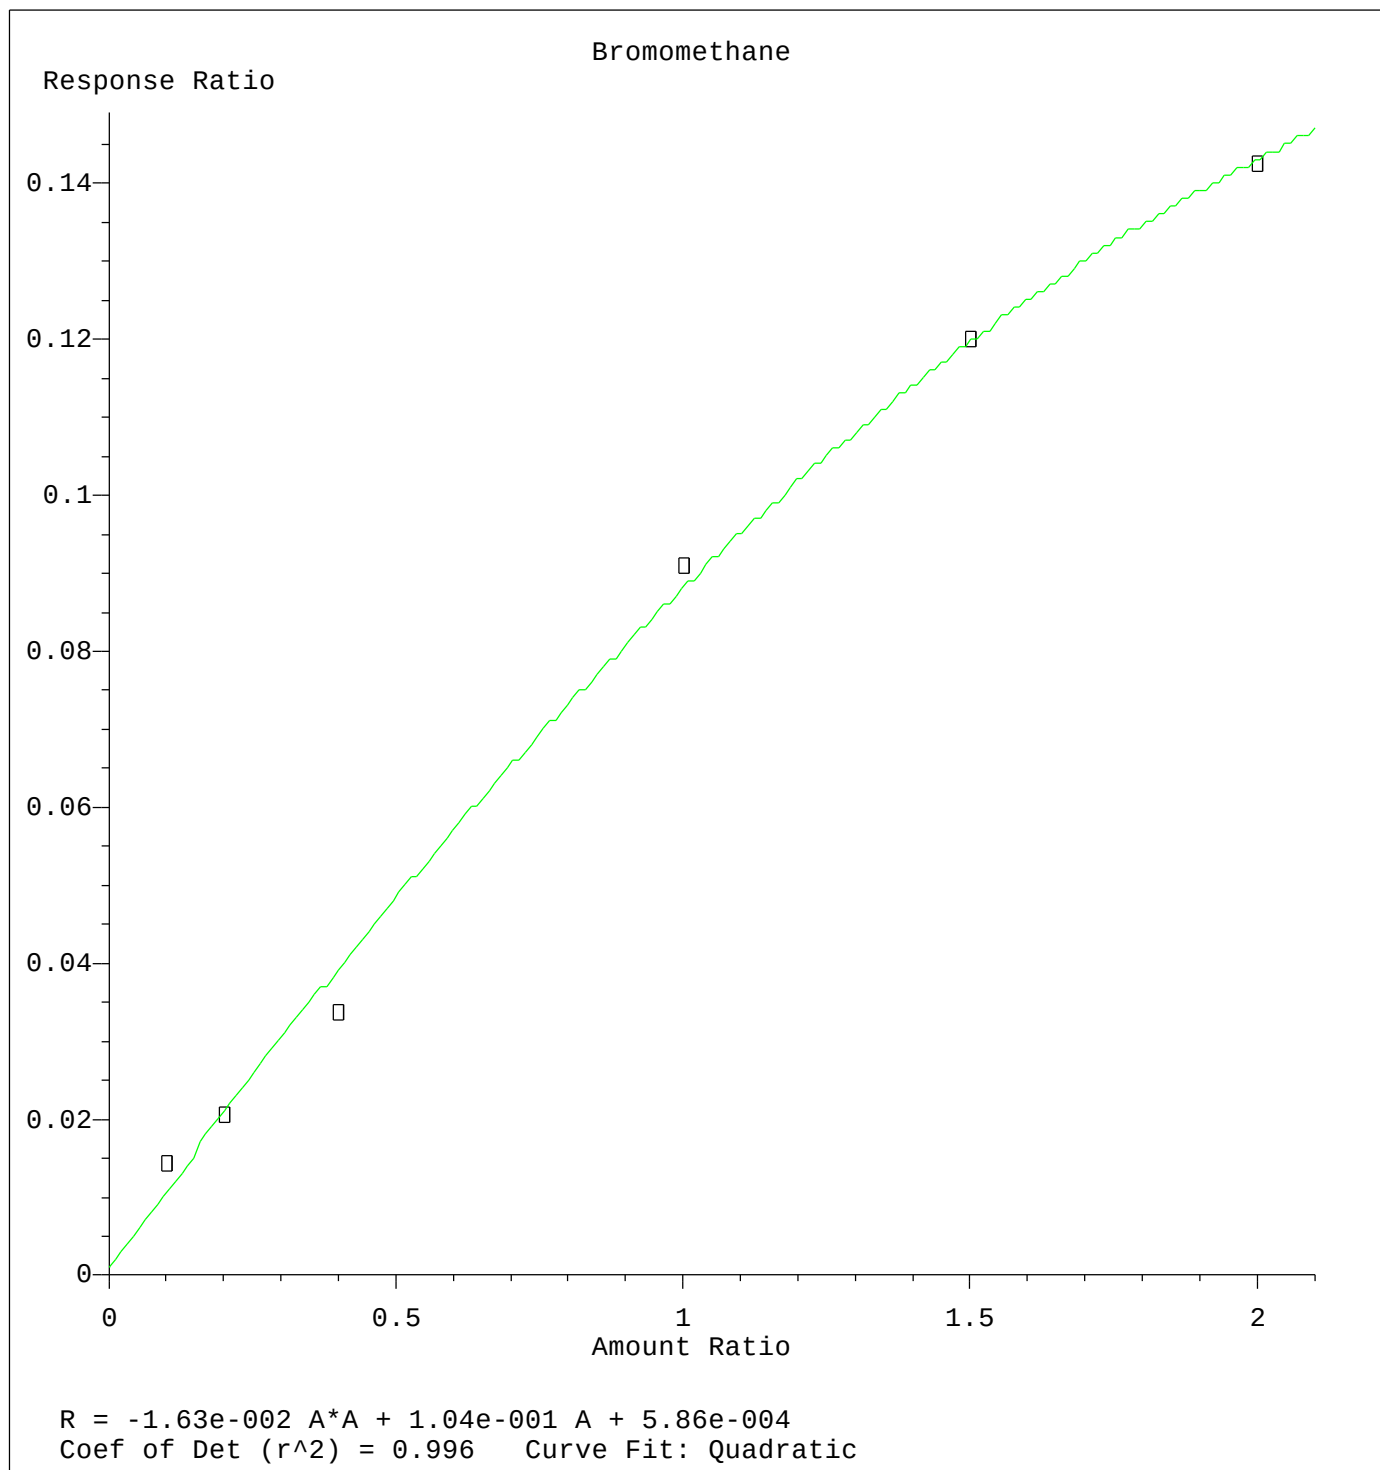

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D061918S.M
Calibration Table Last Updated: Wed Jun 20 05:52:56 2018

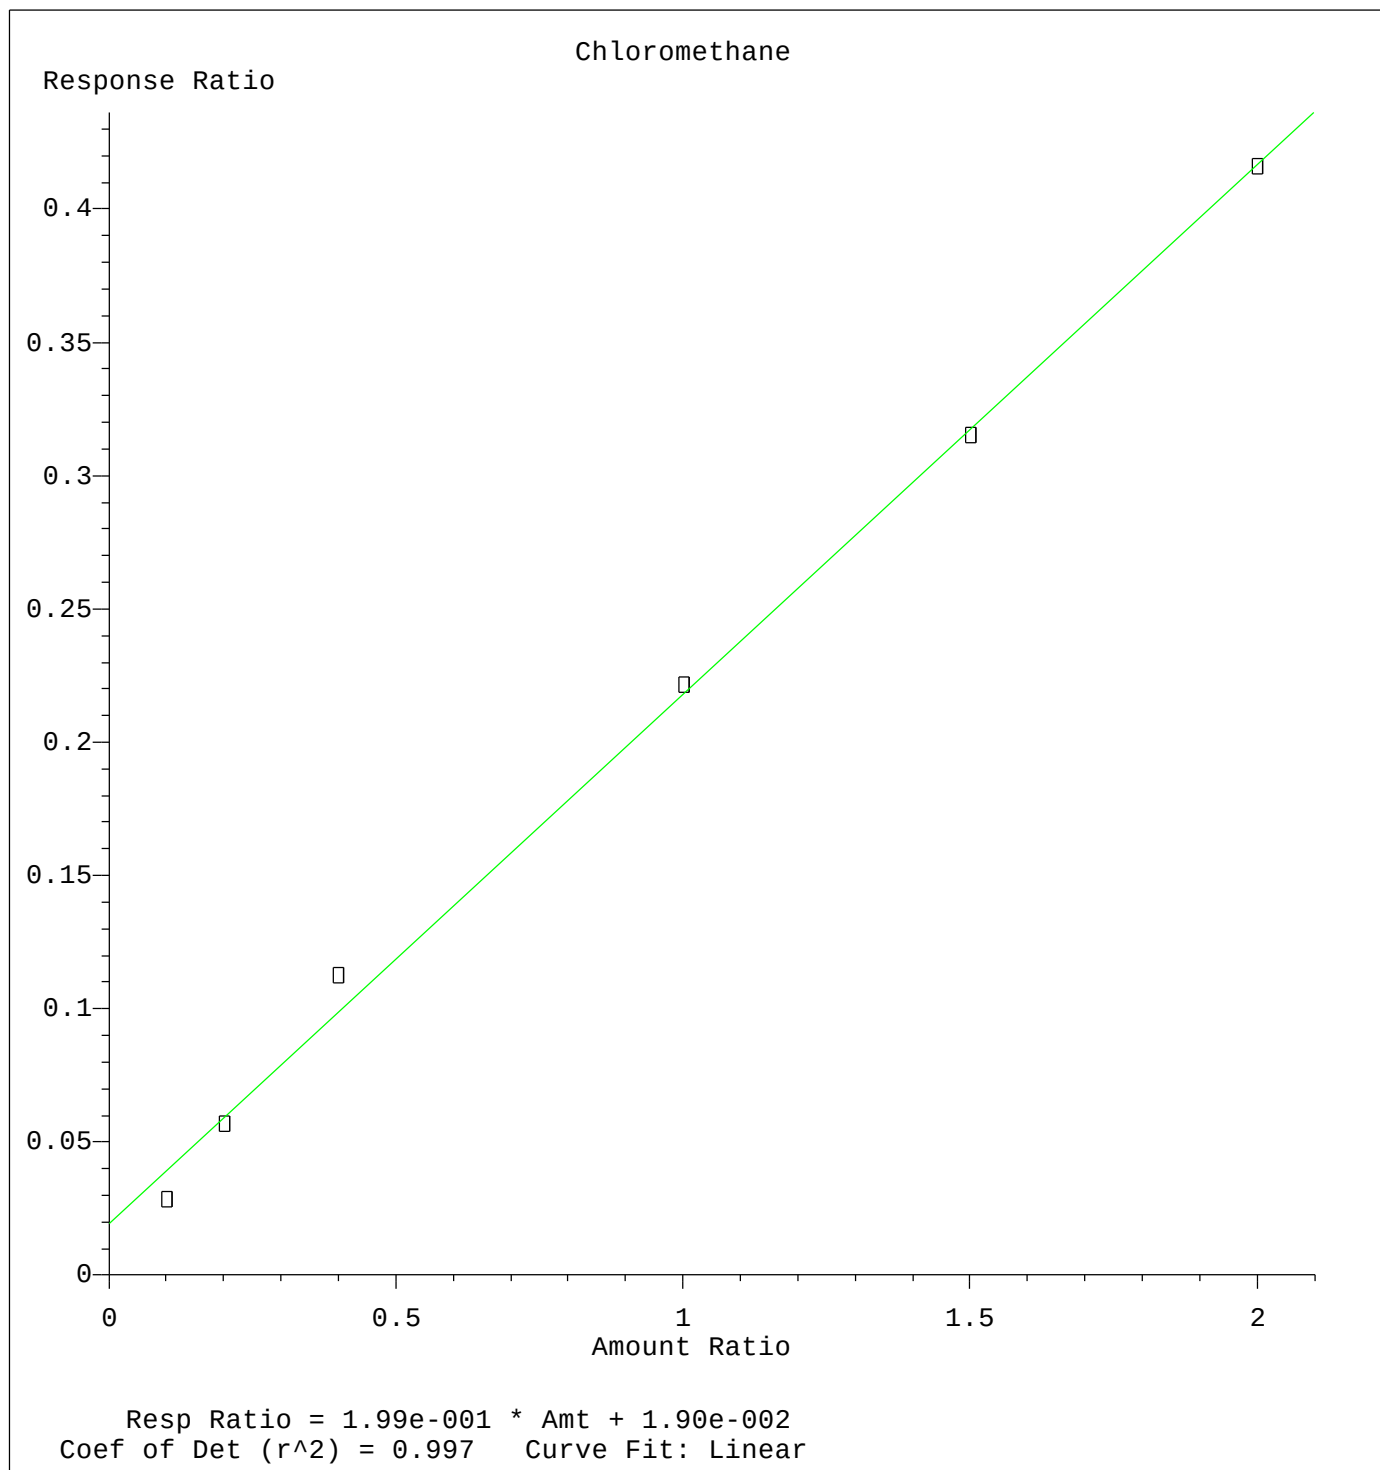

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D061918S.M
Calibration Table Last Updated: Wed Jun 20 05:52:56 2018