


Data Path : Z:\VOASRV\HPCHEM1\MSVOA D\DATA\VD061918\
Data File : VD058193.D
Acq On : 19 Jun 2018 12:36
Operator : VA/AP
Sample : BFB
Misc : 5.00g/5ml/MSVOA D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_D\METHOD\82D061918S.M
Title : SW846 8260
Last Update : Wed Jun 20 05:52:56 2018

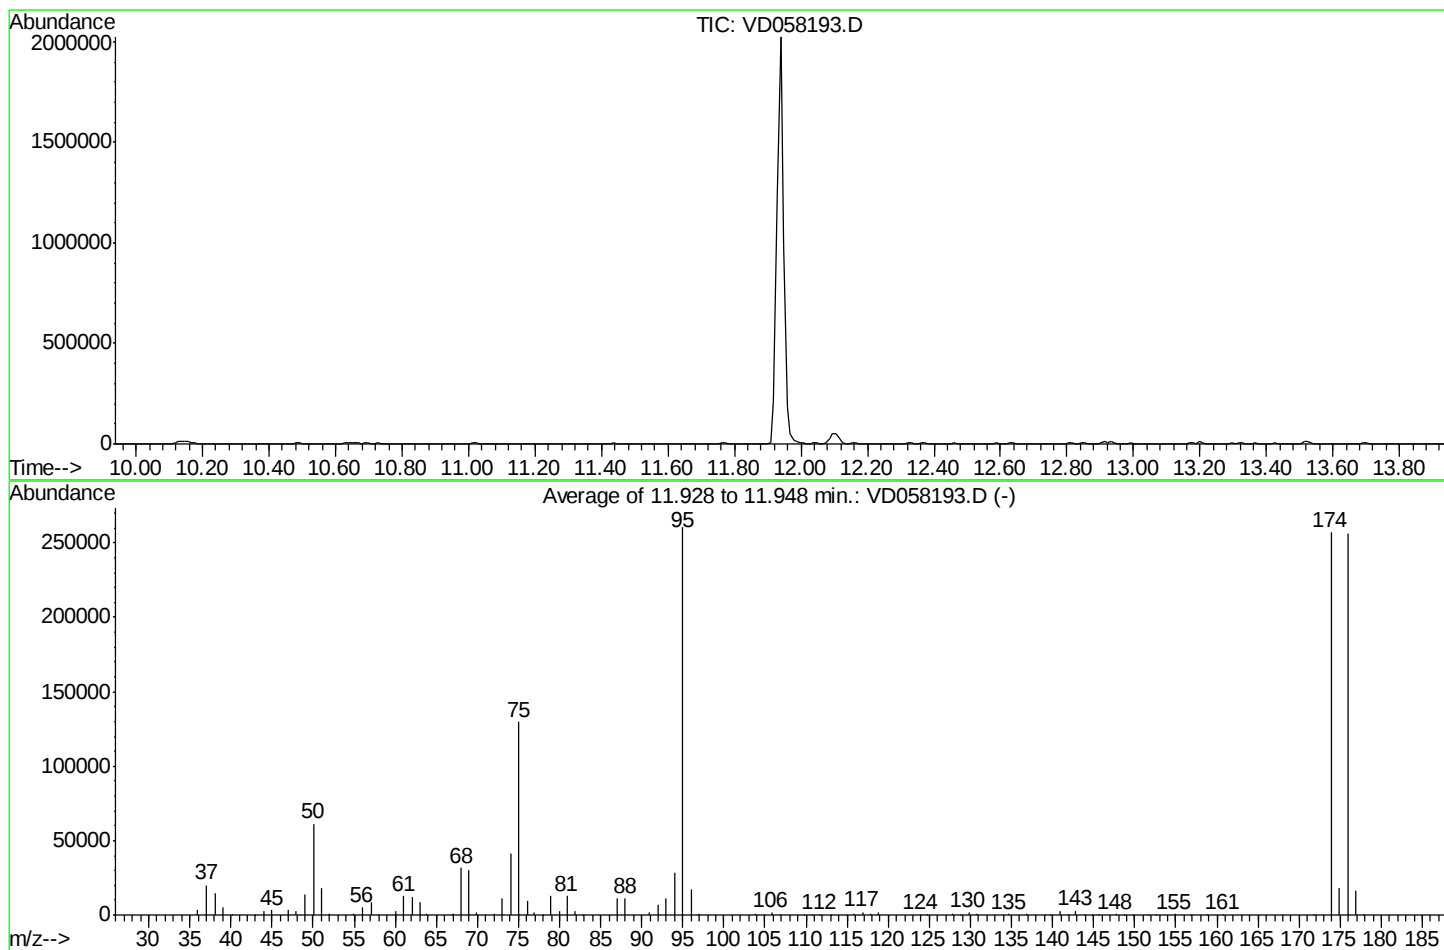

AutoFind: Scans 1189, 1190, 1191; Background Corrected with Scan 1184

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	23.6	61400	PASS
75	95	30	60	49.7	129573	PASS
95	95	100	100	100.0	260480	PASS
96	95	5	9	6.5	16919	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	98.8	257408	PASS
175	174	5	9	7.2	18428	PASS
176	174	95	101	99.7	256597	PASS
177	176	5	9	6.3	16055	PASS