

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061923\
 Data File : VD076477.D
 Acq On : 19 Jun 2023 18:45
 Operator : KP/SY
 Sample : 03289-08
 Misc : 5.07G/5.0ml/MSVOA_D/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 SB-03-4.0-6.0

Quant Time: Jun 20 05:28:06 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061623S.M
 Quant Title : SW846 8260
 QLast Update : Mon Jun 19 04:51:45 2023
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	7.881	168	5437	50.000	ug/l	# 0.00
34) 1,4-Difluorobenzene	8.775	114	9147	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.581	117	9445	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.516	152	4391	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.222	65	4991	91.622	ug/l	0.00
Spiked Amount	50.000	Range	50 - 163	Recovery	= 183.240%#	
35) Dibromofluoromethane	7.810	113	4233	77.899	ug/l	0.00
Spiked Amount	50.000	Range	54 - 147	Recovery	= 155.800%#	
50) Toluene-d8	10.269	98	12156	58.987	ug/l	0.00
Spiked Amount	50.000	Range	58 - 134	Recovery	= 117.980%	
62) 4-Bromofluorobenzene	12.575	95	3950	59.059	ug/l	0.00
Spiked Amount	50.000	Range	30 - 143	Recovery	= 118.120%	
Target Compounds						
						Qvalue
2) Dichlorodifluoromethane	2.164	85	60	1.452	ug/l	# 43
3) Chloromethane	2.152	50	279	3.247	ug/l	# 41
5) Bromomethane	2.699	94	434	6.964	ug/l	# 49
6) Chloroethane	2.934	64	86	1.309	ug/l	# 43
10) Methyl Iodide	4.158	142	91	1.511	ug/l	# 46
11) Tert butyl alcohol	5.040	59	119	25.301	ug/l	# 73
13) Acrolein	3.910	56	59	11.646	ug/l	# 43
14) Allyl chloride	4.505	41	182	2.000	ug/l	# 42
15) Acrylonitrile	5.299	53	54	3.538	ug/l	# 18
16) Acetone	4.040	43	441	34.021	ug/l	# 32
18) Methyl Acetate	4.540	43	124	2.076	ug/l	# 42
20) Methylene Chloride	4.793	84	385	Below Cal	#	36
21) trans-1,2-Dichloroethene	5.122	96	69	1.200	ug/l	# 4
25) 2-Butanone	7.093	43	239	11.921	ug/l	# 37
27) cis-1,2-Dichloroethene	7.304	96	71	1.020	ug/l	# 1
28) Bromochloromethane	7.446	49	56	Below Cal	#	1
29) Tetrahydrofuran	7.475	42	180	13.970	ug/l	# 23
36) 1,1-Dichloropropene	7.893	75	78	1.025	ug/l	# 39
37) Ethyl Acetate	7.199	43	64	1.451	ug/l	# 62
38) Carbon Tetrachloride	7.887	117	166	2.441	ug/l	# 11
41) Methacrylonitrile	7.434	41	55	2.209	ug/l	# 17
43) Isopropyl Acetate	8.351	43	127	1.521	ug/l	# 43
48) Methyl methacrylate	9.381	41	137	3.581	ug/l	# 1
51) 4-Methyl-2-Pentanone	10.092	43	95	2.226	ug/l	# 28
59) 2-Hexanone	10.934	43	225	7.580	ug/l	# 16
76) 1,2,3-Trichloropropane	12.575	75	2256	51.767	ug/l	# 100
81) trans-1,4-Dichloro-2-b...	12.575	75	2256	113.434	ug/l	# 17
90) Hexachloroethane	13.933	117	57	1.161	ug/l	# 11
92) 1,2-Dibromo-3-Chloropr...	14.681	75	111	12.088	ug/l	# 1
94) Hexachlorobutadiene	15.457	225	54	1.331	ug/l	# 19
95) Naphthalene	15.333	128	447	2.679	ug/l	# 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061923\
Data File : VD076477.D
Acq On : 19 Jun 2023 18:45
Operator : KP/SY
Sample : 03289-08
Misc : 5.07G/5.0ml/MSVOA_D/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
SB-03-4.0-6.0

Quant Time: Jun 20 05:28:06 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D061623S.M
Quant Title : SW846 8260
QLast Update : Mon Jun 19 04:51:45 2023
Response via : Initial Calibration

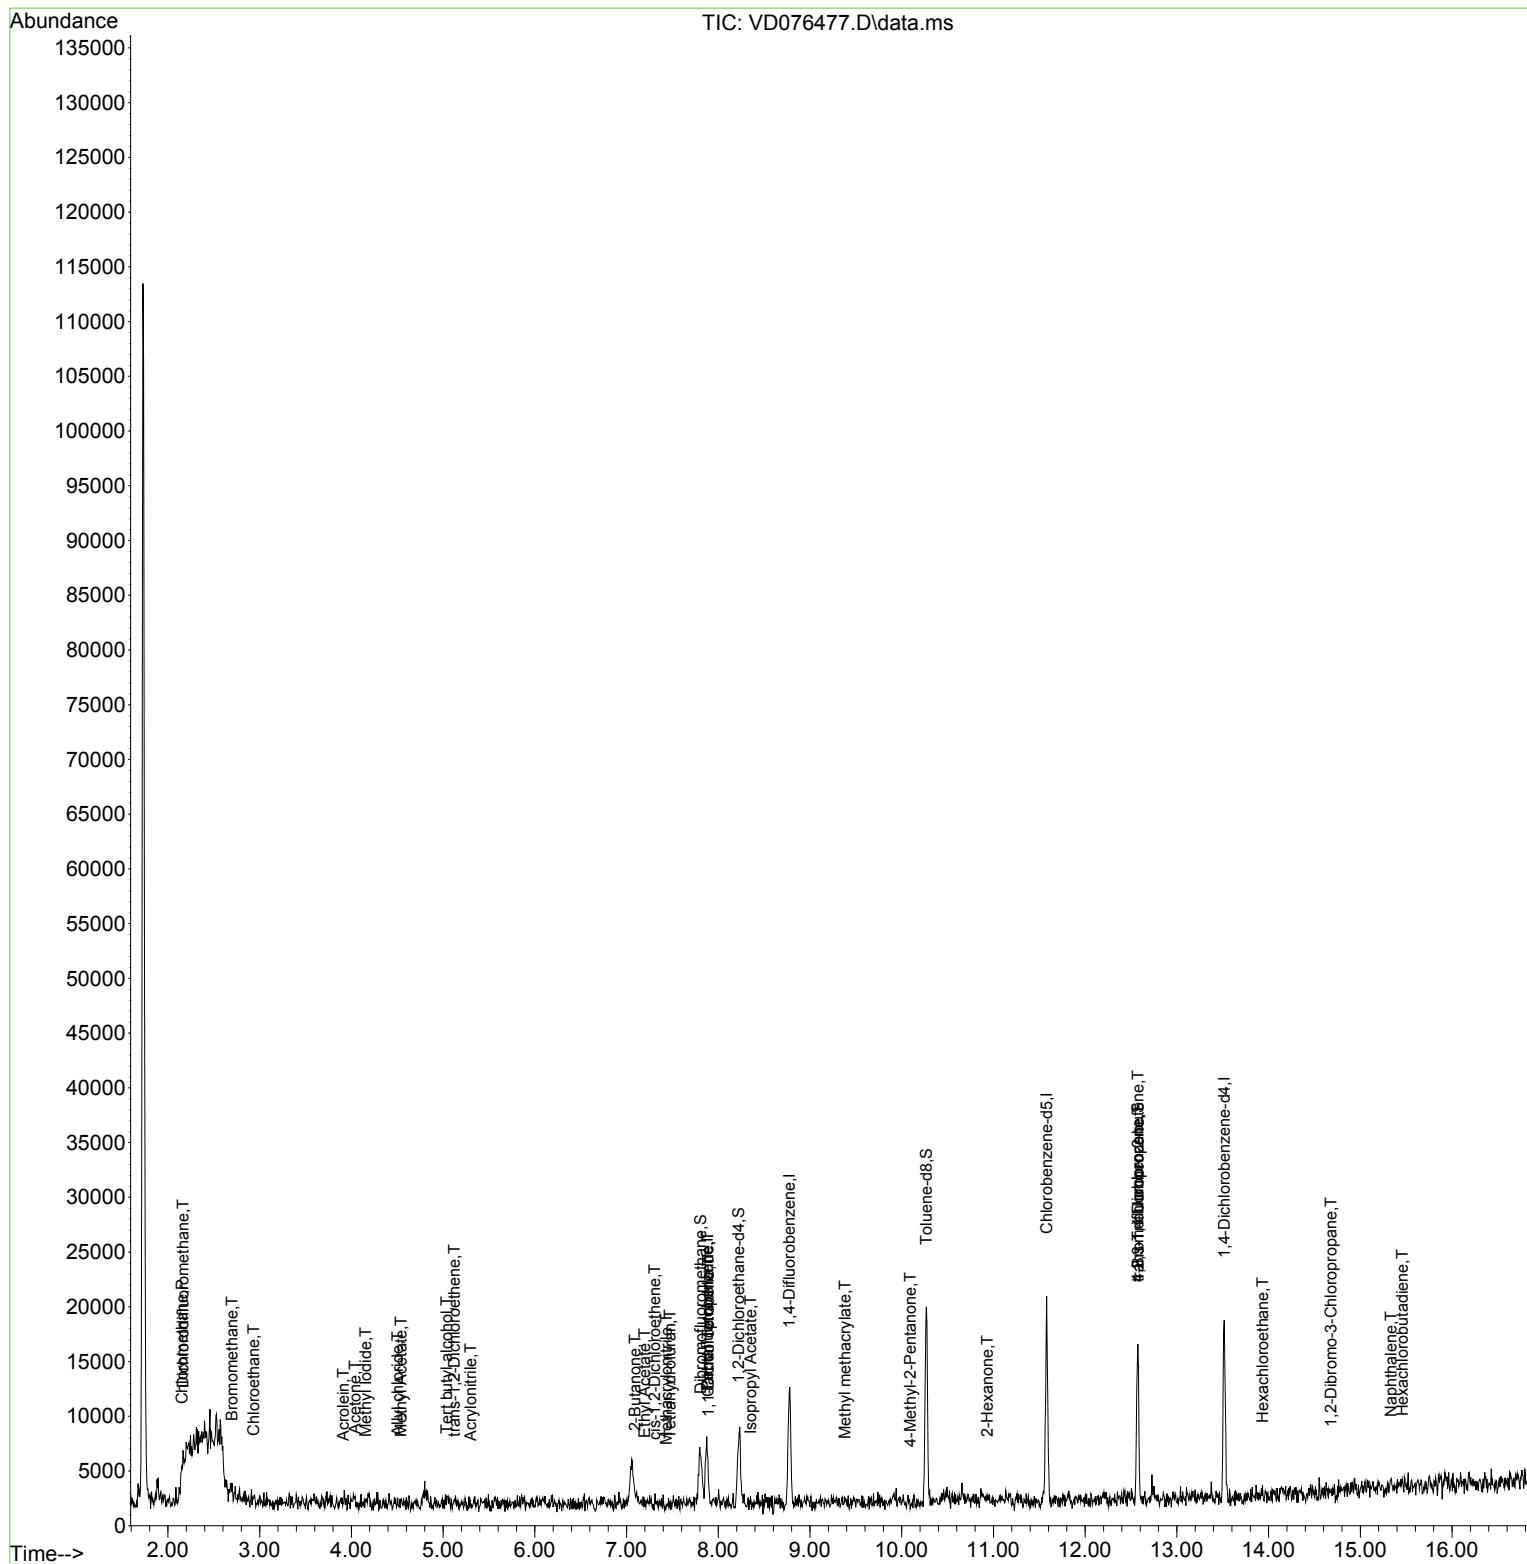



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.881 min Scan# 10

Delta R.T. 0.006 min

Lab File: VD076477.D

Acq: 19 Jun 2023 18:45

Instrument :

MSVOA_D

ClientSampleId :





SB-03-4.0-6.0

Tgt Ion:168 Resp: 5437

Ion Ratio Lower Upper

168 100

99 25.0 36.7 55.1#



#2

Dichlorodifluoromethane

Concen: 1.452 ug/l

RT: 2.164 min Scan# 98

Delta R.T. 0.235 min

Lab File: VD076477.D




Acq: 19 Jun 2023 18:45


Tgt Ion: 85 Resp: 60

Ion Ratio Lower Upper

85 100

87 0.0 15.7 47.0#




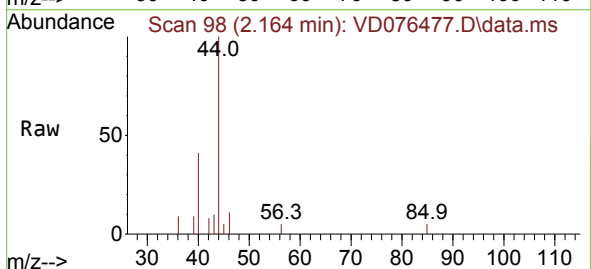


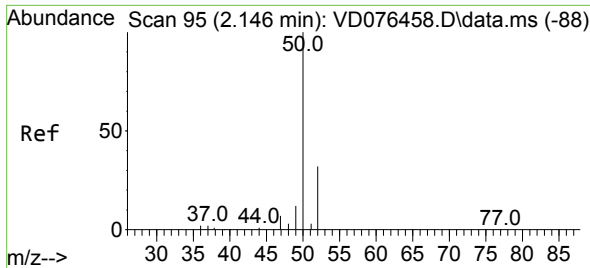

#3
Chloromethane
Concen: 3.247 ug/l
RT: 2.152 min Scan# 90
Delta R.T. 0.006 min
Lab File: VD076477.D
Acq: 19 Jun 2023 18:45




Instrument :
MSVOA_D
ClientSampleId :
SB-03-4.0-6.0


Tgt Ion: 50 Resp: 279
Ion Ratio Lower Upper
50 100
52 0.0 26.6 40.0#

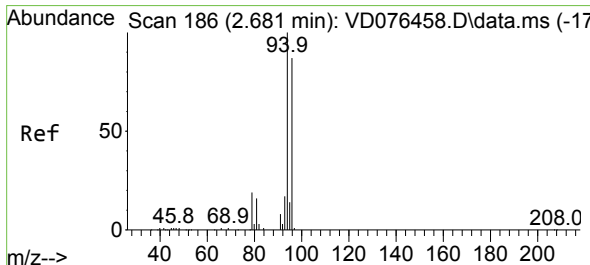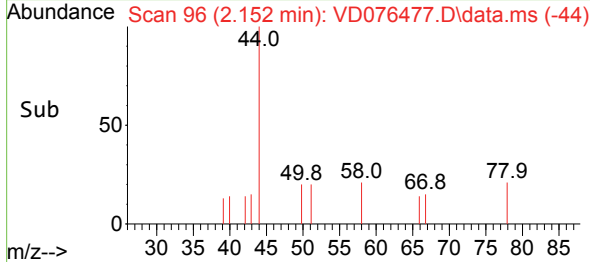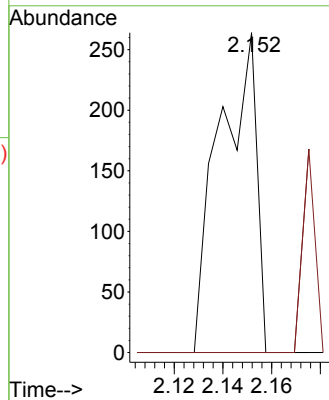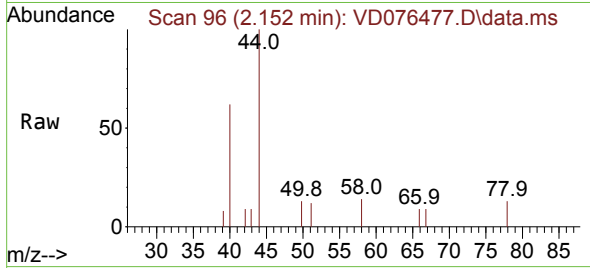

#5
Bromomethane
Concen: 6.964 ug/l
RT: 2.699 min Scan# 189
Delta R.T. 0.017 min
Lab File: VD076477.D
Acq: 19 Jun 2023 18:45

Tgt Ion: 94 Resp: 434
Ion Ratio Lower Upper
94 100
96 144.2 75.8 113.8#


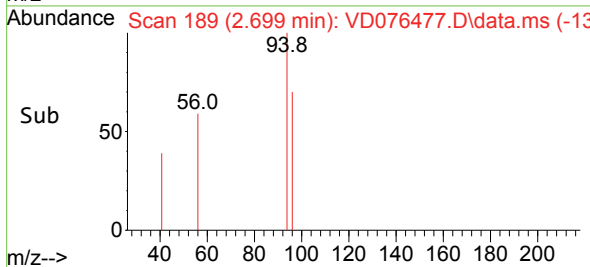
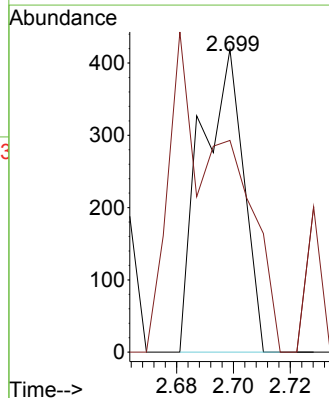
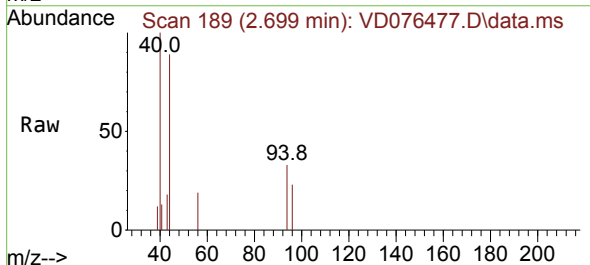




#6
Chloroethane
Concen: 1.309 ug/l
RT: 2.934 min Scan# 211
Delta R.T. 0.106 min
Lab File: VD076477.D
Acq: 19 Jun 2023 18:45




Instrument :
MSVOA_D
ClientSampleId :
SB-03-4.0-6.0


Tgt Ion: 64 Resp: 86
Ion Ratio Lower Upper
64 100
66 0.0 25.5 38.3#

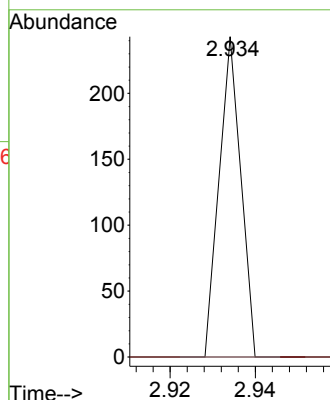

#10
Methyl Iodide
Concen: 1.511 ug/l
RT: 4.158 min Scan# 437
Delta R.T. -0.000 min
Lab File: VD076477.D
Acq: 19 Jun 2023 18:45

Tgt Ion: 142 Resp: 91
Ion Ratio Lower Upper
142 100
127 0.0 29.4 44.0#
141 0.0 11.1 16.7#

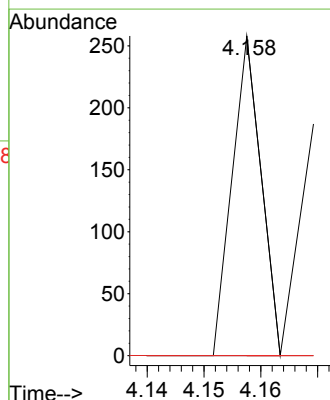



#11

Tert butyl alcohol

Concen: 25.301 ug/l

RT: 5.040 min Scan# 51

Delta R.T. -0.018 min

Lab File: VD076477.D

Acq: 19 Jun 2023 18:45

Instrument :

MSVOA_D

ClientSampleId :





SB-03-4.0-6.0

Tgt Ion: 59 Resp: 119

Ion Ratio Lower Upper

59 100

57 0.0 7.8 11.8#

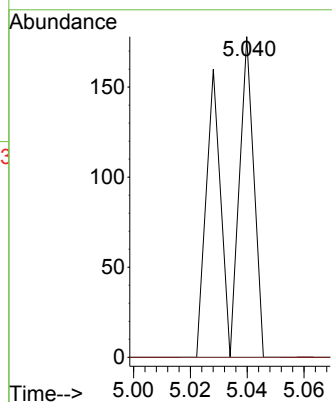

#13

Acrolein

Concen: 11.646 ug/l

RT: 3.910 min Scan# 395

Delta R.T. 0.117 min

Lab File: VD076477.D




Acq: 19 Jun 2023 18:45


Tgt Ion: 56 Resp: 59

Ion Ratio Lower Upper

56 100

55 115.3 55.1 82.7#



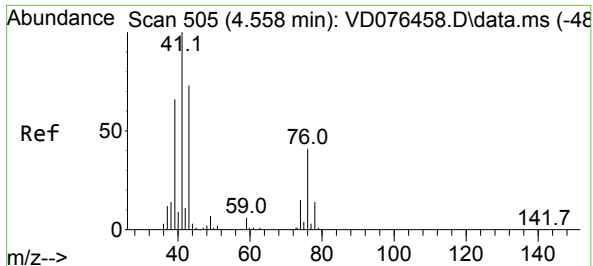

#14

Allyl chloride

Concen: 2.000 ug/l

RT: 4.505 min Scan# 496

Delta R.T. -0.053 min

Lab File: VD076477.D

Acq: 19 Jun 2023 18:45





Instrument :

MSVOA_D

ClientSampleId :

SB-03-4.0-6.0

Tgt Ion:	41	Resp:	182
Ion	Ratio	Lower	Upper
41	100		
39	34.1	53.8	80.6#
76	0.0	45.8	68.8#

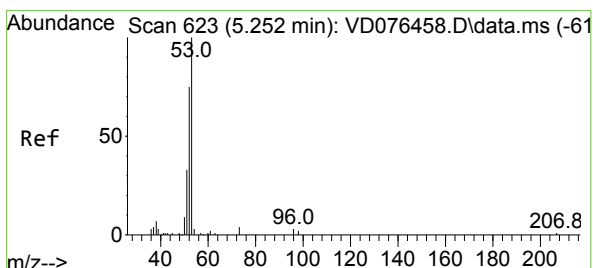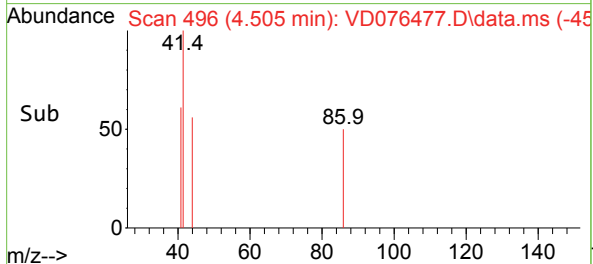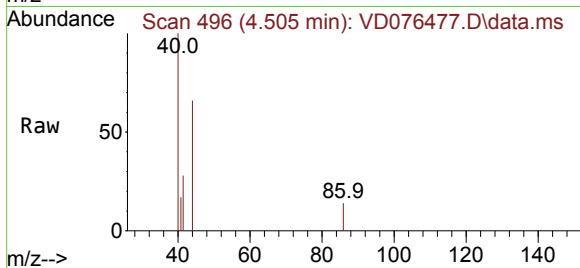

#15

Acrylonitrile

Concen: 3.538 ug/l




RT: 5.299 min Scan# 631


Delta R.T. 0.047 min

Lab File: VD076477.D

Acq: 19 Jun 2023 18:45

Tgt Ion:	53	Resp:	54
Ion	Ratio	Lower	Upper
53	100		
52	0.0	65.0	97.4#
51	0.0	28.3	42.5#


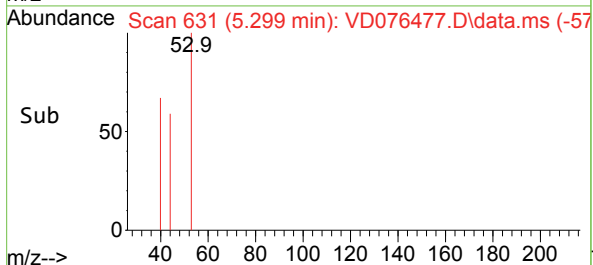

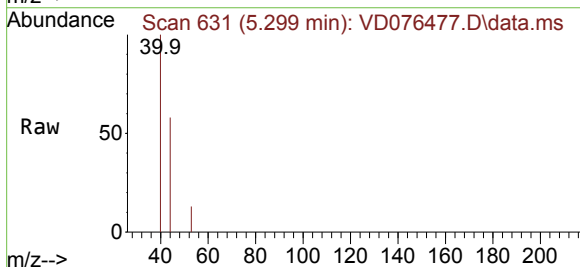




#16
Acetone
Concen: 34.021 ug/l
RT: 4.040 min Scan# 41
Delta R.T. 0.023 min
Lab File: VD076477.D
Acq: 19 Jun 2023 18:45




Instrument :
MSVOA_D
ClientSampleId :
SB-03-4.0-6.0


Tgt Ion: 43 Resp: 441
Ion Ratio Lower Upper
43 100
58 0.0 34.7 52.1#

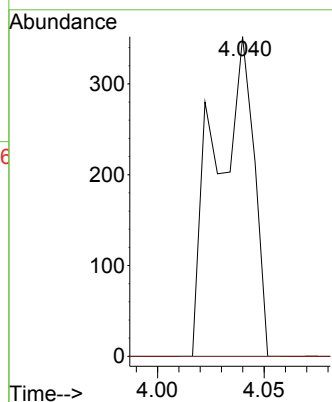

#18
Methyl Acetate
Concen: 2.076 ug/l
RT: 4.540 min Scan# 502
Delta R.T. -0.018 min
Lab File: VD076477.D
Acq: 19 Jun 2023 18:45

Tgt Ion: 43 Resp: 124
Ion Ratio Lower Upper
43 100
74 0.0 26.4 39.6#



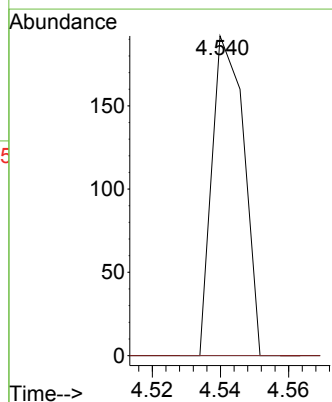





#20
Methylene Chloride
Concen: Below Cal
RT: 4.793 min Scan# 54
Delta R.T. -0.006 min
Lab File: VD076477.D
Acq: 19 Jun 2023 18:45




Instrument :
MSVOA_D
ClientSampleId :
SB-03-4.0-6.0


Tgt Ion:	84	Resp:	385
Ion	Ratio	Lower	Upper
84	100		
49	0.0	71.4	107.2#
51	0.0	24.5	36.7#
86	78.0	48.7	73.1#

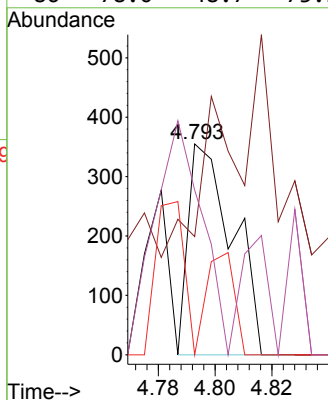

#21
trans-1,2-Dichloroethene
Concen: 1.200 ug/l
RT: 5.122 min Scan# 601
Delta R.T. -0.188 min
Lab File: VD076477.D
Acq: 19 Jun 2023 18:45

Tgt Ion:	96	Resp:	69
Ion	Ratio	Lower	Upper
96	100		
61	0.0	89.3	133.9#
98	0.0	48.6	73.0#


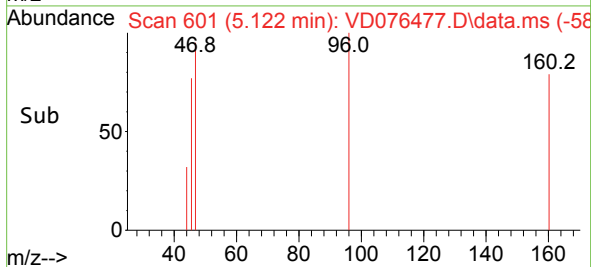
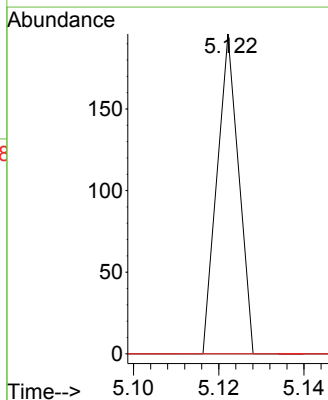
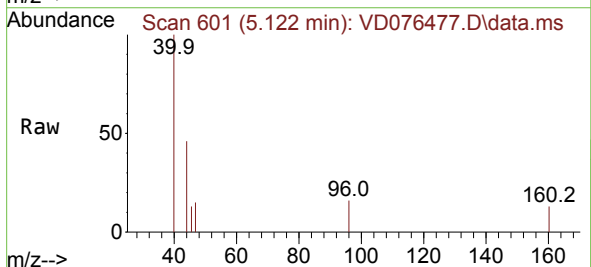




#25
2-Butanone
Concen: 11.921 ug/l
RT: 7.093 min Scan# 911
Delta R.T. 0.012 min
Lab File: VD076477.D
Acq: 19 Jun 2023 18:45




Instrument :
MSVOA_D
ClientSampleId :
SB-03-4.0-6.0


Tgt Ion: 43 Resp: 239
Ion Ratio Lower Upper
43 100
72 0.0 30.7 46.1#

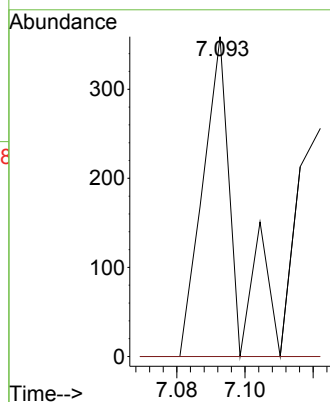

#27
cis-1,2-Dichloroethene
Concen: 1.020 ug/l
RT: 7.304 min Scan# 972
Delta R.T. 0.223 min
Lab File: VD076477.D
Acq: 19 Jun 2023 18:45

Tgt Ion: 96 Resp: 71
Ion Ratio Lower Upper
96 100
61 0.0 0.0 239.2
98 0.0 0.0 128.6

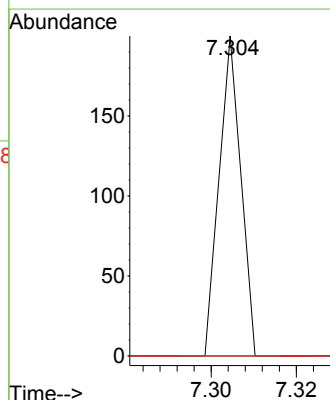

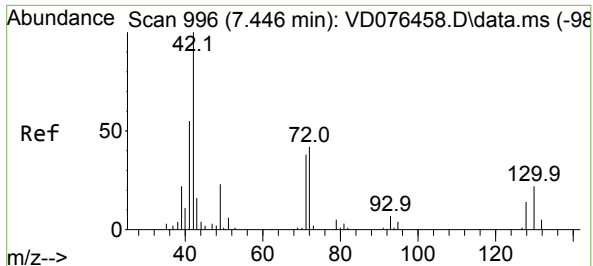

#29

Tetrahydrofuran

Concen: 13.970 ug/l

RT: 7.475 min Scan# 1001

Delta R.T. 0.029 min

Lab File: VD076477.D

Acq: 19 Jun 2023 18:45

Instrument :

MSVOA_D

ClientSampleId :

SB-03-4.0-6.0





Tgt Ion: 42 Resp: 180

Ion Ratio Lower Upper

42 100

72 0.0 46.5 69.7#

71 0.0 44.5 66.7#

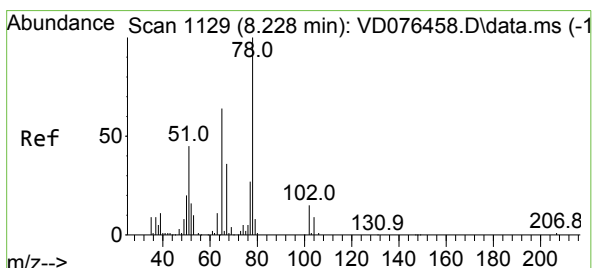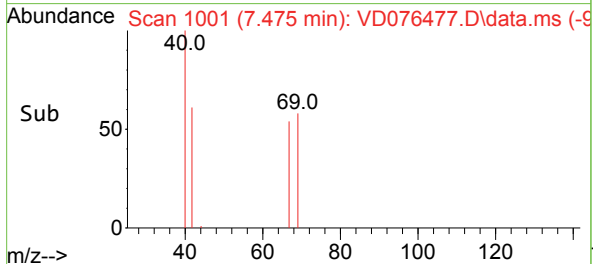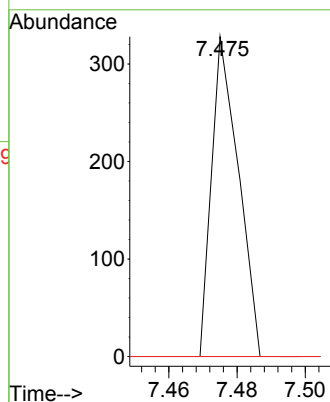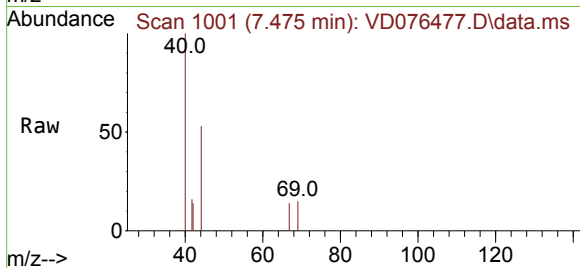

#33

1,2-Dichloroethane-d4

Concen: 91.622 ug/l

RT: 8.222 min Scan# 1128

Delta R.T. -0.006 min

Lab File: VD076477.D




Acq: 19 Jun 2023 18:45


Tgt Ion: 65 Resp: 4991

Ion Ratio Lower Upper

65 100

67 66.4 0.0 115.0

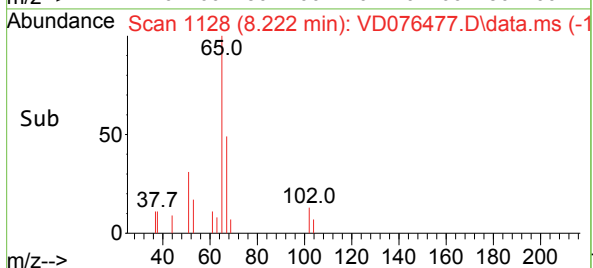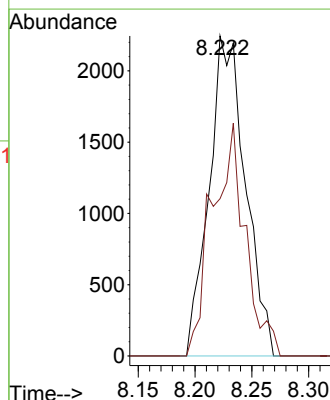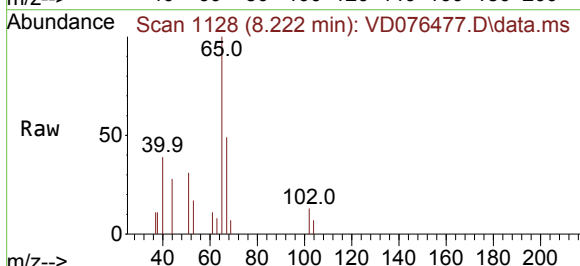



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.775 min Scan# 11

Delta R.T. -0.000 min

Lab File: VD076477.D

Acq: 19 Jun 2023 18:45

Instrument :

MSVOA_D

ClientSampleId :

SB-03-4.0-6.0





Tgt Ion:114 Resp: 9147

Ion Ratio Lower Upper

114 100

63 25.8 0.0 33.4

88 16.7 0.0 26.2



#35

Dibromofluoromethane

Concen: 77.899 ug/l

RT: 7.810 min Scan# 1058

Delta R.T. 0.006 min

Lab File: VD076477.D

Acq: 19 Jun 2023 18:45




Tgt Ion:113 Resp: 4233


Ion Ratio Lower Upper

113 100

111 96.8 84.7 127.1

192 19.6 16.8 25.2





#36

1,1-Dichloropropene

Concen: 1.025 ug/l

RT: 7.893 min Scan# 1091

Delta R.T. -0.112 min

Lab File: VD076477.D


Acq: 19 Jun 2023 18:45

Instrument :




MSVOA_D

ClientSampleId :

SB-03-4.0-6.0



Tgt Ion:	75	Resp:	78
Ion	Ratio	Lower	Upper
75	100		
110	0.0	19.9	59.6#
77	0.0	24.7	37.1#

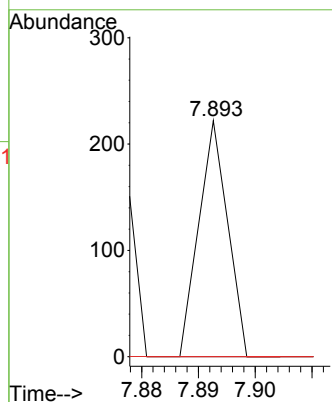

#37

Ethyl Acetate

Concen: 1.451 ug/l




RT: 7.199 min Scan# 954


Delta R.T. 0.029 min

Lab File: VD076477.D

Acq: 19 Jun 2023 18:45


Tgt Ion:	43	Resp:	64
Ion	Ratio	Lower	Upper
43	100		
61	0.0	14.9	22.3#
70	0.0	10.0	15.0#

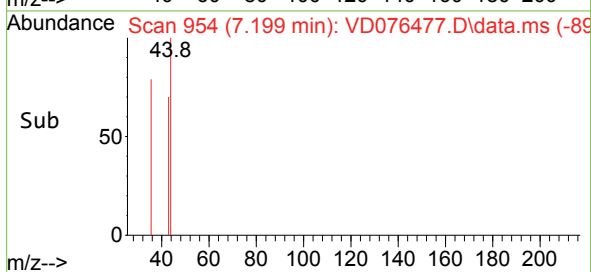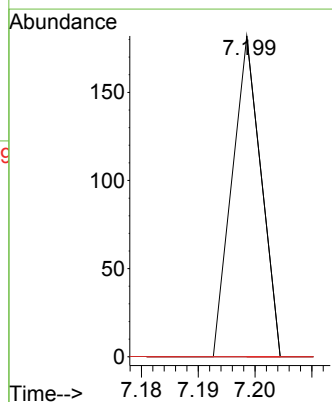






#38
Carbon Tetrachloride
Concen: 2.441 ug/l
RT: 7.887 min Scan# 1088
Delta R.T. -0.100 min
Lab File: VD076477.D
Acq: 19 Jun 2023 18:45

Instrument :
MSVOA_D
ClientSampleId :
SB-03-4.0-6.0







Tgt Ion:117 Resp: 166
Ion Ratio Lower Upper
117 100
119 0.0 78.0 117.0#
121 0.0 24.2 36.2#



#41
Methacrylonitrile
Concen: 2.209 ug/l
RT: 7.434 min Scan# 994
Delta R.T. 0.035 min
Lab File: VD076477.D
Acq: 19 Jun 2023 18:45


Tgt Ion: 41 Resp: 55
Ion Ratio Lower Upper
41 100
39 0.0 34.0 51.0#
67 0.0 77.0 115.4#
52 0.0 27.9 41.9#








#43
Isopropyl Acetate
Concen: 1.521 ug/l
RT: 8.351 min Scan# 1151
Delta R.T. -0.006 min
Lab File: VD076477.D
Acq: 19 Jun 2023 18:45

Instrument :
MSVOA_D
ClientSampleId :
SB-03-4.0-6.0







Tgt Ion: 43 Resp: 127
Ion Ratio Lower Upper
43 100
61 0.0 31.4 47.0#
87 0.0 14.9 22.3#

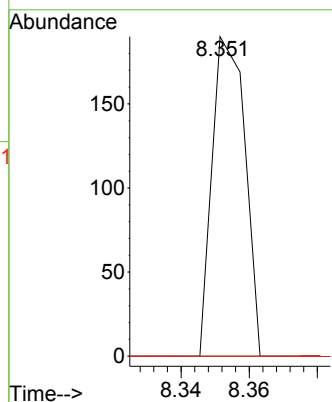

#48
Methyl methacrylate
Concen: 3.581 ug/l
RT: 9.381 min Scan# 1325
Delta R.T. -0.000 min
Lab File: VD076477.D
Acq: 19 Jun 2023 18:45

Tgt Ion: 41 Resp: 137
Ion Ratio Lower Upper
41 100
69 0.0 102.2 153.2#
39 131.4 41.4 62.2#



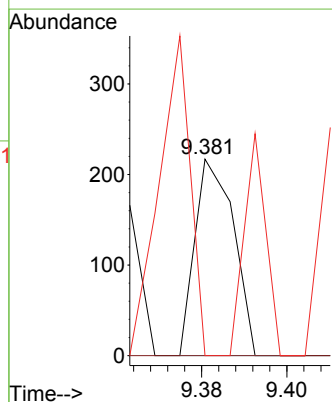
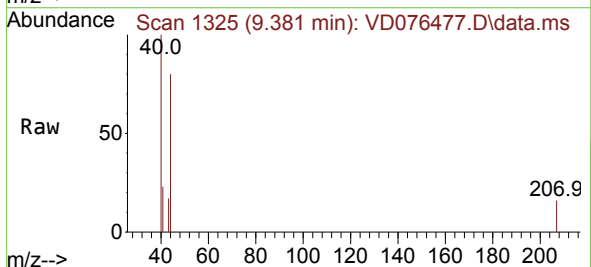




#50
Toluene-d8
Concen: 58.987 ug/l
RT: 10.269 min Scan# 1476
Delta R.T. -0.000 min
Lab File: VD076477.D
Acq: 19 Jun 2023 18:45




Instrument :
MSVOA_D
ClientSampleId :
SB-03-4.0-6.0


Tgt Ion: 98 Resp: 12156
Ion Ratio Lower Upper
98 100
100 60.7 50.3 75.5

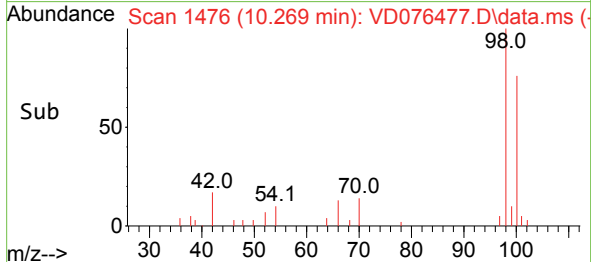

#51
4-Methyl-2-Pentanone
Concen: 2.226 ug/l
RT: 10.092 min Scan# 1446
Delta R.T. -0.065 min
Lab File: VD076477.D
Acq: 19 Jun 2023 18:45

Tgt Ion: 43 Resp: 95
Ion Ratio Lower Upper
43 100
58 0.0 38.9 58.3#


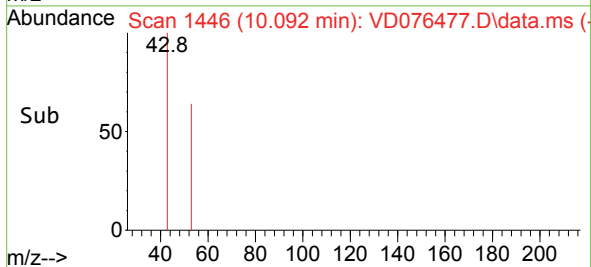

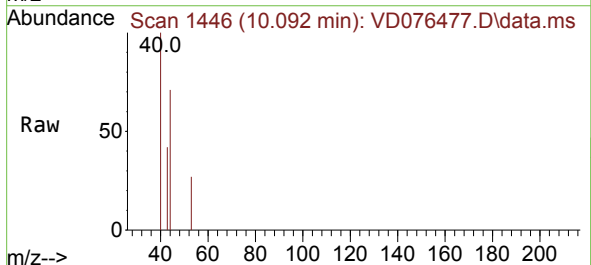




#59
2-Hexanone
Concen: 7.580 ug/l
RT: 10.934 min Scan# 11
Delta R.T. 0.012 min
Lab File: VD076477.D
Acq: 19 Jun 2023 18:45




Instrument :
MSVOA_D
ClientSampleId :
SB-03-4.0-6.0


Tgt Ion: 43 Resp: 225
Ion Ratio Lower Upper
43 100
58 0.0 34.1 102.2#

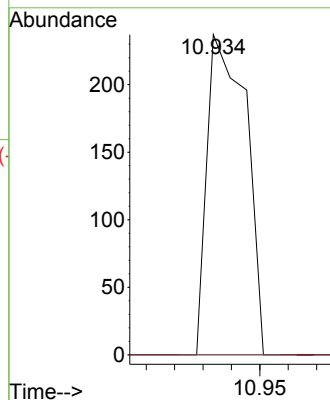

#62
4-Bromofluorobenzene
Concen: 59.059 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.000 min
Lab File: VD076477.D
Acq: 19 Jun 2023 18:45

Tgt Ion: 95 Resp: 3950
Ion Ratio Lower Upper
95 100
174 100.6 0.0 201.8
176 91.4 0.0 191.8



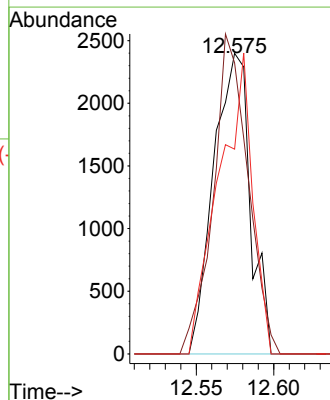
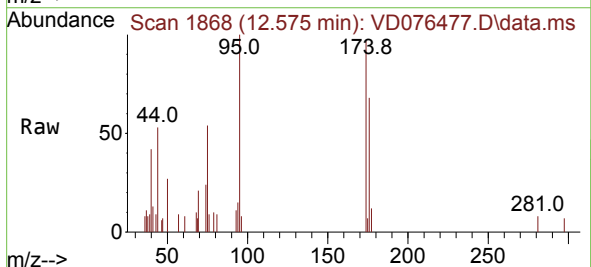




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.581 min Scan# 1699
Delta R.T. -0.000 min
Lab File: VD076477.D
Acq: 19 Jun 2023 18:45




Instrument :
MSVOA_D
ClientSampleId :
SB-03-4.0-6.0


Tgt Ion:117 Resp: 9445
Ion Ratio Lower Upper
117 100
82 53.7 38.3 57.5
119 36.7 25.0 37.4

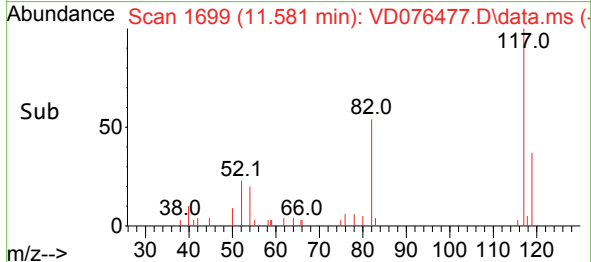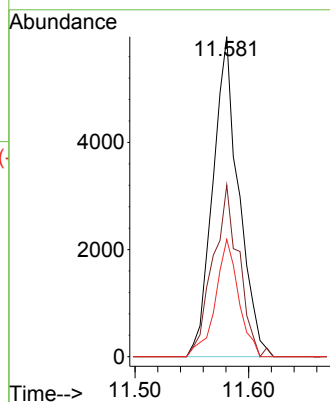

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.516 min Scan# 2028
Delta R.T. -0.000 min
Lab File: VD076477.D
Acq: 19 Jun 2023 18:45

Tgt Ion:152 Resp: 4391
Ion Ratio Lower Upper
152 100
115 55.0 27.1 81.3
150 159.3 0.0 353.6


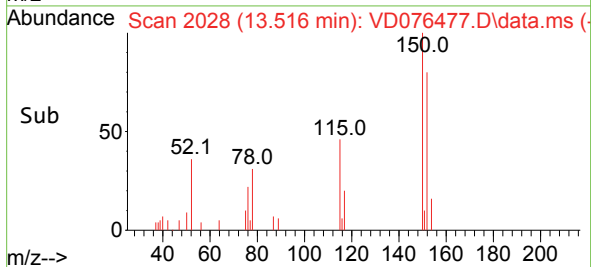
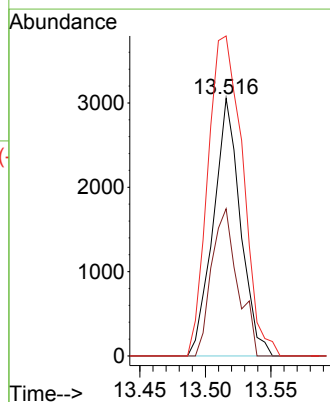
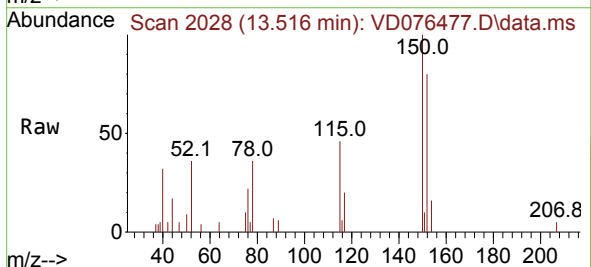




#76
1,2,3-Trichloropropane
Concen: 51.767 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. -0.147 min
Lab File: VD076477.D
Acq: 19 Jun 2023 18:45




Instrument :
MSVOA_D
ClientSampleId :
SB-03-4.0-6.0


Tgt Ion: 75 Resp: 2256
Ion Ratio Lower Upper
75 100
77 0.0 0.0 0.0



#81
trans-1,4-Dichloro-2-butene
Concen: 113.434 ug/l
RT: 12.575 min Scan# 1868
Delta R.T. 0.106 min
Lab File: VD076477.D
Acq: 19 Jun 2023 18:45

Tgt Ion: 75 Resp: 2256
Ion Ratio Lower Upper
75 100
53 0.0 63.0 94.4#
89 0.0 37.9 56.9#







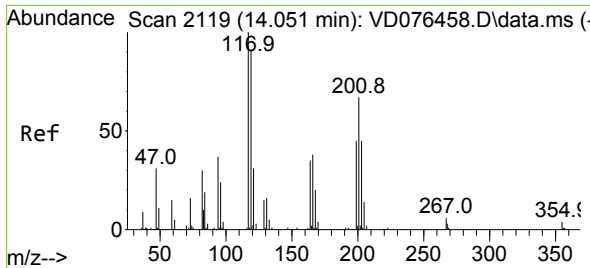

#90
Hexachloroethane
Concen: 1.161 ug/l
RT: 13.933 min Scan# 2099
Delta R.T. -0.118 min
Lab File: VD076477.D
Acq: 19 Jun 2023 18:45




Instrument :
MSVOA_D
ClientSampleId :
SB-03-4.0-6.0


Tgt Ion:117 Resp: 57
Ion Ratio Lower Upper
117 100
201 0.0 38.5 115.5#

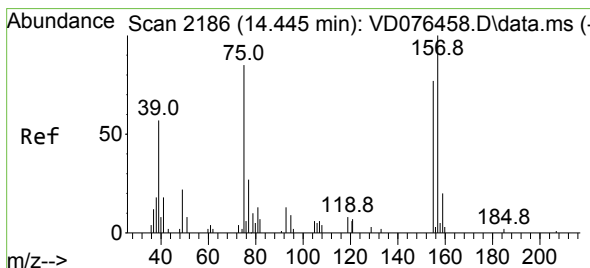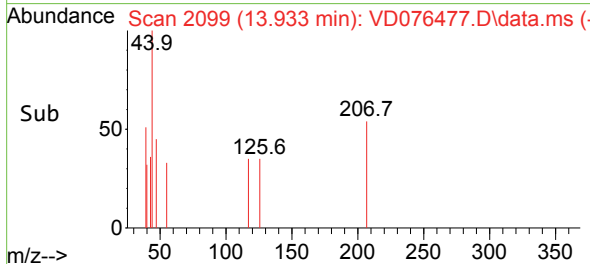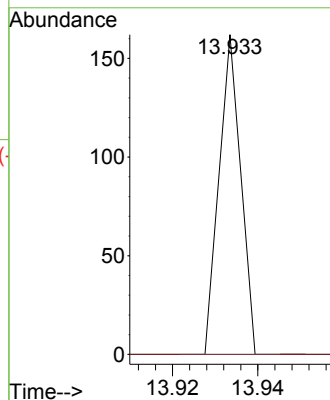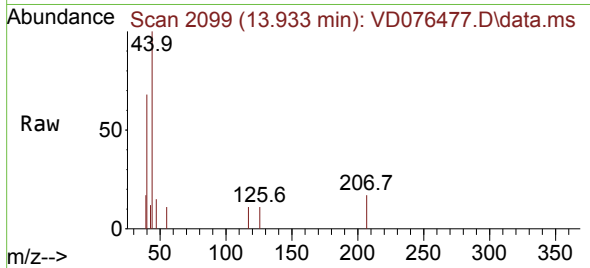

#92
1,2-Dibromo-3-Chloropropane
Concen: 12.088 ug/l
RT: 14.681 min Scan# 2226
Delta R.T. 0.235 min
Lab File: VD076477.D
Acq: 19 Jun 2023 18:45

Tgt Ion: 75 Resp: 111
Ion Ratio Lower Upper
75 100
155 0.0 47.9 143.8#
157 0.0 59.9 179.7#


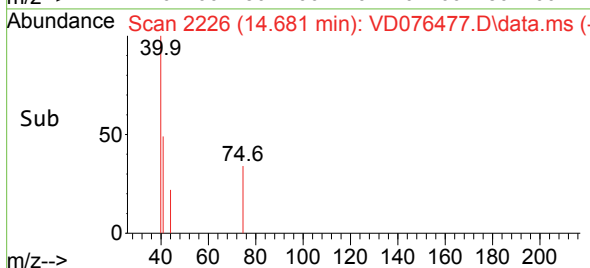
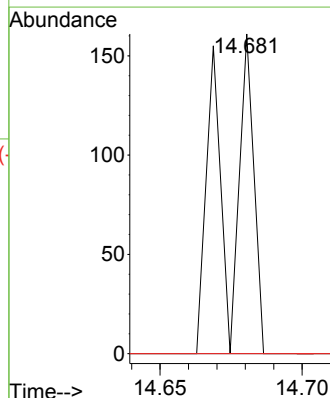
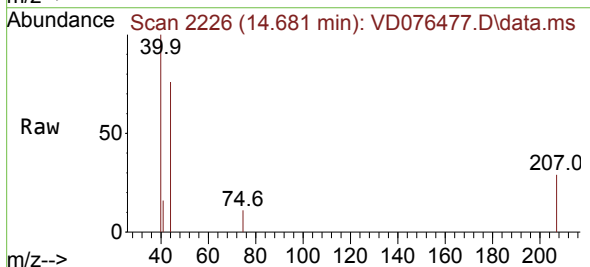




#94
Hexachlorobutadiene
Concen: 1.331 ug/l
RT: 15.457 min Scan# 21
Delta R.T. 0.253 min
Lab File: VD076477.D
Acq: 19 Jun 2023 18:45

Instrument :
MSVOA_D
ClientSampleId :
SB-03-4.0-6.0

Tgt Ion:225 Resp: 54
Ion Ratio Lower Upper
225 100
223 0.0 31.6 94.8#
227 0.0 31.7 95.1#

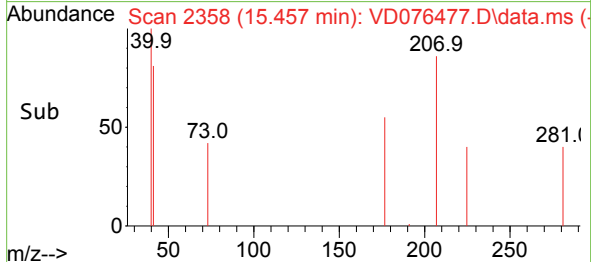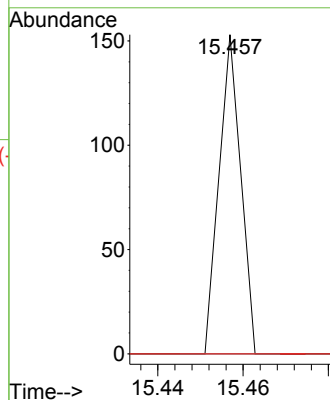

#95
Naphthalene
Concen: 2.679 ug/l
RT: 15.333 min Scan# 2337
Delta R.T. -0.000 min
Lab File: VD076477.D
Acq: 19 Jun 2023 18:45

Tgt Ion:128 Resp: 447
Ion Ratio Lower Upper
128 100
127 0.0 10.5 15.7#
129 0.0 8.7 13.1#

