
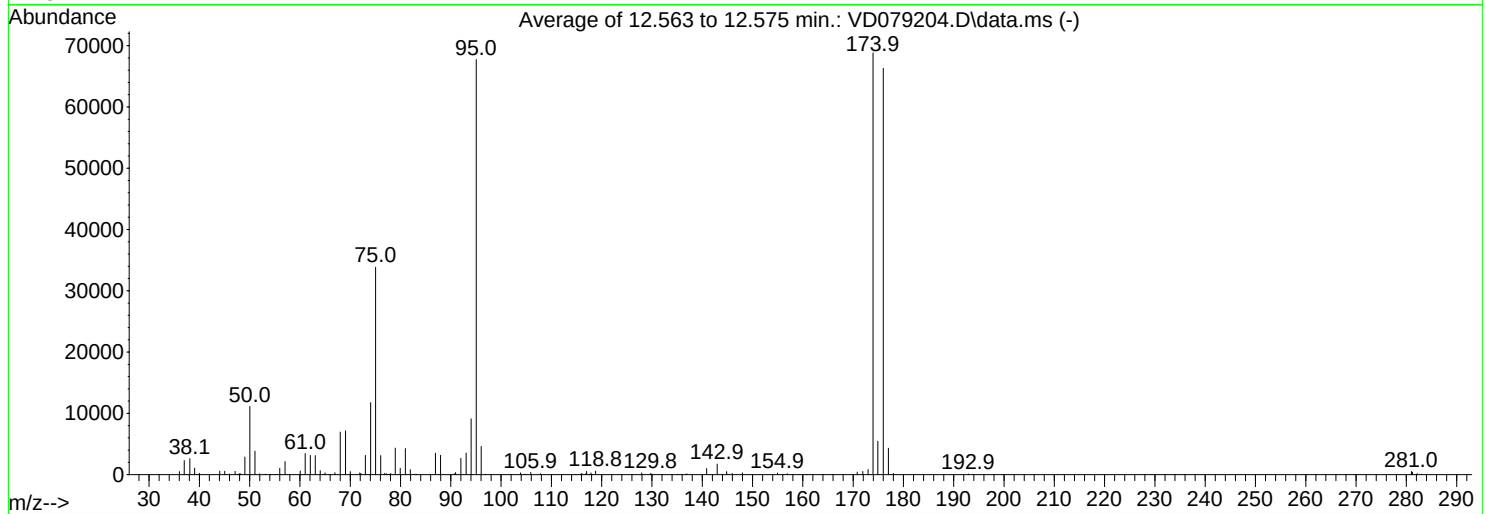


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD061924\
Data File : VD079204.D
Acq On : 19 Jun 2024 09:08
Operator : RP/MD
Sample : BFB811
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB811

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM052924SMA.M
Title : SFAM01.0
Last Update : Fri Jun 21 04:13:10 2024

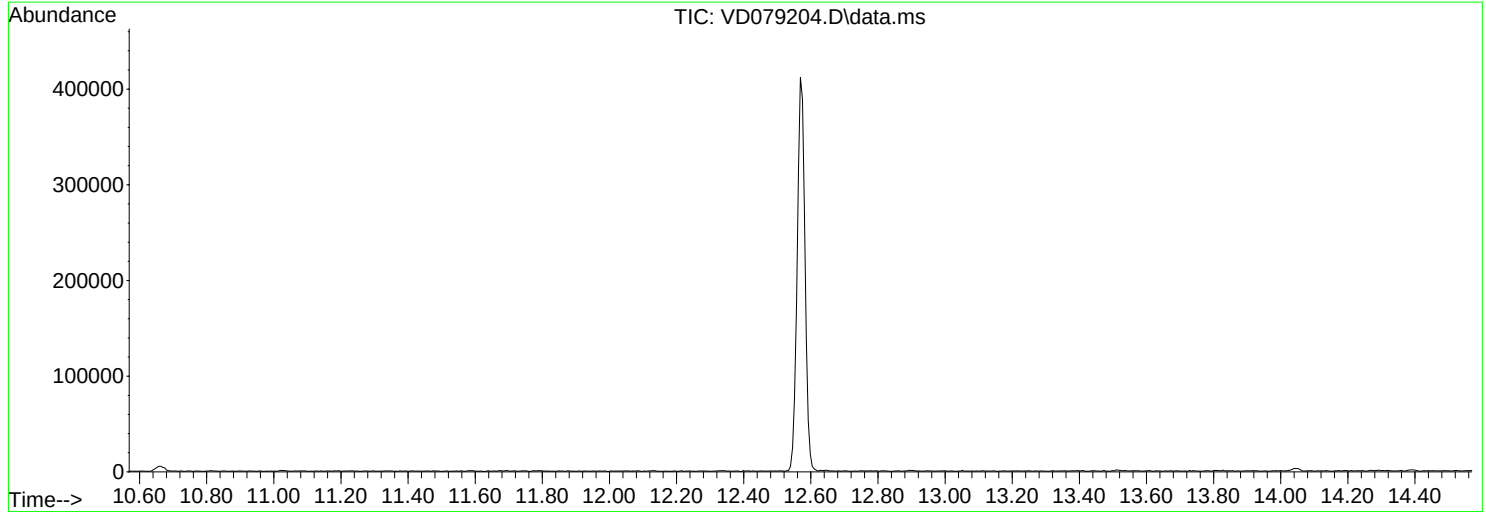

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1859

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	11131	PASS
75	95	30	80	50.0	33851	PASS
95	95	100	100	100.0	67723	PASS
96	95	5	9	6.8	4608	PASS
173	174	0.00	2	1.2	844	PASS
174	95	50	120	101.6	68827	PASS
175	174	5	9	7.9	5450	PASS
176	174	95	105	96.4	66317	PASS
177	176	5	10	6.5	4309	PASS

Scan 1859 (12.522 min): VD079204.D\data.ms
BFB811

m/z	Abundance
40.00	514.0
44.10	166.0

Instrument :
MSVOA_D
ClientSampleId :
BFB811

m/z	Abundance
36.00	519.0
37.00	1820.0
38.10	2589.0
39.00	701.0
39.90	813.0
44.00	722.0
45.00	603.0
47.20	563.0
48.00	215.0
49.00	2749.0
50.10	9131.0
51.00	3559.0
52.00	247.0
55.90	961.0
57.00	1795.0
60.10	445.0
61.10	2873.0
62.00	2584.0
63.00	2685.0
64.00	334.0
65.00	265.0
67.00	388.0
68.00	5905.0
69.00	6120.0
70.00	378.0
71.90	321.0
73.00	2780.0
74.00	10493.0
75.00	29888.0
76.10	2295.0
77.00	402.0
77.90	271.0
78.90	3699.0
79.90	964.0
80.90	4074.0
81.90	675.0
85.90	250.0
86.90	3033.0
88.00	2779.0
90.70	452.0
92.00	2584.0
93.10	3141.0
94.00	8064.0
95.00	59552.0
96.10	4464.0
103.90	206.0
105.80	215.0
107.90	219.0
115.80	281.0
116.80	419.0
117.60	178.0
118.10	172.0
118.80	571.0
129.70	185.0
137.00	208.0
140.90	1056.0
142.90	1319.0
145.10	270.0
146.00	156.0
148.00	328.0
155.00	201.0
170.70	356.0
171.80	624.0
173.00	531.0
173.90	55464.0
174.90	4713.0
176.00	53016.0
177.00	3750.0
178.00	223.0
281.00	487.0

Instrument :
MSVOA_D
ClientSampleId :
BFB811

m/z	Abundance
36.10	424.0
37.00	2743.0
38.10	2509.0
39.00	1139.0
40.00	522.0
44.10	793.0
45.10	588.0
45.90	160.0
47.10	521.0
47.90	367.0
49.00	2842.0
50.10	13309.0
51.10	3990.0
51.90	174.0
53.10	208.0
54.10	189.0
55.20	180.0
56.00	1173.0
57.00	2206.0
57.90	200.0
60.00	564.0
61.10	3809.0
62.10	3658.0
63.10	3504.0
64.00	1037.0
65.00	254.0
67.00	400.0
68.00	7680.0
69.00	8170.0
70.00	550.0
72.10	659.0
73.00	3463.0
74.00	13158.0
75.10	37536.0
76.10	3742.0
76.80	330.0
77.60	237.0
78.10	296.0
79.00	4877.0
80.00	1095.0
80.90	4824.0
82.00	986.0
83.20	175.0
87.00	3415.0
87.90	3513.0
91.00	470.0
92.00	3172.0
93.00	3843.0
94.00	9290.0
95.10	73096.0
96.00	4917.0
96.90	257.0
103.80	304.0
105.90	482.0
107.80	272.0
114.90	151.0
116.00	347.0
117.00	731.0
117.80	479.0
118.90	654.0
128.10	311.0
129.70	231.0
130.00	273.0
136.70	170.0
140.80	904.0
142.90	2176.0
144.80	696.0
145.90	187.0
147.90	285.0
154.80	331.0
156.90	208.0
170.80	439.0
171.90	462.0
173.00	834.0
174.00	77256.0
174.90	5988.0
176.00	74344.0
177.00	4566.0
178.00	260.0
192.90	165.0
281.00	1078.0
282.10	159.0
283.00	217.0

Instrument :
MSVOA_D
ClientSampleId :
BFB811

m/z	Abundance
36.00	511.0
37.00	2371.0
38.10	2774.0
39.10	1408.0
40.10	830.0
44.00	737.0
45.00	452.0
46.00	192.0
47.00	486.0
47.60	192.0
48.20	418.0
49.10	3025.0
50.00	10954.0
51.00	3934.0
56.10	1017.0
57.10	2443.0
60.00	825.0
61.00	3676.0
62.00	3129.0
63.10	3124.0
64.10	611.0
65.00	361.0
66.80	189.0
68.00	7229.0
69.10	7145.0
70.00	597.0
71.90	565.0
73.00	3174.0
74.10	11620.0
75.00	34128.0
76.00	3292.0
77.20	388.0
78.00	245.0
79.00	4414.0
79.90	995.0
81.00	3893.0
82.00	795.0
82.90	203.0
87.00	4061.0
88.00	3197.0
90.90	538.0
92.00	2258.0
93.00	3600.0
94.10	9949.0
95.00	70520.0
96.10	4443.0
103.90	375.0
104.80	261.0
106.00	387.0
116.10	312.0
117.00	869.0
117.90	420.0
118.70	488.0
127.90	575.0
129.80	254.0
135.10	198.0
136.90	173.0
140.90	993.0
143.00	1658.0
144.90	778.0
145.90	251.0
148.00	250.0
155.00	223.0
156.90	248.0
160.80	158.0
170.90	472.0
172.00	491.0
172.90	1168.0
174.00	73760.0
174.90	5648.0
176.00	71592.0
177.00	4611.0
178.00	184.0
192.90	184.0
281.20	1147.0
282.20	341.0

Instrument :
MSVOA_D
ClientSampleId :
BFB811