




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062024\
Data File : VD079215.D
Acq On : 20 Jun 2024 13:15
Operator : RP/MD
Sample : P2897-20
Misc : 5.07G/10ml/MSVOA_D/SOIL/A
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C0T68

Manual IntegrationsAPPROVED

Quant Time: Jun 21 04:14:20 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM052924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 21 04:13:10 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/24/2024
Supervised By :Semsettin Yesilyurt 06/24/2024

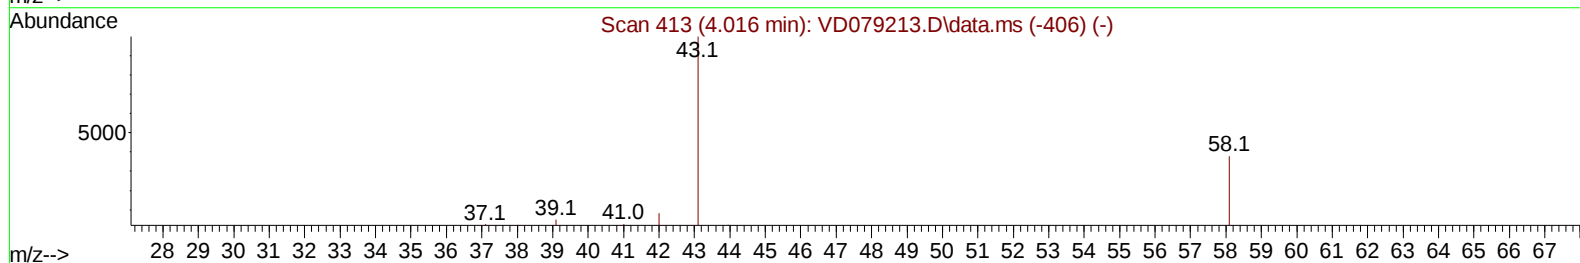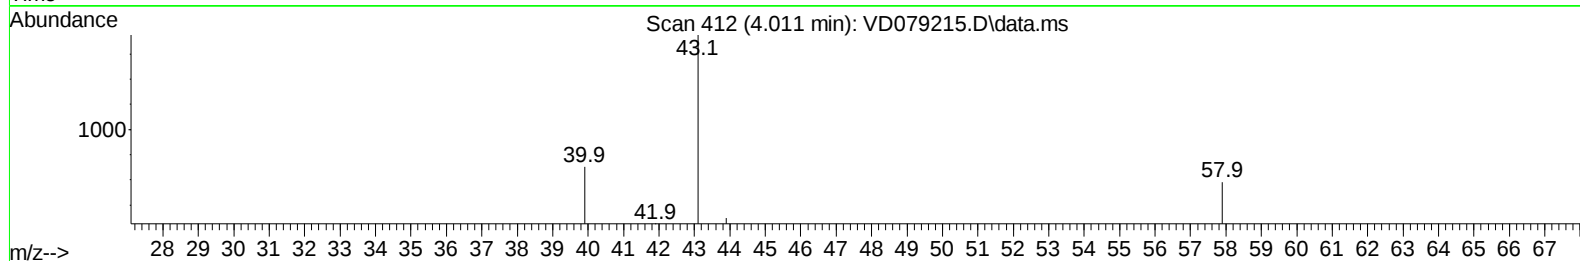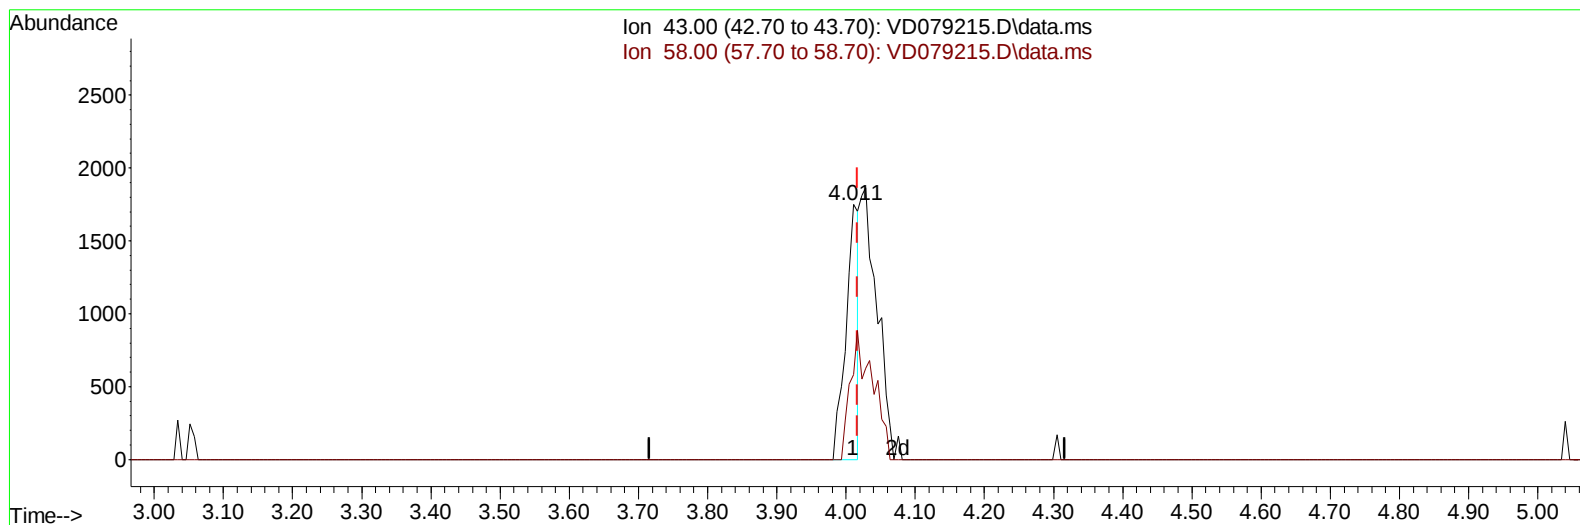

TIC: VD079215.D\data.ms

(13) Acetone (T)

4.011min (-0.006) 2.41 ug/L

response 2221

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	39.10	44.57
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062024\
Data File : VD079215.D
Acq On : 20 Jun 2024 13:15
Operator : RP/MD
Sample : P2897-20
Misc : 5.07G/10ml/MSVOA_D/SOIL/A
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C0T68

Manual IntegrationsAPPROVED

Quant Time: Jun 21 04:14:20 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM052924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 21 04:13:10 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 06/24/2024
Supervised By :Semsettin Yesilyurt 06/24/2024

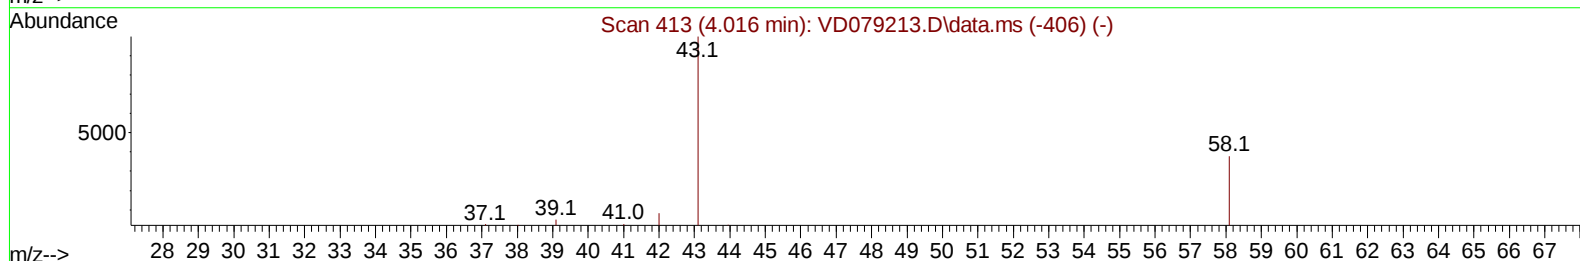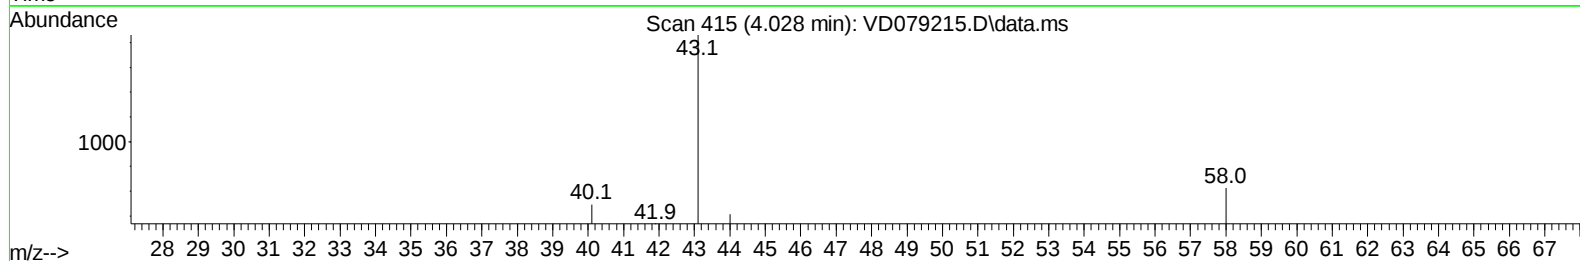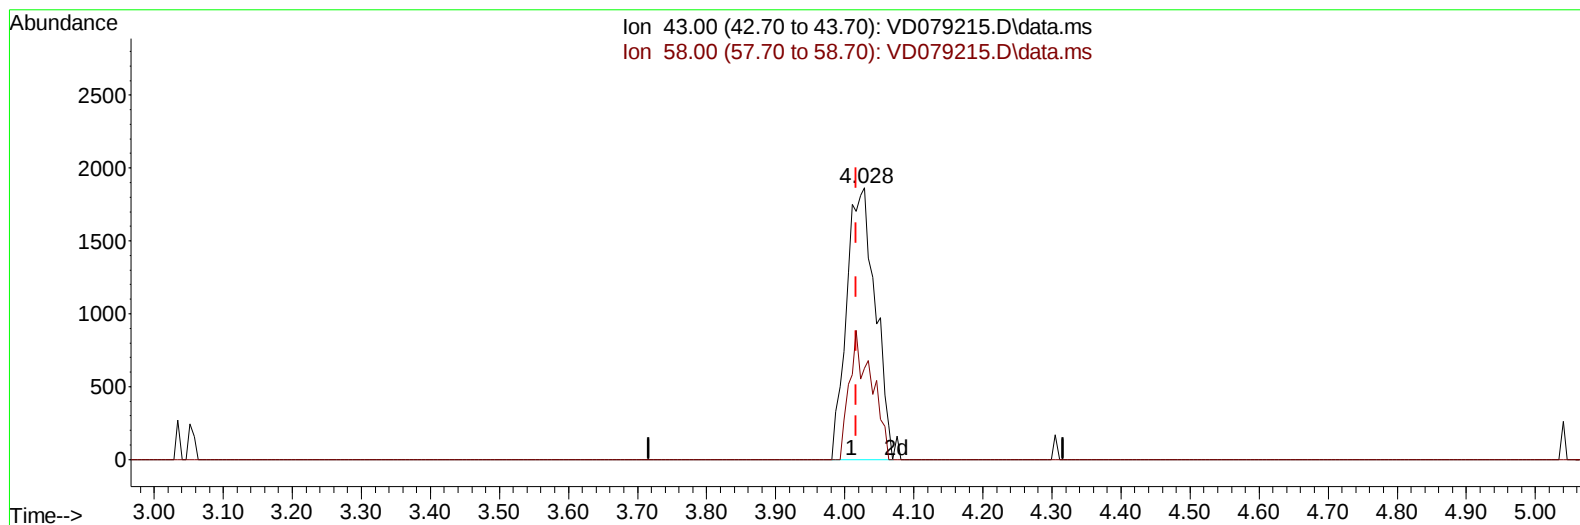

TIC: VD079215.D\data.ms

(13) Acetone (T)

4.028min (+ 0.012) 5.82 ug/L m

response 5358

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	39.10	18.48
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062024\
 Data File : VD079215.D
 Acq On : 20 Jun 2024 13:15
 Operator : RP/MD
 Sample : P2897-20
 Misc : 5.07G/10ml/MSVOA_D/SOIL/A
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 C0T68

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 06/24/2024
 Supervised By :Semsettin Yesilyurt 06/24/2024

Quant Time: Jun 21 04:14:20 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM052924SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Jun 21 04:13:10 2024
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.775	114		270298	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.581	117		273983	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.516	152		116918	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.276	65		111751	13.435	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	53.760%		
7) Chloroethane-d5	2.799	69		110907	13.790	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	55.160%		
11) 1,1-Dichloroethene-d2	3.917	65		20274	13.730	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	54.920%		
21) 2-Butanone-d5	6.987	46		27347	42.984	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	85.960%		
24) Chloroform-d	7.563	84		117712	15.575	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	62.320%		
26) 1,2-Dichloroethane-d4	8.222	65		62710	17.987	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	71.960%		
32) Benzene-d6	8.199	84		237869	15.661	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	62.640%		
36) 1,2-Dichloropropane-d6	9.205	67		74221	16.964	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	67.840%#		
41) Toluene-d8	10.263	98		213091	14.984	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	59.920%		
43) trans-1,3-Dichloroprop...	10.522	79		32077	17.443	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	69.760%		
47) 2-Hexanone-d5	10.875	63		24291	42.947	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	85.900%		
56) 1,1,2,2-Tetrachloroeth...	12.646	84		75440	19.467	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	77.880%		
66) 1,2-Dichlorobenzene-d4	13.810	152		78039	19.340	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	77.360%		
Target Compounds							
13) Acetone	4.028	43		5358m	5.817	ug/L	
16) Methylene chloride	4.799	84		22187	4.607	ug/L	90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062024\
Data File : VD079215.D
Acq On : 20 Jun 2024 13:15
Operator : RP/MD
Sample : P2897-20
Misc : 5.07G/10ml/MSVOA_D/SOIL/A
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
C0T68

Manual IntegrationsAPPROVED

Reviewed By :Mahesh Dadoda 06/24/2024
Supervised By :Semsettin Yesilyurt 06/24/2024

Quant Time: Jun 21 04:14:20 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM052924SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Jun 21 04:13:10 2024
Response via : Initial Calibration

