


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062024\
Data File : VD079212.D
Acq On : 20 Jun 2024 10:20
Operator : RP/MD
Sample : BFB812
Misc : 5.00G/10ml/MSVOA_D/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_D
ClientSampleId :
BFB812

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\SFAMDLM052924SMA.M
Title : SFAM01.0
Last Update : Fri Jun 21 04:13:10 2024

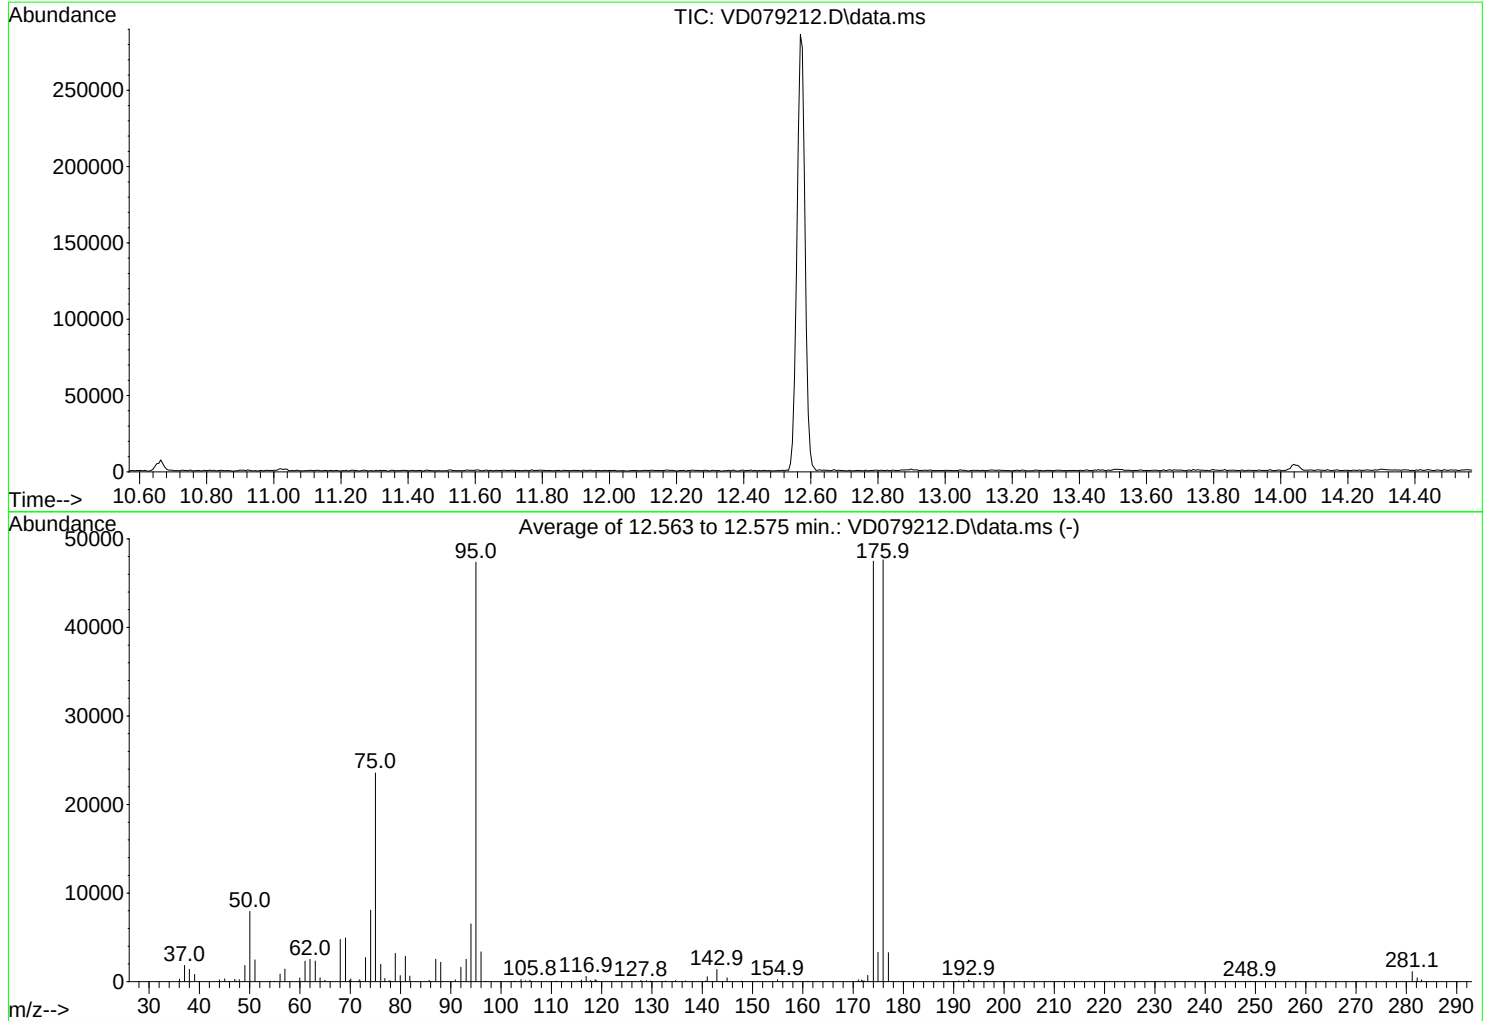

AutoFind: Scans 1866, 1867, 1868; Background Corrected with Scan 1860

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.7	7928	PASS
75	95	30	80	49.7	23557	PASS
95	95	100	100	100.0	47368	PASS
96	95	5	9	7.1	3357	PASS
173	174	0.00	2	1.5	705	PASS
174	95	50	120	100.3	47488	PASS
175	174	5	9	6.9	3300	PASS
176	174	95	105	100.3	47629	PASS
177	176	5	10	6.9	3270	PASS

Scan 1860 (12.528 min): VD079212.D\data.ms
BFB812

m/z	Abundance
39.90	685.0
44.10	354.0
207.10	207.0

Instrument :
MSVOA_D
ClientSampleId :
BFB812

m/z	Abundance
36.10	263.0
37.00	1617.0
38.00	1347.0
39.10	818.0
40.00	753.0
44.00	685.0
45.00	226.0
47.00	189.0
47.90	304.0
49.10	1565.0
50.00	7450.0
51.10	1813.0
56.10	817.0
57.00	1322.0
59.90	235.0
61.00	1976.0
62.00	2216.0
63.00	2353.0
64.10	412.0
68.00	3942.0
69.10	4475.0
69.90	467.0
72.00	163.0
73.00	2339.0
74.10	6231.0
75.00	19968.0
76.00	1793.0
76.80	452.0
78.00	200.0
78.90	3386.0
79.90	594.0
80.90	2560.0
81.90	469.0
85.70	200.0
87.00	2048.0
88.00	1722.0
90.90	300.0
92.00	1167.0
93.00	2175.0
94.00	5716.0
95.00	39192.0
96.00	2899.0
103.90	437.0
115.70	171.0
116.90	638.0
118.70	258.0
128.90	185.0
140.70	268.0
141.10	245.0
142.90	701.0
145.00	472.0
155.00	196.0
171.70	209.0
172.90	638.0
174.00	39576.0
175.00	2191.0
176.00	39616.0
177.00	2814.0
192.90	203.0
207.00	267.0
281.10	875.0
282.20	236.0
283.00	255.0

Instrument :
MSVOA_D
ClientSampleId :
BFB812

m/z	Abundance
36.00	376.0
37.10	1977.0
38.00	1478.0
39.00	738.0
40.00	725.0
44.00	615.0
45.10	274.0
47.10	354.0
48.00	380.0
49.00	2090.0
50.00	7990.0
51.00	2867.0
54.10	171.0
54.90	182.0
55.90	1072.0
57.00	1611.0
59.90	420.0
61.00	2636.0
62.00	2408.0
63.00	2689.0
63.90	230.0
64.90	348.0
68.00	5569.0
69.00	5297.0
70.10	526.0
71.60	202.0
72.00	200.0
73.00	3046.0
74.00	8952.0
75.00	24640.0
76.00	2310.0
76.90	356.0
77.70	172.0
79.00	3478.0
79.90	841.0
81.00	2948.0
81.80	626.0
85.70	228.0
87.00	2580.0
88.00	2238.0
90.90	159.0
92.00	2318.0
93.00	2887.0
94.00	7031.0
95.00	52688.0
96.00	3707.0
97.00	159.0
104.00	292.0
104.90	172.0
105.80	202.0
111.00	159.0
116.00	360.0
116.90	716.0
117.80	457.0
118.70	434.0
127.80	212.0
128.90	197.0
134.70	214.0
141.10	595.0
142.90	2131.0
144.90	432.0
154.90	241.0
171.20	254.0
171.90	355.0
172.80	757.0
174.00	50696.0
174.90	4027.0
176.00	53184.0
177.00	3526.0
193.20	245.0
206.80	203.0
248.90	151.0
281.10	967.0
282.10	485.0

Instrument :
MSVOA_D
ClientSampleId :
BFB812

m/z	Abundance
36.00	218.0
37.00	1906.0
38.00	1346.0
39.00	893.0
40.10	610.0
44.10	387.0
45.00	482.0
47.00	254.0
47.40	229.0
49.00	1849.0
50.10	8343.0
51.00	2672.0
56.10	663.0
57.00	1377.0
60.00	609.0
61.00	2312.0
62.00	2907.0
63.10	1957.0
64.00	657.0
65.00	159.0
68.00	4827.0
69.00	5005.0
70.10	377.0
71.80	308.0
73.10	2765.0
74.00	9016.0
75.00	26064.0
76.10	1746.0
77.00	267.0
77.80	164.0
79.00	2739.0
80.00	653.0
81.00	3109.0
81.80	776.0
87.00	2955.0
88.00	2617.0
91.00	152.0
92.00	1388.0
93.10	2523.0
94.00	6827.0
95.00	50224.0
96.00	3464.0
102.70	177.0
104.80	163.0
105.70	294.0
115.90	211.0
116.80	438.0
118.90	500.0
127.80	218.0
129.70	223.0
132.70	237.0
134.60	154.0
136.70	257.0
140.90	868.0
142.90	1300.0
144.90	417.0
147.80	178.0
154.90	203.0
161.00	153.0
171.00	347.0
171.70	328.0
172.20	225.0
173.00	721.0
174.00	52192.0
175.00	3681.0
175.90	50088.0
177.00	3469.0
191.00	249.0
193.00	333.0
281.20	1576.0
282.10	573.0
283.00	369.0

Instrument :
MSVOA_D
ClientSampleId :
BFB812