
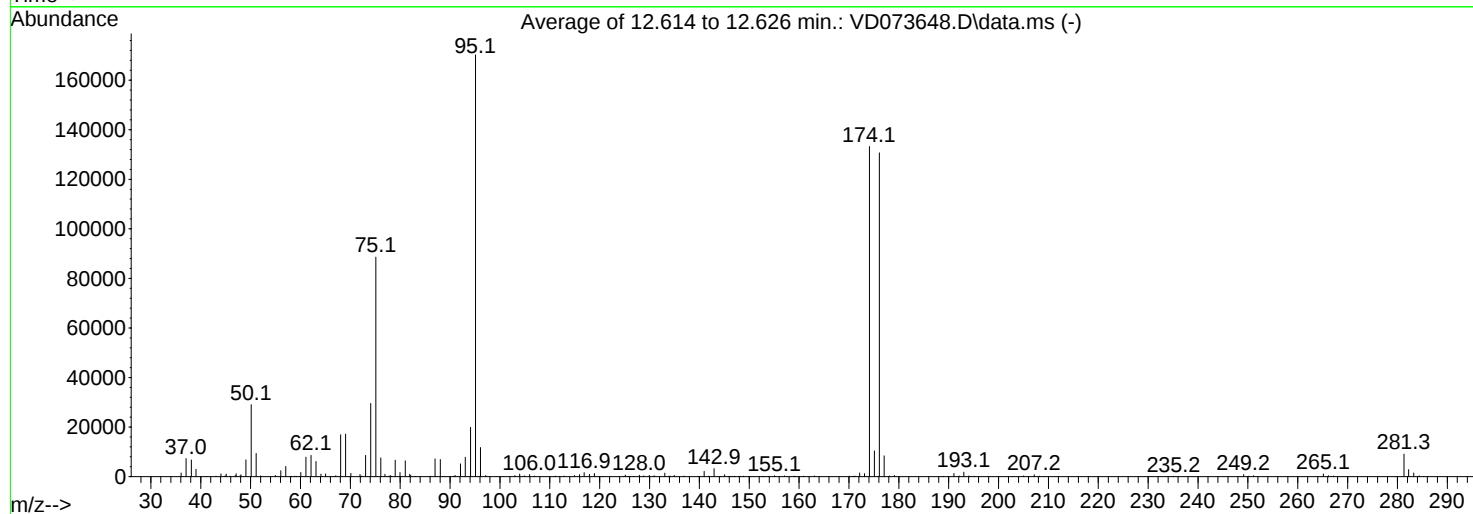


Data Path : Z:\voasrv\HPCHEM1\MSVOA_D\Data\VD062222\
 Data File : VD073648.D
 Acq On : 22 Jun 2022 08:48
 Operator : VA/SY
 Sample : BFB
 Misc : 5.00G/5.00ml/MSVOA_D/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_D
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_D\Method\82D062022S.M
 Title : SW846 8260
 Last Update : Tue Jun 21 05:24:45 2022

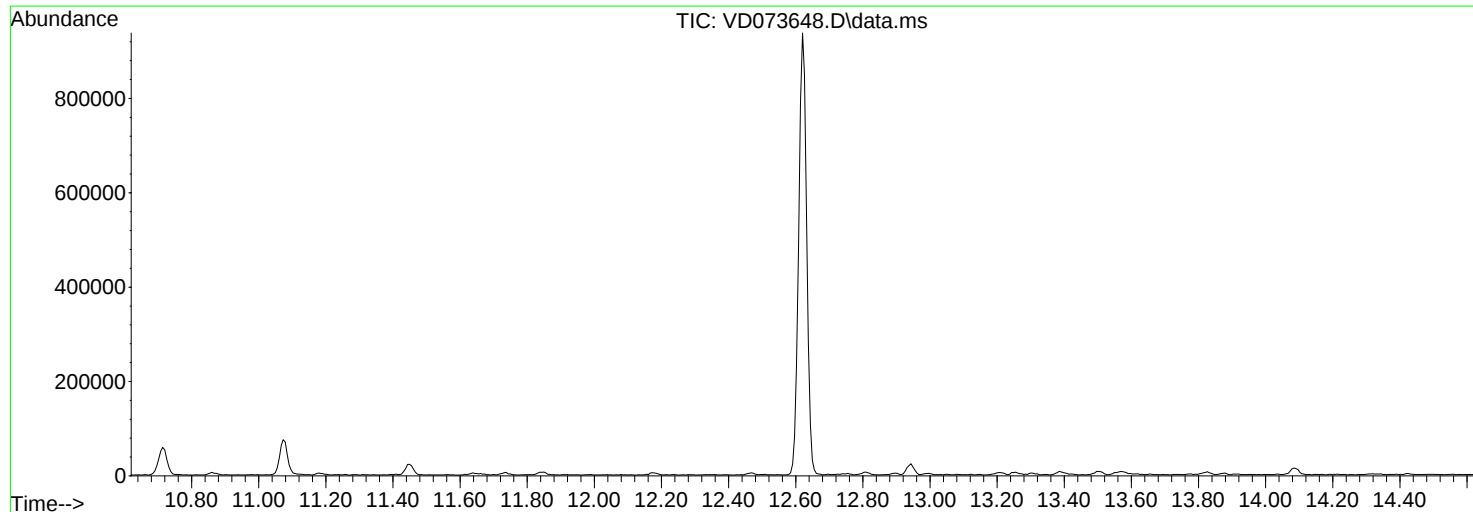

AutoFind: Scans 1818, 1819, 1820; Background Corrected with Scan 1809

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	29085	PASS
75	95	30	60	52.1	88600	PASS
95	95	100	100	100.0	170219	PASS
96	95	5	9	6.9	11739	PASS
173	174	0.00	2	0.9	1230	PASS
174	95	50	100	78.3	133240	PASS
175	174	5	9	7.8	10369	PASS
176	174	95	101	98.1	130701	PASS
177	176	5	9	6.4	8414	PASS